

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW013020\
Quantitation Report (QT Reviewed)


Data File : VW014808.D
Acq On : 30 Jan 2020 13:03
Operator : SY/VA
Sample : L1303-09
Misc : 3.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 01:18:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
C0AF4

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:22:24 PM

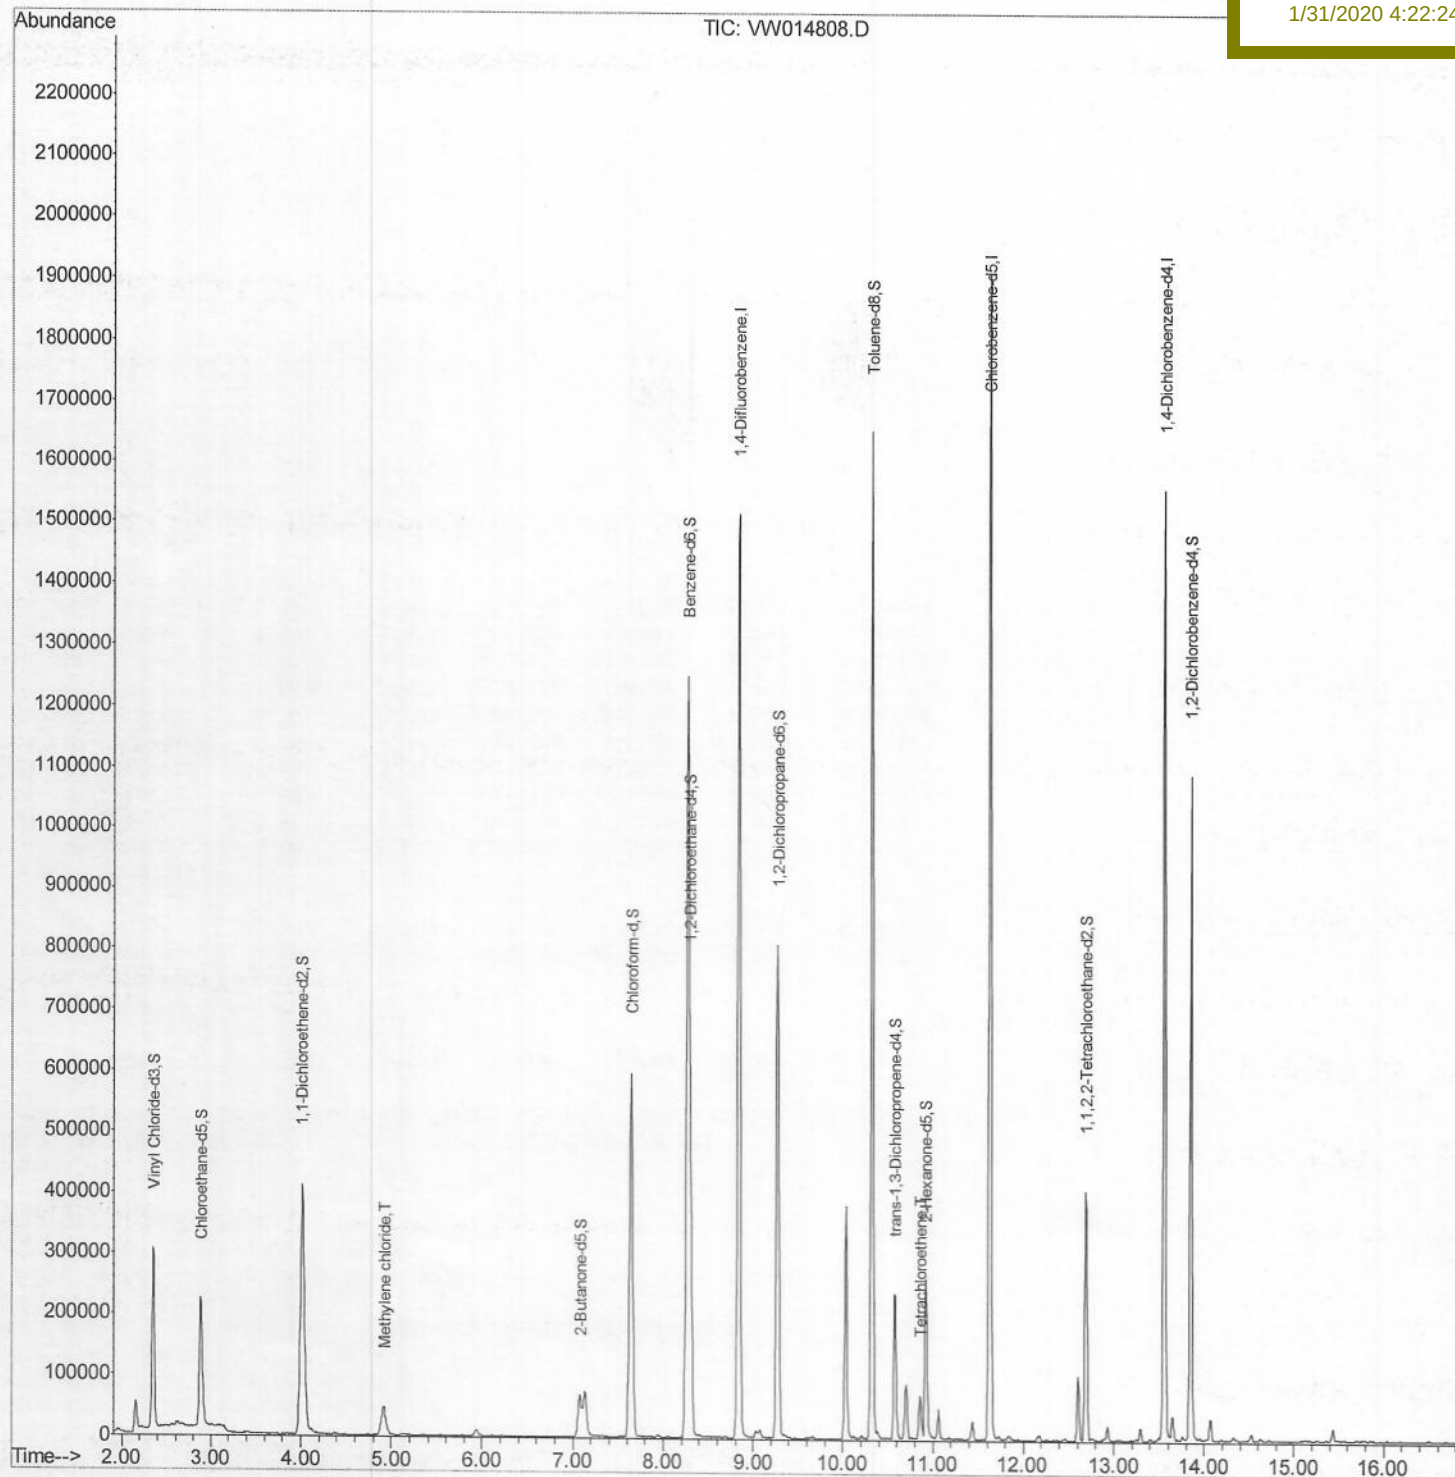

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW013020\
Quantitation Report (Qedit)




Data File : VW014808.D
Acq On : 30 Jan 2020 13:03
Operator : SY/VA
Sample : L1303-09
Misc : 3.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 01:11:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sample Id :
C0AF4

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:22:24 PM

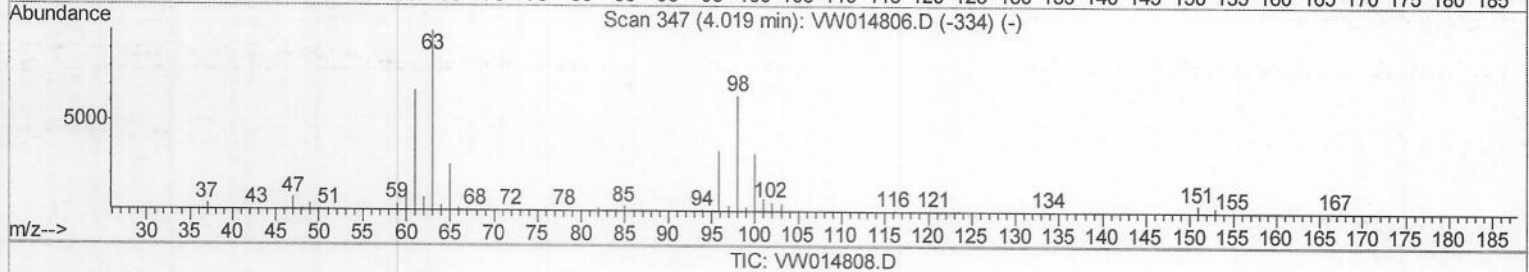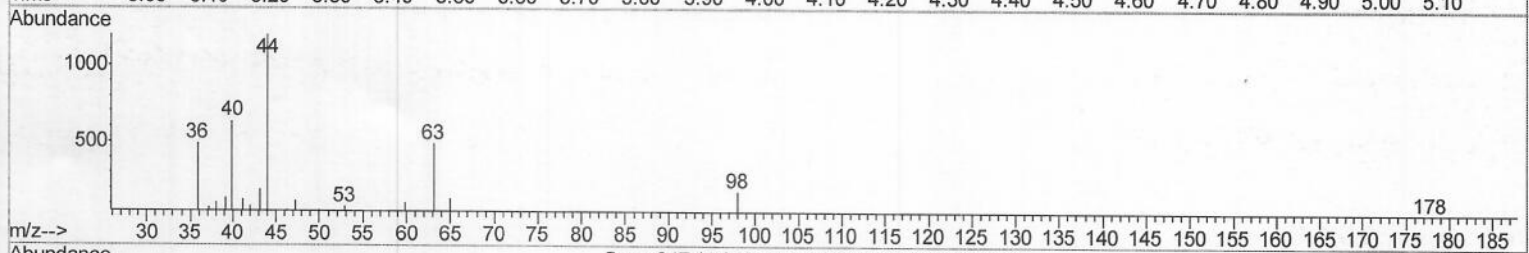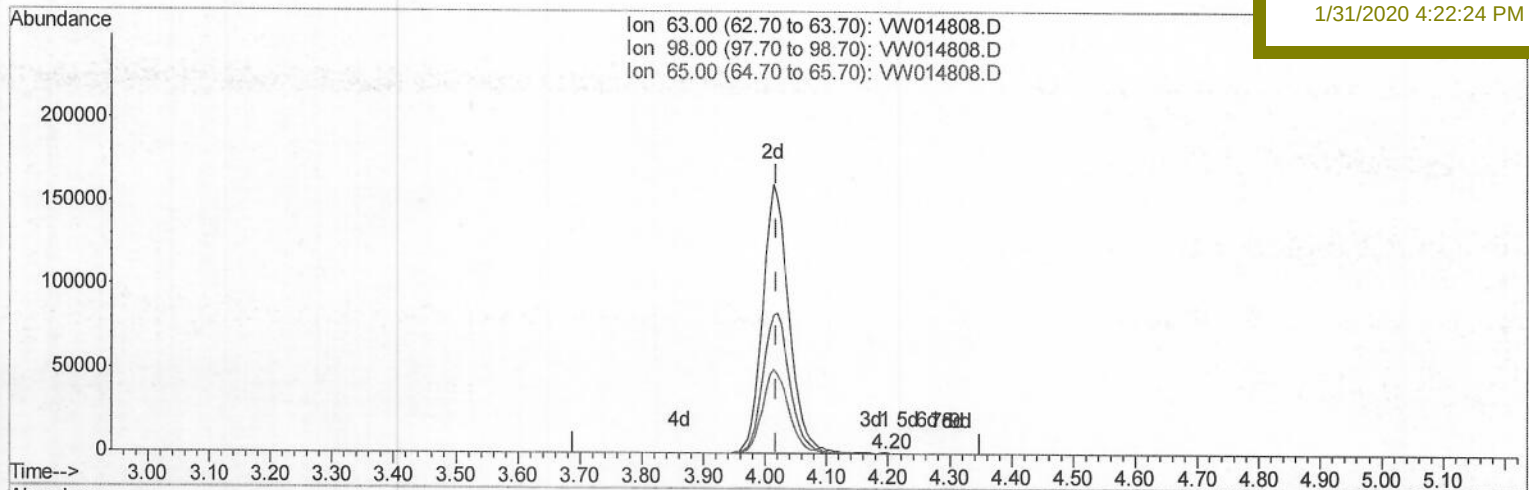

(10) 1,1-Dichloroethene-d2 (S)

4.196min (+0.177) 0.02ug/L

response 515

Ion	Exp%	Act%
63.00	100	100
98.00	70.70	49.90
65.00	23.70	17.09
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW013020\
Quantitation Report (Qedit)




Data File : VW014808.D
Acq On : 30 Jan 2020 13:03
Operator : SY/VA
Sample : L1303-09
Misc : 3.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 01:11:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
C0AF4

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:22:24 PM

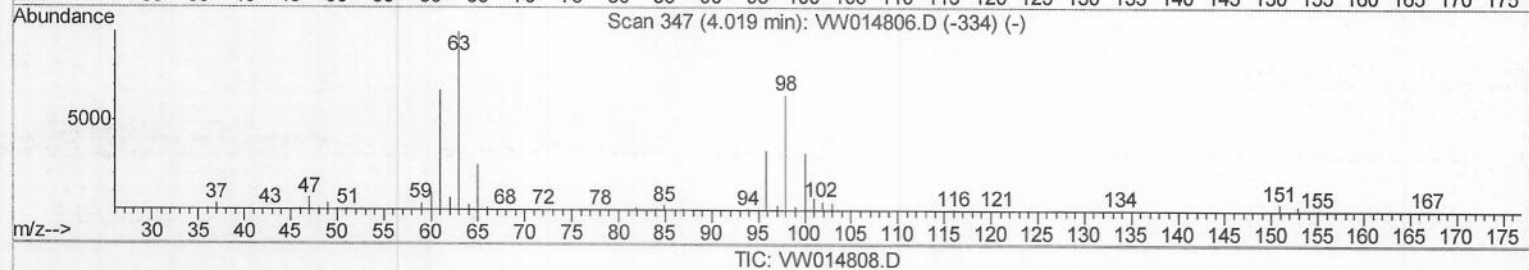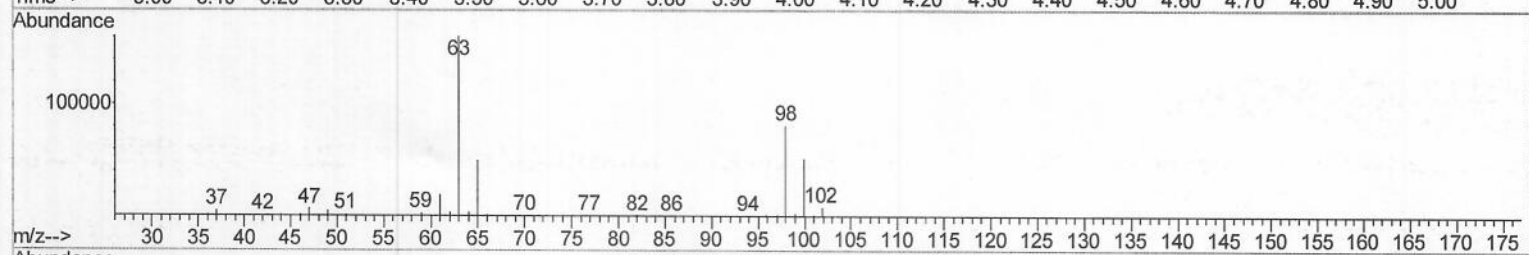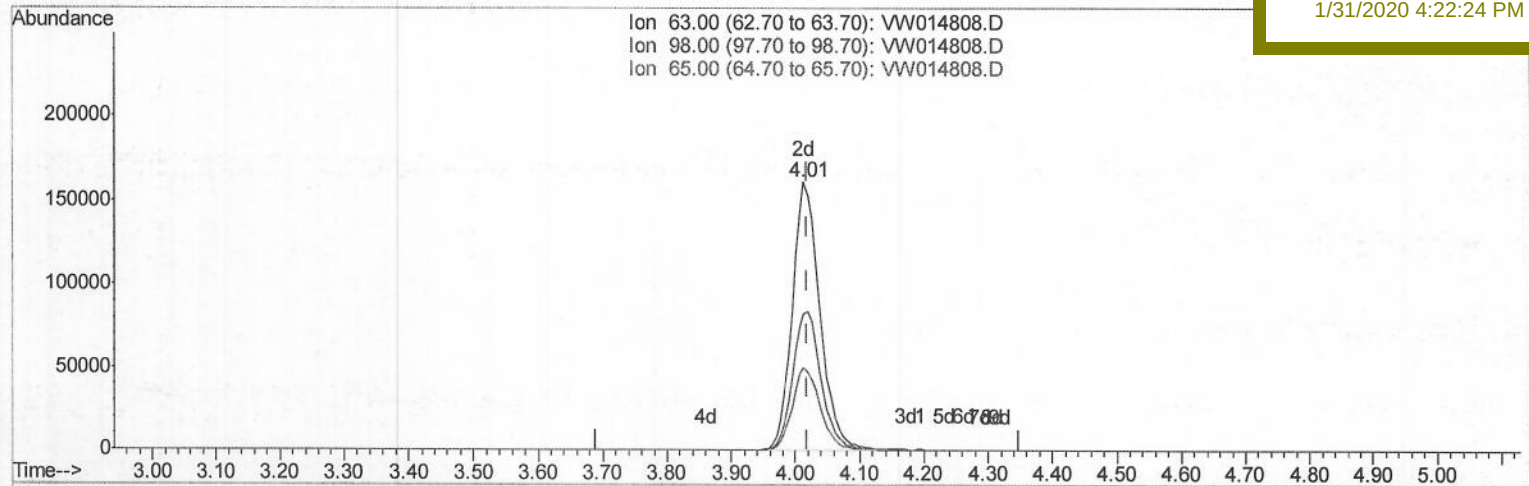

(10) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 14.22ug/L m

response 481729

Ion	Exp%	Act%
63.00	100	100
98.00	70.70	0.05#
65.00	23.70	0.02#
0.00	0.00	0.00

02/04/20 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW013020\
Quantitation Report (Qedit)




Data File : VW014808.D
Acq On : 30 Jan 2020 13:03
Operator : SY/VA
Sample : L1303-09
Misc : 3.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 01:11:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
C0AF4

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:22:24 PM

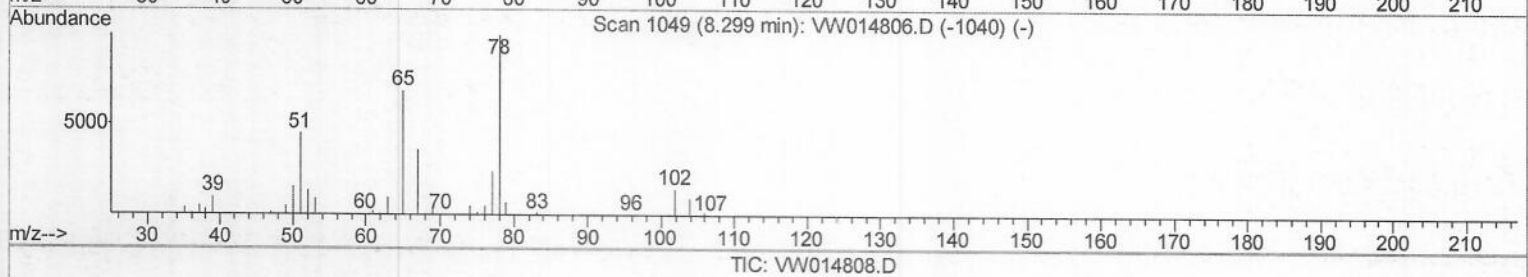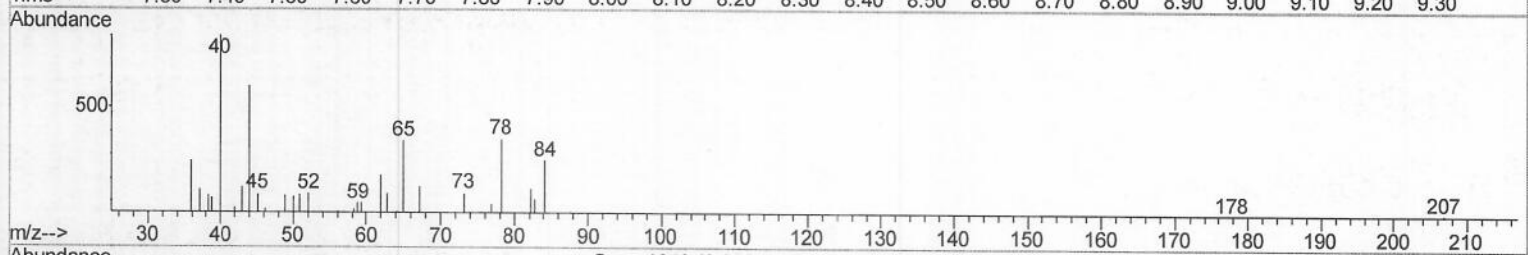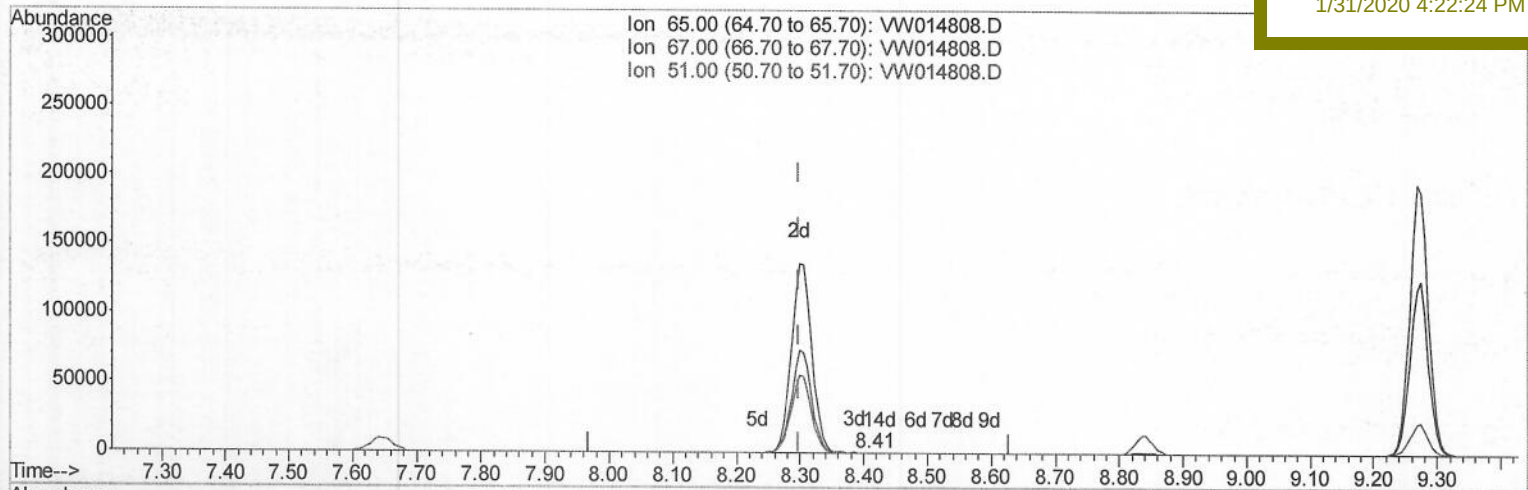

(26) 1,2-Dichloroethane-d4 (S)

8.409min (+0.110) 0.01ug/L

response 232

Ion	Exp%	Act%
65.00	100	100
67.00	53.40	54.74
51.00	102.70	90.52
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW013020\
Quantitation Report (Qedit)




Data File : VW014808.D
Acq On : 30 Jan 2020 13:03
Operator : SY/VA
Sample : L1303-09
Misc : 3.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0AF4

Quant Time: Jan 31 01:11:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:22:24 PM

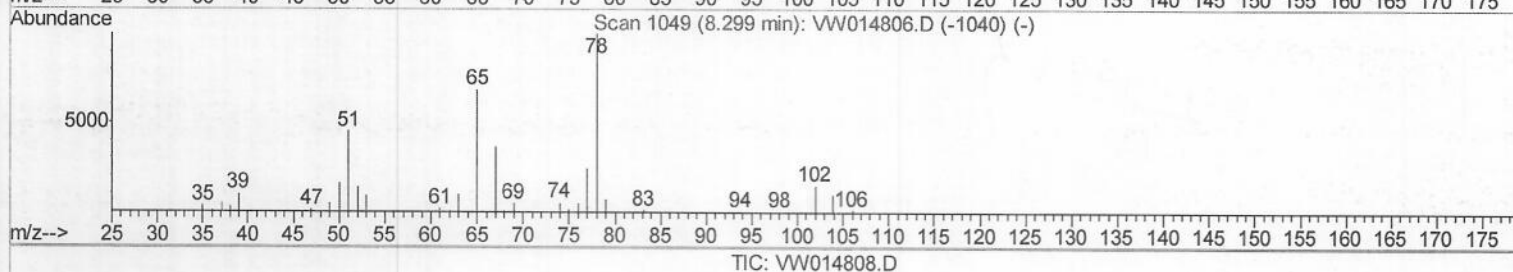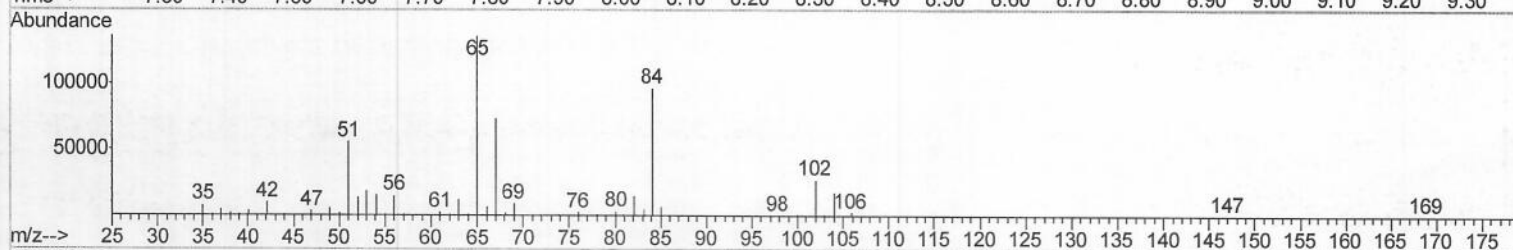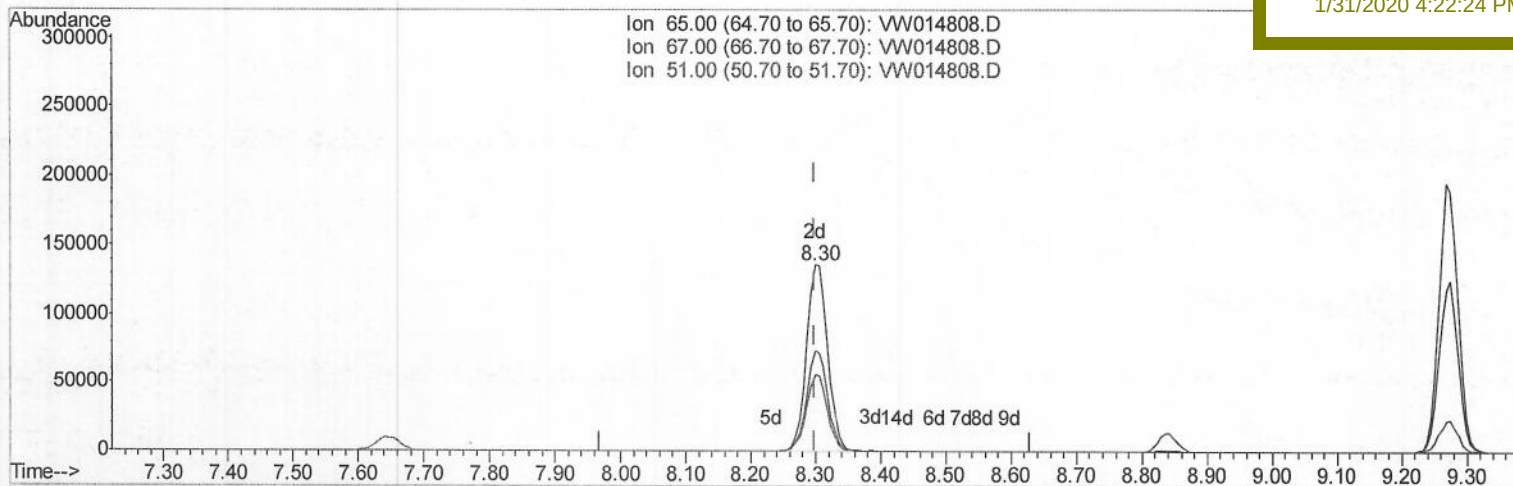

(26) 1,2-Dichloroethane-d4 (S)

8.299min (+0.000) 17.48ug/L m

response 307021

Ion	Exp%	Act%
65.00	100	100
67.00	53.40	0.04#
51.00	102.70	0.07#
0.00	0.00	0.00

802104/20 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW013020\
Quantitation Report (QT Reviewed)

Data File : VW014808.D
Acq On : 30 Jan 2020 13:03
Operator : SY/VA
Sample : L1303-09
Misc : 3.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 01:18:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
C0AF4

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:22:24 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	1181670	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1030896	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	412823	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	329267	17.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.36%
7) Chloroethane-d5	2.89	69	283034	17.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.20%
10) 1,1-Dichloroethene-d2	4.01	63	481729m	14.22	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.88%
20) 2-Butanone-d5	7.07	46	125799	23.67	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	47.34%
24) Chloroform-d	7.65	84	604548	18.53	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.12%
26) 1,2-Dichloroethane-d4	8.30	65	307021m	17.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	69.92%#
29) Benzene-d6	8.27	84	1258135	19.39	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.56%
33) 1,2-Dichloropropane-d6	9.27	67	390341	19.35	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.40%
37) Toluene-d8	10.32	98	1048842	18.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.60%
38) trans-1,3-Dichloropropene-	10.57	79	132875	16.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.12%
39) 2-Hexanone-d5	10.92	63	89004	23.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	47.04%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	208693	13.19	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	52.76%
61) 1,2-Dichlorobenzene-d4	13.85	152	290131	17.93	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	71.72%#

Target Compounds					Qvalue
16) Methylene chloride	4.92	84	36711	1.838 ug/L	92
47) Tetrachloroethene	10.86	164	15786	1.178 ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

02/04/2020