




Data File : VW014816.D
Acq On : 30 Jan 2020 19:03
Operator : SY/VA
Sample : L1323-01
Misc : 5.07G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT41

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:23:49 PM

Quant Time: Jan 31 01:12:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

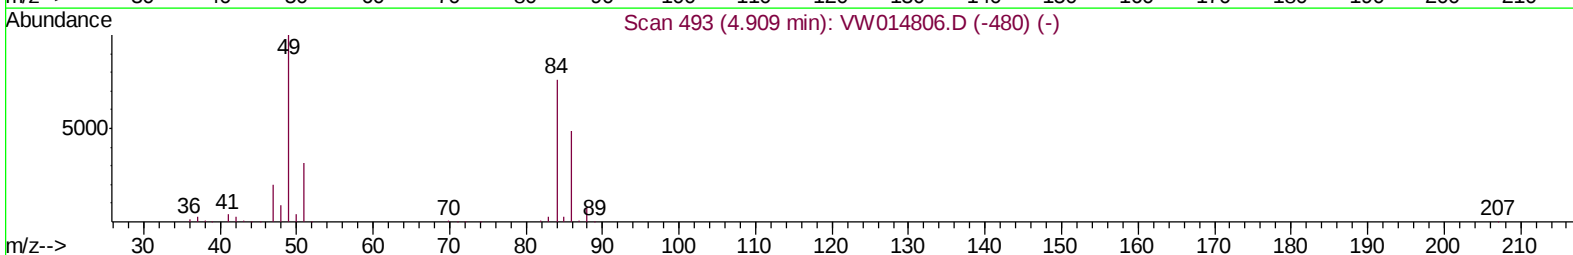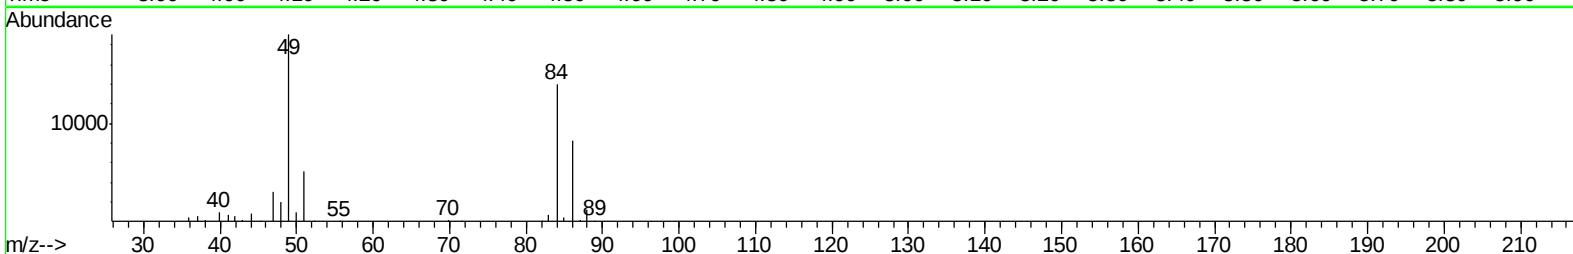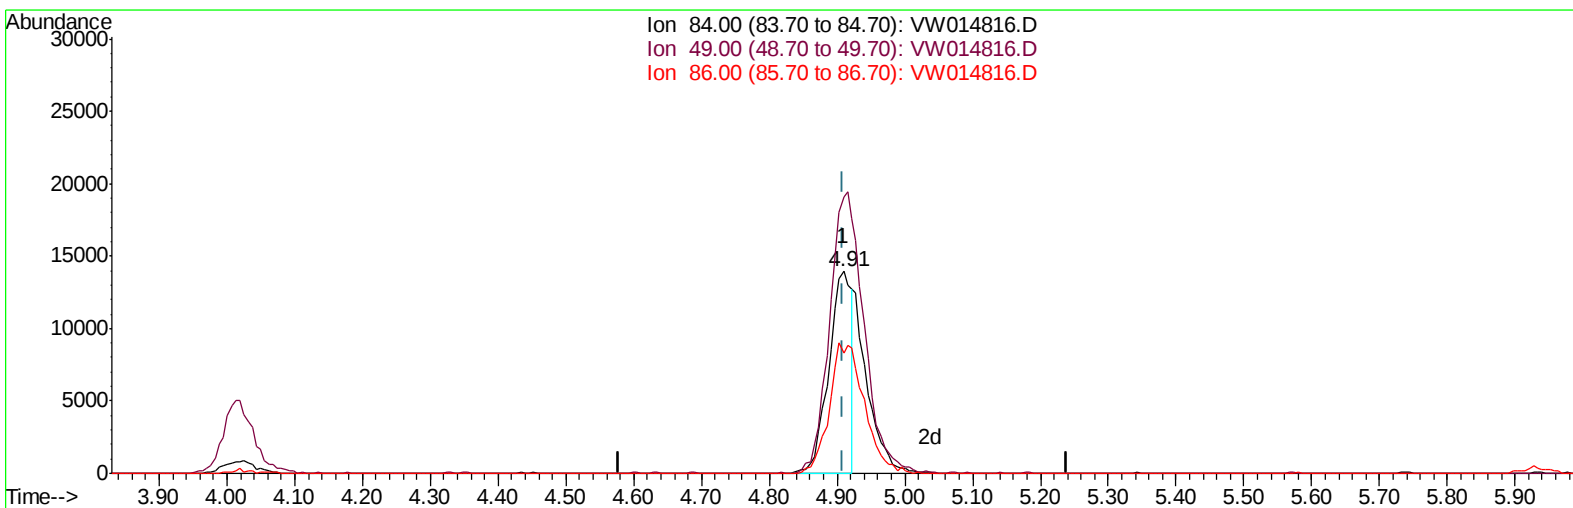

TIC: VW014816.D

(16) Methylene chloride (T)

4.909min (+0.000) 1.35ug/L

response 32562

Ion	Exp%	Act%
84.00	100	100
49.00	129.80	136.65
86.00	62.10	59.35
0.00	0.00	0.00




Data File : VW014816.D
Acq On : 30 Jan 2020 19:03
Operator : SY/VA
Sample : L1323-01
Misc : 5.07G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT41

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:23:49 PM

Quant Time: Jan 31 01:12:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

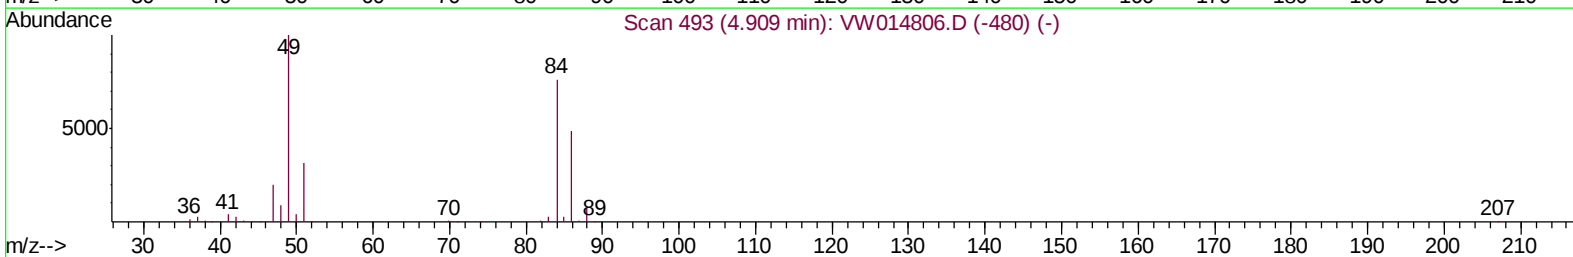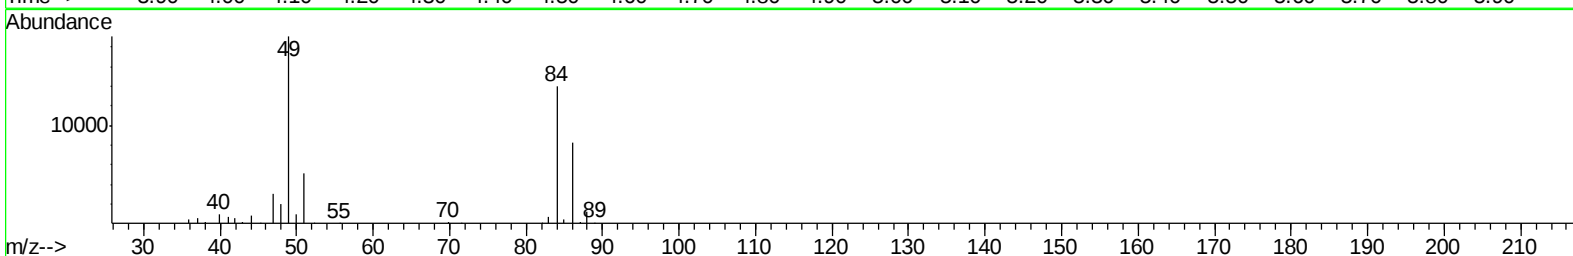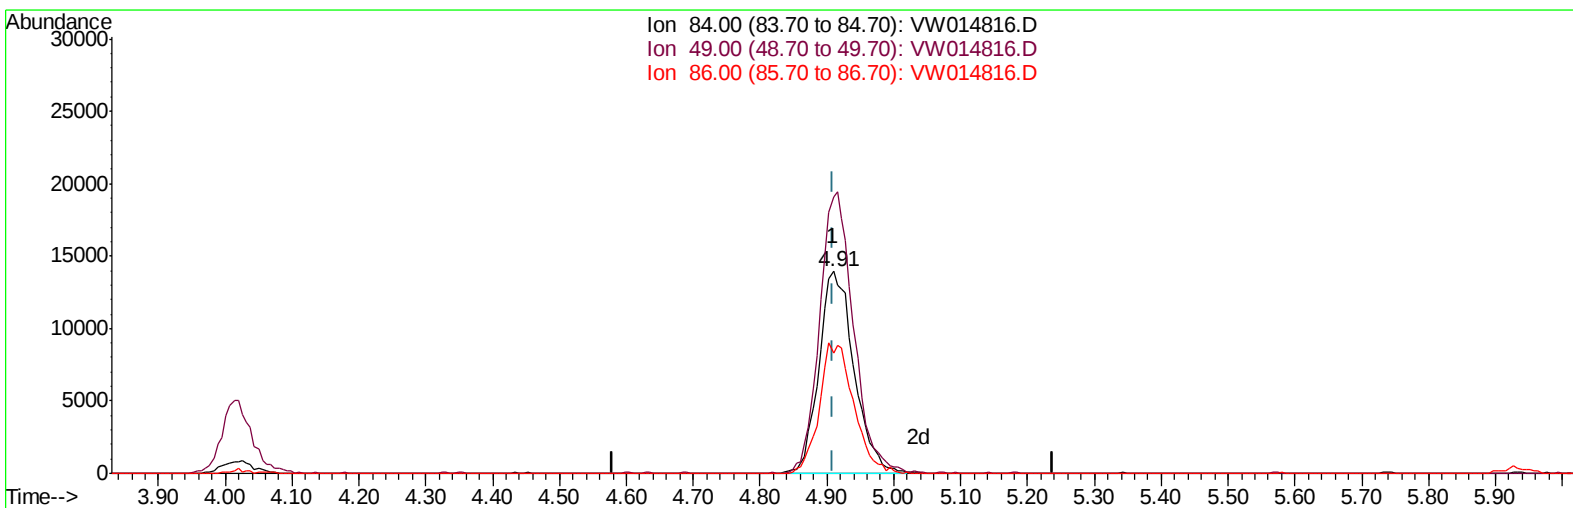

TIC: VW014816.D

(16) Methylene chloride (T)

4.909min (+0.000) 2.10ug/L m

response 50754

Ion	Exp%	Act%
84.00	100	100
49.00	129.80	136.65
86.00	62.10	59.35
0.00	0.00	0.00

Data File : VW014816.D
Acq On : 30 Jan 2020 19:03
Operator : SY/VA
Sample : L1323-01
Misc : 5.07G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT41

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:23:49 PM

Quant Time: Jan 31 03:21:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1432240	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1237617	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	540469	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	385700	17.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.00%
7) Chloroethane-d5	2.89	69	373415	19.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.48%
10) 1,1-Dichloroethene-d2	4.01	63	690023	16.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.24%
20) 2-Butanone-d5	7.07	46	260107	40.38	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.76%
24) Chloroform-d	7.65	84	878983	22.23	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.92%
26) 1,2-Dichloroethane-d4	8.30	65	466797	21.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.68%
29) Benzene-d6	8.27	84	1890163	24.27	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.08%
33) 1,2-Dichloropropane-d6	9.27	67	599256	24.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.00%
37) Toluene-d8	10.32	98	1651490	23.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.20%
38) trans-1,3-Dichloropropene-	10.57	79	225758	23.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.60%
39) 2-Hexanone-d5	10.92	63	205401	45.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.42%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	398247	20.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.84%
61) 1,2-Dichlorobenzene-d4	13.85	152	496639	23.45	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.80%

Target Compounds					Qvalue
16) Methylene chloride	4.91	84	50754m	2.097	ug/L
44) Toluene	10.38	91	71425	0.887	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014816.D
Acq On : 30 Jan 2020 19:03
Operator : SY/VA
Sample : L1323-01
Misc : 5.07G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT41

Manual Integrations
APPROVED

MMDadoda
1/31/2020 4:23:49 PM

Quant Time: Jan 31 03:21:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

