
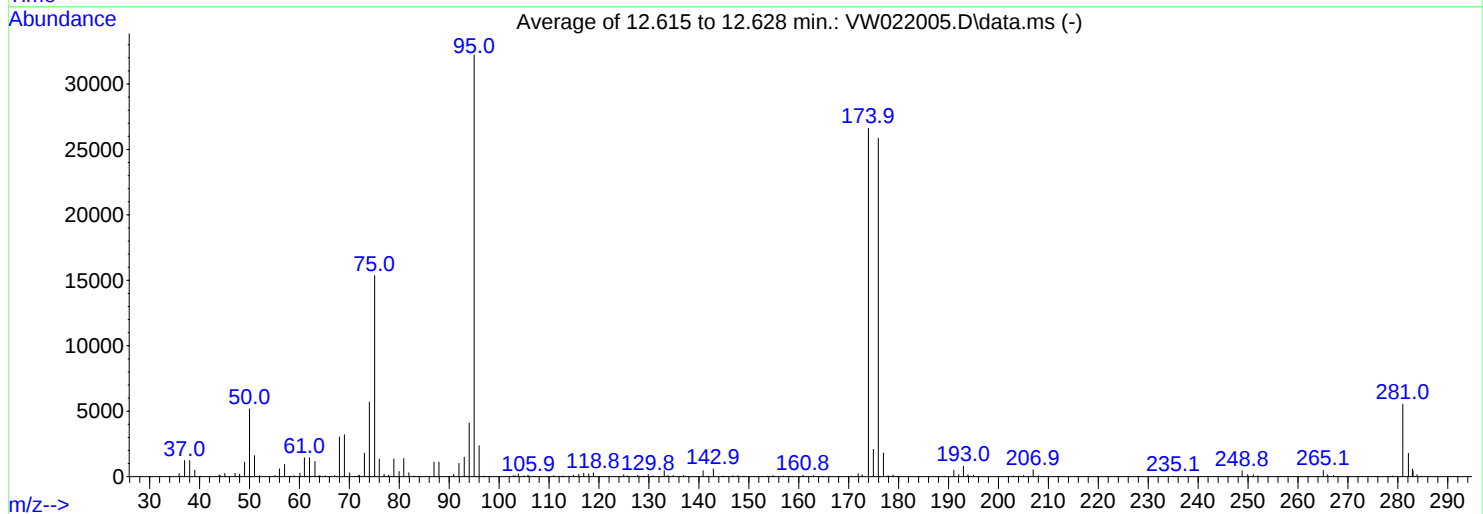


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020122\
Data File : VW022005.D
Acq On : 01 Feb 2022 10:55
Operator : SY/VA
Sample : BFB506
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB506

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
Title : SFAM01.0
Last Update : Thu Feb 03 01:57:48 2022

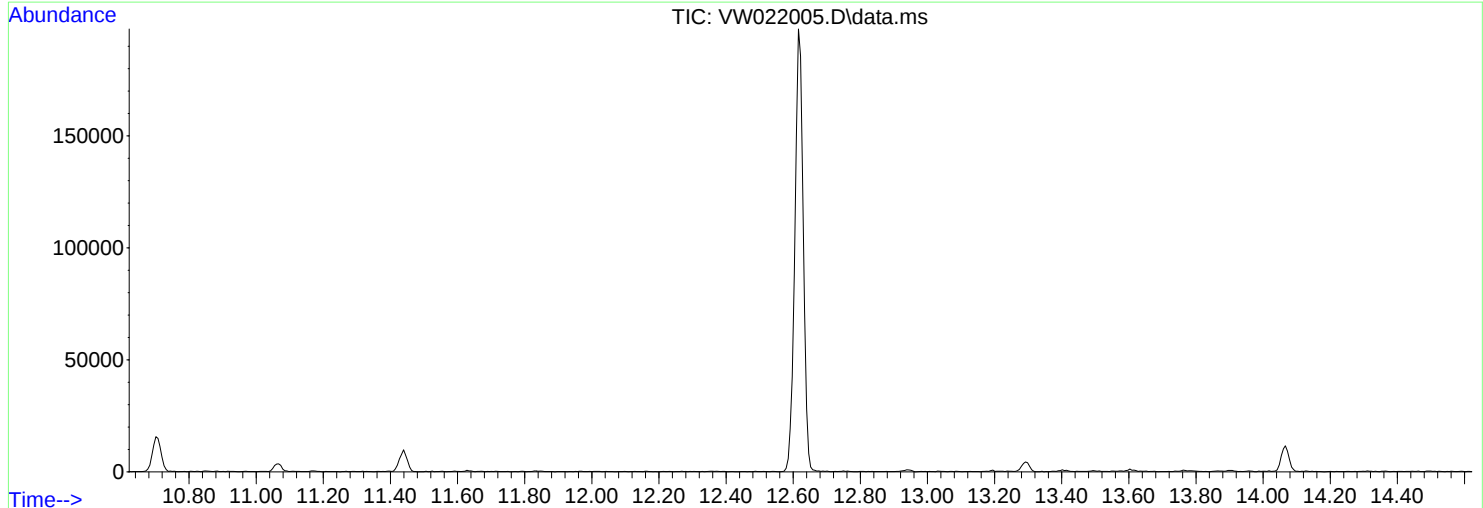

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	5176	PASS
75	95	30	80	47.7	15366	PASS
95	95	100	100	100.0	32227	PASS
96	95	5	9	7.3	2355	PASS
173	174	0.00	2	0.6	147	PASS
174	95	50	120	82.6	26619	PASS
175	174	5	9	7.8	2081	PASS
176	174	95	105	97.1	25853	PASS
177	176	5	10	6.9	1796	PASS

m/z	Abundance
39.90	117.0
44.00	64.0
281.00	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB506

m/z	Abundance
36.00	294.0
37.00	1510.0
38.00	1327.0
39.10	556.0
39.90	91.0
43.90	343.0
45.10	311.0
45.80	52.0
47.10	297.0
48.00	258.0
49.00	1413.0
50.00	6271.0
51.00	1761.0
52.00	73.0
55.10	125.0
56.00	791.0
57.00	1159.0
58.20	51.0
59.00	108.0
60.10	370.0
61.00	1672.0
62.00	1652.0
63.10	1332.0
63.90	149.0
65.20	102.0
67.00	94.0
68.00	3424.0
69.00	3443.0
70.00	363.0
71.00	62.0
72.10	148.0
73.00	2346.0
74.00	6508.0
75.10	17608.0
76.00	1761.0
76.90	204.0
77.80	154.0
78.90	1491.0
79.90	433.0
80.90	1598.0
81.90	334.0
82.90	81.0
87.00	1213.0
87.90	1296.0
90.90	218.0
91.90	1167.0
93.00	1631.0
94.00	4518.0
95.00	36080.0
96.00	2716.0
103.20	189.0
103.80	189.0
105.10	57.0
105.70	192.0
107.00	65.0
109.70	62.0
111.00	108.0
112.00	116.0
112.80	52.0
114.90	143.0
116.00	195.0
117.10	253.0
118.00	256.0
118.90	381.0
125.00	229.0
125.70	103.0
127.70	119.0
129.00	63.0
129.90	189.0
130.60	101.0
133.10	834.0
133.90	207.0
134.90	199.0
137.00	100.0
140.90	488.0
142.90	521.0
144.90	92.0
146.90	155.0
147.70	128.0
149.00	58.0
153.80	53.0
154.90	128.0
160.90	152.0
162.90	138.0
164.70	94.0
171.90	196.0
174.00	26248.0
174.90	2096.0
175.90	27376.0
177.00	2065.0
177.90	101.0
178.90	338.0

Instrument :
MSVOA_W
ClientSampleId :
BFB506

179.70	84.0
189.20	123.0
191.10	772.0
192.10	203.0
193.00	1277.0
193.90	244.0
195.00	248.0
203.10	109.0
205.00	204.0
206.00	123.0
207.00	866.0
208.00	160.0
209.10	85.0
235.10	53.0
248.80	639.0
249.90	206.0
251.00	229.0
251.90	104.0
265.00	753.0
265.90	324.0
267.10	217.0
268.10	55.0
278.00	90.0
279.00	180.0
281.00	9163.0
282.10	3239.0
282.90	1752.0
283.90	280.0
284.80	115.0

Instrument :
MSVOA_W
ClientSampleId :
BFB506

m/z	Abundance
35.90	227.0
37.00	1487.0
38.00	1474.0
39.00	541.0
40.20	59.0
44.10	342.0
45.00	286.0
47.00	322.0
48.00	209.0
49.00	1212.0
50.00	5581.0
51.00	1684.0
52.10	79.0
54.90	74.0
56.00	554.0
57.00	1093.0
58.10	54.0
58.90	134.0
60.10	283.0
61.00	1490.0
62.00	1518.0
63.10	1295.0
63.90	103.0
65.10	67.0
67.00	91.0
68.00	3369.0
69.00	3660.0
70.00	289.0
72.00	170.0
73.00	1884.0
74.00	6260.0
75.00	16440.0
76.00	1192.0
77.00	161.0
77.90	120.0
78.90	1495.0
79.90	394.0
80.90	1579.0
81.90	333.0
83.00	60.0
87.00	1202.0
88.00	1215.0
90.90	203.0
92.00	1098.0
93.00	1640.0
94.00	4319.0
95.00	36128.0
96.00	2367.0
96.90	57.0
102.90	166.0
103.80	225.0
105.00	62.0
105.90	219.0
107.00	56.0
110.90	72.0
112.80	66.0
114.80	132.0
116.00	219.0
116.90	305.0
117.80	236.0
118.80	298.0
125.00	92.0
125.70	75.0
127.70	168.0
128.60	65.0
129.80	150.0
130.80	119.0
132.00	53.0
132.90	431.0
133.60	187.0
134.80	106.0
136.90	116.0
140.90	504.0
141.80	63.0
142.90	685.0
145.20	58.0
146.80	91.0
147.90	95.0
149.10	67.0
153.70	63.0
154.80	114.0
156.90	75.0
158.70	51.0
160.80	117.0
163.00	140.0
164.90	67.0
170.60	54.0
172.00	320.0
172.70	441.0
173.90	30064.0
175.00	2263.0
176.00	26688.0

Instrument :
MSVOA_W
ClientSampleId :
BFB506

176.90	1771.0
177.90	109.0
178.90	63.0
191.00	484.0
192.10	128.0
193.00	858.0
193.90	182.0
194.70	67.0
195.00	82.0
203.00	81.0
205.10	68.0
206.90	527.0
208.10	64.0
235.00	60.0
248.80	443.0
250.00	196.0
251.10	115.0
252.00	67.0
265.10	444.0
265.70	124.0
267.10	69.0
278.40	50.0
281.00	5475.0
282.10	1382.0
283.10	955.0
283.80	167.0

Instrument :
MSVOA_W
ClientSampleId :
BFB506

m/z	Abundance
35.80	177.0
37.10	705.0
38.10	881.0
39.00	410.0
40.00	63.0
43.10	63.0
43.90	234.0
45.10	178.0
47.20	136.0
47.90	133.0
49.00	695.0
50.00	3677.0
51.00	1374.0
51.90	78.0
55.20	88.0
56.00	439.0
56.90	535.0
60.10	164.0
61.00	1160.0
62.00	1150.0
63.00	861.0
64.20	111.0
65.10	62.0
67.10	84.0
68.00	2312.0
69.00	2525.0
70.10	241.0
71.80	266.0
73.00	1162.0
74.00	4314.0
75.00	12050.0
76.00	1068.0
76.90	176.0
77.90	69.0
78.90	1100.0
80.00	335.0
80.80	974.0
82.00	207.0
86.00	69.0
86.90	913.0
88.00	844.0
91.00	125.0
92.00	778.0
93.00	1150.0
94.00	3438.0
95.00	24472.0
96.00	1983.0
97.10	97.0
102.80	65.0
103.90	215.0
104.90	61.0
105.70	65.0
106.10	77.0
110.90	72.0
112.80	53.0
115.00	74.0
115.80	96.0
116.80	220.0
118.00	174.0
118.90	205.0
124.90	115.0
128.00	128.0
129.00	80.0
129.90	146.0
130.90	81.0
132.80	83.0
133.20	90.0
136.90	84.0
140.80	381.0
141.80	50.0
142.90	547.0
144.70	57.0
145.20	64.0
145.60	51.0
147.80	105.0
152.70	64.0
155.10	81.0
157.00	66.0
158.70	70.0
160.80	87.0
170.60	51.0
171.20	54.0
171.80	181.0
173.90	23544.0
174.90	1885.0
175.90	23496.0
176.90	1551.0
190.90	224.0
192.00	112.0
192.80	265.0
194.10	73.0
206.80	172.0

Instrument :
MSVOA_W
ClientSampleId :
BFB506

248.90	246.0
250.10	62.0
251.00	57.0
265.00	240.0
266.10	82.0
281.00	2288.0
282.00	697.0
283.00	345.0
284.20	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB506