


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020222\
 Data File : VW022023.D
 Acq On : 02 Feb 2022 08:52
 Operator : SY/VA
 Sample : BFB507
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB507

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
 Title : SFAM01.0
 Last Update : Thu Feb 03 01:57:48 2022

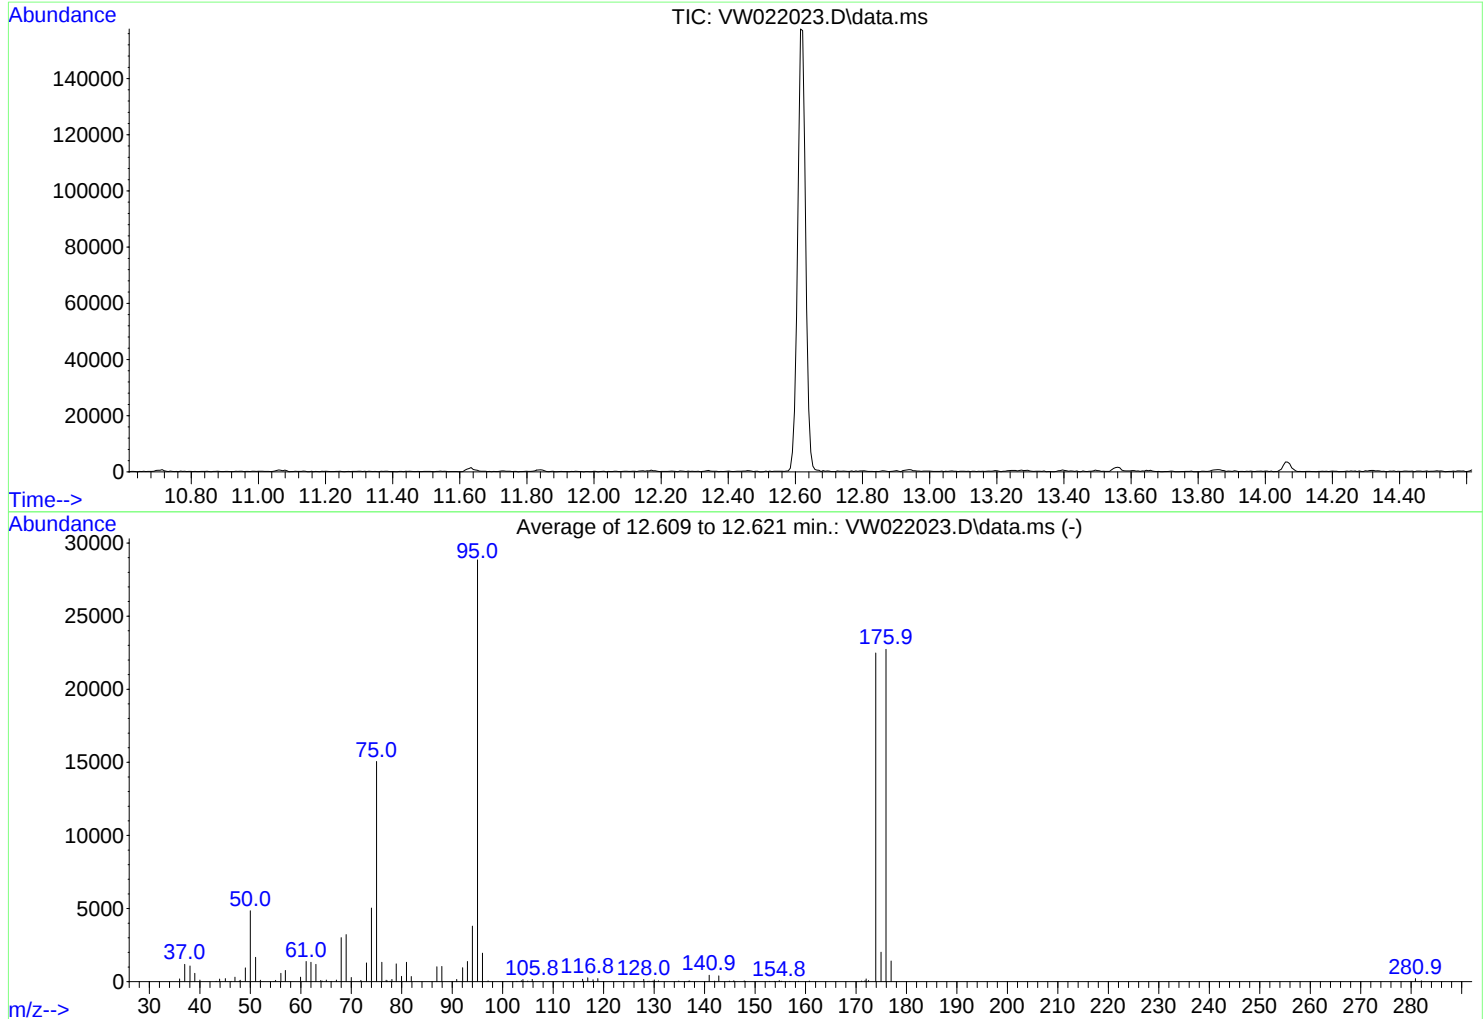

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	4847	PASS
75	95	30	80	52.2	15059	PASS
95	95	100	100	100.0	28851	PASS
96	95	5	9	6.7	1946	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.9	22477	PASS
175	174	5	9	8.9	2009	PASS
176	174	95	105	101.1	22735	PASS
177	176	5	10	6.2	1408	PASS

m/z	Abundance
36.00	99.0
40.30	66.0
43.90	72.0
57.10	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB507

m/z	Abundance
36.10	258.0
37.00	975.0
38.10	911.0
39.00	538.0
40.00	60.0
44.00	231.0
45.10	149.0
46.90	227.0
47.80	125.0
49.00	906.0
50.00	4083.0
51.10	1381.0
52.10	109.0
54.70	52.0
55.10	77.0
56.10	392.0
56.90	663.0
60.00	292.0
61.00	1172.0
62.00	1206.0
63.00	1039.0
64.00	106.0
65.10	94.0
66.00	62.0
67.00	77.0
68.00	2520.0
69.00	2583.0
70.00	212.0
71.90	118.0
73.00	995.0
74.00	3985.0
75.00	12322.0
76.10	1108.0
76.90	144.0
77.70	90.0
78.20	134.0
78.90	1038.0
79.90	281.0
81.00	1305.0
81.90	228.0
87.00	821.0
87.90	890.0
90.90	113.0
92.00	807.0
93.00	1068.0
94.00	3154.0
95.00	22968.0
96.00	1370.0
104.00	164.0
105.80	150.0
115.80	138.0
116.90	195.0
117.90	128.0
118.90	169.0
128.00	121.0
130.00	105.0
137.00	69.0
140.90	348.0
142.80	388.0
144.90	75.0
147.80	72.0
155.20	101.0
160.70	52.0
171.20	77.0
171.80	207.0
172.50	238.0
173.90	16896.0
174.90	1537.0
175.90	15629.0
177.00	1008.0
280.90	310.0
282.00	102.0

Instrument :
MSVOA_W
ClientSampleId :
BFB507

m/z	Abundance
36.00	321.0
37.00	1450.0
38.10	1206.0
39.00	644.0
40.00	130.0
43.90	219.0
45.00	251.0
47.00	313.0
48.00	135.0
49.00	1022.0
50.00	5505.0
51.10	1990.0
52.00	133.0
55.10	77.0
56.10	663.0
57.00	914.0
60.00	321.0
61.00	1464.0
62.00	1455.0
63.00	1263.0
64.20	128.0
65.10	102.0
66.90	80.0
68.00	3323.0
69.00	3806.0
70.00	385.0
71.90	153.0
73.00	1445.0
74.00	5981.0
75.00	16311.0
76.00	1659.0
77.10	160.0
78.00	170.0
78.90	1308.0
79.90	431.0
81.00	1326.0
81.90	455.0
86.90	991.0
88.00	959.0
91.00	159.0
92.10	1122.0
93.00	1641.0
94.00	4060.0
95.00	32832.0
96.00	2205.0
97.10	61.0
102.80	57.0
103.70	186.0
104.90	56.0
105.90	152.0
115.90	168.0
116.80	339.0
117.90	135.0
118.90	243.0
128.00	196.0
129.00	99.0
130.10	124.0
130.90	78.0
134.90	82.0
137.10	92.0
140.90	527.0
142.90	427.0
144.90	67.0
145.80	76.0
148.10	62.0
153.90	60.0
154.80	99.0
160.80	71.0
172.00	276.0
173.90	24504.0
175.00	2129.0
175.90	24736.0
176.90	1615.0
280.80	186.0
282.00	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB507

m/z	Abundance
36.00	279.0
37.00	1126.0
38.00	1111.0
39.00	541.0
40.00	142.0
43.20	75.0
43.90	289.0
45.00	208.0
46.20	56.0
47.00	371.0
48.00	174.0
49.00	914.0
50.00	4954.0
51.00	1633.0
51.90	70.0
54.90	118.0
56.00	658.0
57.00	866.0
59.90	312.0
61.10	1491.0
62.00	1309.0
63.00	1248.0
63.90	139.0
65.00	120.0
67.10	179.0
68.00	3177.0
69.00	3264.0
70.00	247.0
73.00	1393.0
74.00	5129.0
75.00	16544.0
76.00	1220.0
76.90	151.0
78.00	144.0
78.90	1291.0
80.00	384.0
80.90	1336.0
81.90	371.0
86.90	1233.0
87.90	1256.0
90.80	190.0
92.00	943.0
93.00	1432.0
94.00	4173.0
95.00	30752.0
96.00	2264.0
97.10	101.0
104.00	259.0
105.00	79.0
105.80	150.0
115.90	187.0
116.80	254.0
117.90	138.0
118.70	207.0
127.90	134.0
128.70	69.0
129.80	125.0
130.10	125.0
130.80	73.0
134.90	55.0
136.80	90.0
140.90	453.0
142.00	92.0
142.70	381.0
145.80	106.0
147.90	108.0
152.90	55.0
154.80	127.0
156.90	58.0
158.60	64.0
171.00	56.0
172.00	295.0
173.90	26032.0
175.00	2360.0
176.00	27840.0
176.90	1601.0
280.90	113.0

Instrument :
MSVOA_W
ClientSampleId :
BFB507