

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020320\
Quantitation Report (Qedit)




Data File : VW014849.D
Acq On : 03 Feb 2020 21:46
Operator : SY/VA
Sample : L1323-12
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
GAT50

Manual Integrations
APPROVED

MMDadoda
2/4/2020 3:40:07 PM

Quant Time: Feb 04 06:58:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020320S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 04 06:54:20 2020
Response via : Initial Calibration

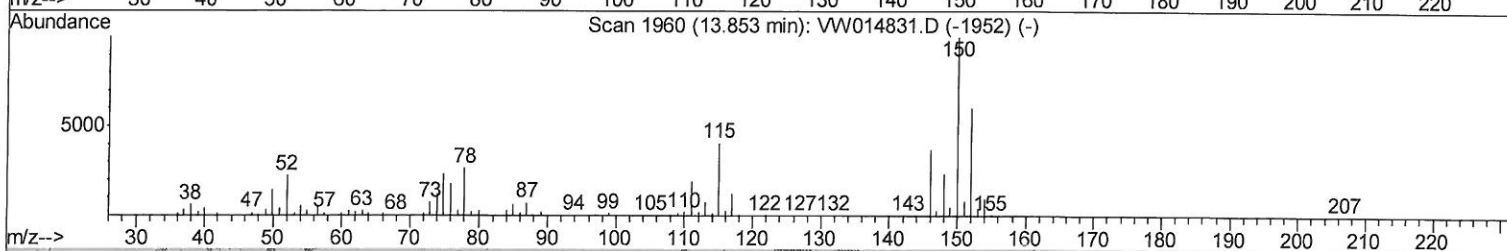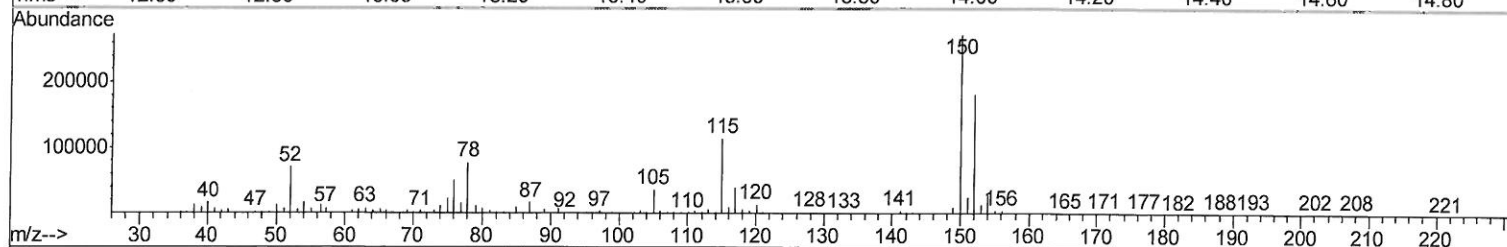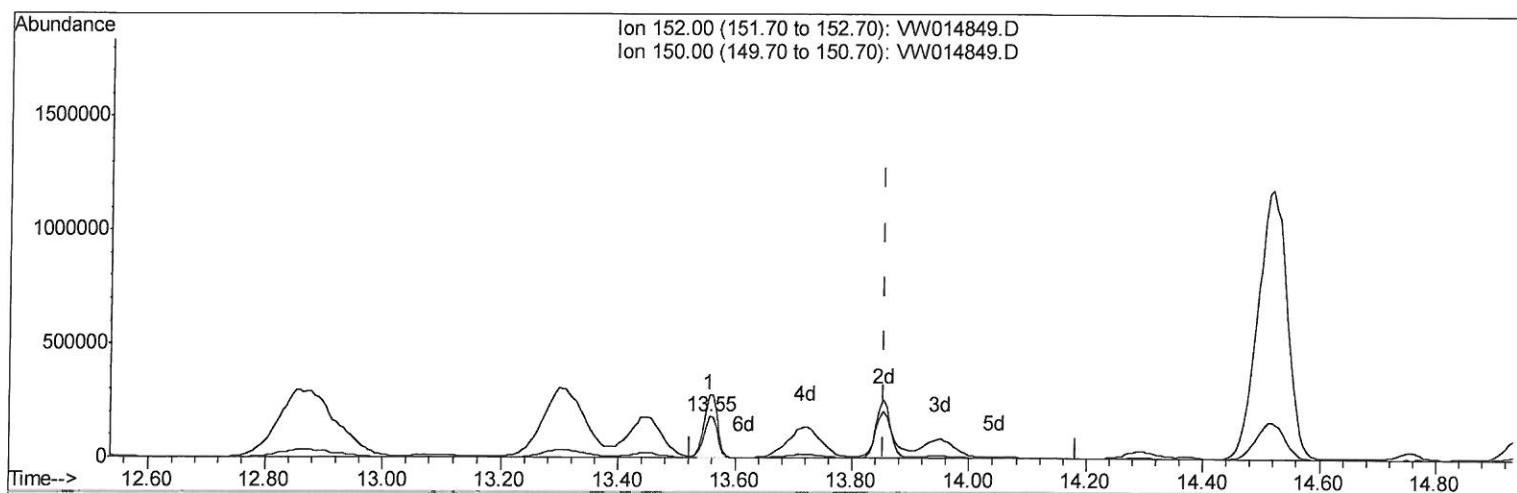

TIC: VW014849.D

(61) 1,2-Dichlorobenzene-d4 (S)

13.554min (-0.299) 22.90ug/L

response 280982

Ion	Exp%	Act%
152.00	100	100
150.00	168.30	155.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020320\
Quantitation Report (Qedit)




Data File : VW014849.D
Acq On : 03 Feb 2020 21:46
Operator : SY/VA
Sample : L1323-12
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT50

Manual Integrations
APPROVED

MMDadoda
2/4/2020 3:40:07 PM

Quant Time: Feb 04 06:58:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020320S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 04 06:54:20 2020
Response via : Initial Calibration

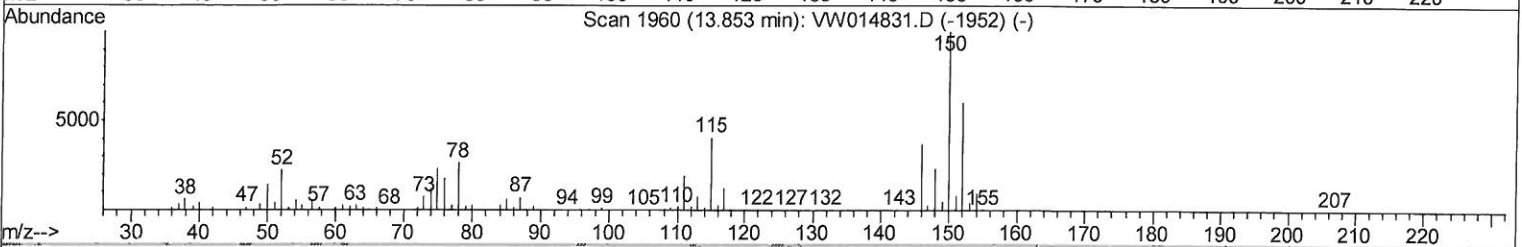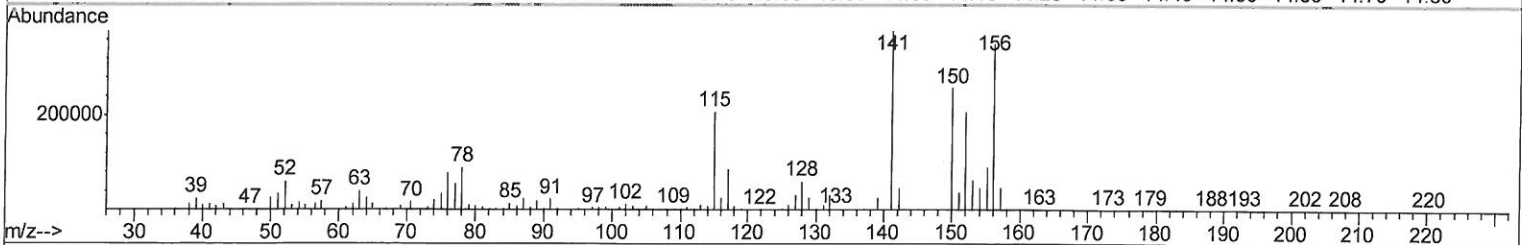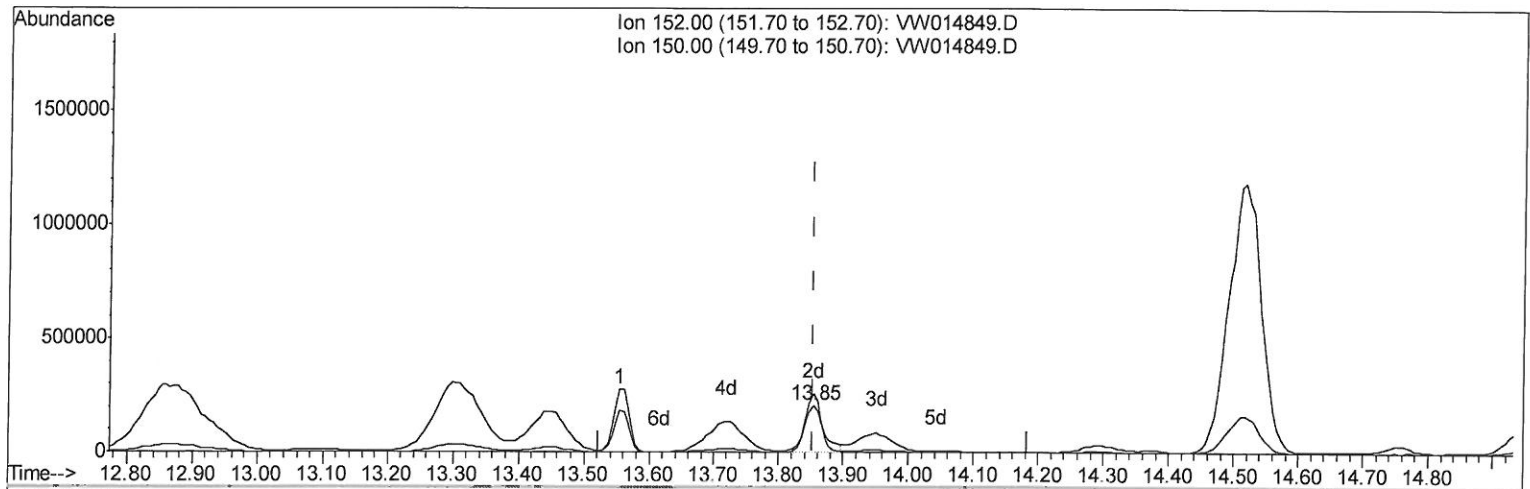

TIC: VW014849.D

(61) 1,2-Dichlorobenzene-d4 (S)

13.853min (0.000) 35.88ug/L m

response 440170

Ion	Exp%	Act%
152.00	100	100
150.00	168.30	98.94#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020320\
Quantitation Report (QT Reviewed)

Data File : VW014849.D
Acq On : 03 Feb 2020 21:46
Operator : SY/VA
Sample : L1323-12
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT50

Manual Integrations
APPROVED

MMDadoda
2/4/2020 3:40:07 PM

Quant Time: Feb 04 08:28:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020320S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 04 06:54:20 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	961202	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	826927	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	292851	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	229049	15.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.84%
7) Chloroethane-d5	2.89	69	225351	15.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.64%
10) 1,1-Dichloroethene-d2	4.01	63	408360	12.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.08%
20) 2-Butanone-d5	7.07	46	179539	31.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.46%
24) Chloroform-d	7.65	84	579515	18.94	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.76%
26) 1,2-Dichloroethane-d4	8.31	65	317223	18.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.76%
29) Benzene-d6	8.27	84	1221780	20.96	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.84%
33) 1,2-Dichloropropane-d6	9.27	67	405607	21.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.92%
37) Toluene-d8	10.32	98	1089491	21.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.64%
38) trans-1,3-Dichloropropene-	10.57	79	141811	18.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.00%
39) 2-Hexanone-d5	10.92	63	151878	40.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.22%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	251049	16.86	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	67.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	440170m	35.88	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	143.52%#

02/04/2020

Target Compounds					Qvalue
13) Acetone	4.12	43	24889	4.067	ug/L 100
16) Methylene chloride	4.91	84	38916	2.193	ug/L 98
44) Toluene	10.38	91	266052	4.592	ug/L 99
53) Ethylbenzene	11.73	91	559379	8.911	ug/L 99
54) m,p-Xylene	11.84	106	2035323	88.605	ug/L 97
55) o-xylene	12.16	106	1471832	68.778	ug/L 96
56) Styrene	12.18	104	6954825	190.853	ug/L 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW020320\
Quantitation Report (QT Reviewed)

Data File : VW014849.D
Acq On : 03 Feb 2020 21:46
Operator : SY/VA
Sample : L1323-12
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT50

Manual Integrations
APPROVED

MMDadoda
2/4/2020 3:40:07 PM

Quant Time: Feb 04 08:28:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020320S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 04 06:54:20 2020
Response via : Initial Calibration

