

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020321\
 Data File : VW018023.D
 Acq On : 03 Feb 2021 11:28
 Operator : SY/VA
 Sample : M1298-11
 Misc : 5.52G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0A37

Quant Time: Feb 03 21:59:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 03 21:58:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	397536	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	328533	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	146246	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	114852	23.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.00%
7) Chloroethane-d5	2.891	69	92985	23.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.84%
10) 1,1-Dichloroethene-d2	4.019	63	177566	17.98	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.92%
20) 2-Butanone-d5	7.074	46	44557	33.79	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.58%
24) Chloroform-d	7.647	84	251571	24.11	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.44%
26) 1,2-Dichloroethane-d4	8.305	65	125959	22.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.68%
29) Benzene-d6	8.275	84	502399	27.85	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.40%
33) 1,2-Dichloropropane-d6	9.274	67	139912	27.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.92%
37) Toluene-d8	10.323	98	461388	26.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	107.52%
38) trans-1,3-Dichloroprop...	10.573	79	56131	24.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.16%
39) 2-Hexanone-d5	10.927	63	35941	37.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.52%
48) 1,1,2,2-Tetrachloroeth...	12.688	84	93046	20.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.96%
61) 1,2-Dichlorobenzene-d4	13.853	152	136248	26.12	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.48%
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	9499	9.74	ug/L	98
16) Methylene chloride	4.909	84	8678	1.36	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020321\
Data File : VW018023.D
Acq On : 03 Feb 2021 11:28
Operator : SY/VA
Sample : M1298-11
Misc : 5.52G/10ML/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0A37

Quant Time: Feb 03 21:59:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 03 21:58:46 2021
Response via : Initial Calibration




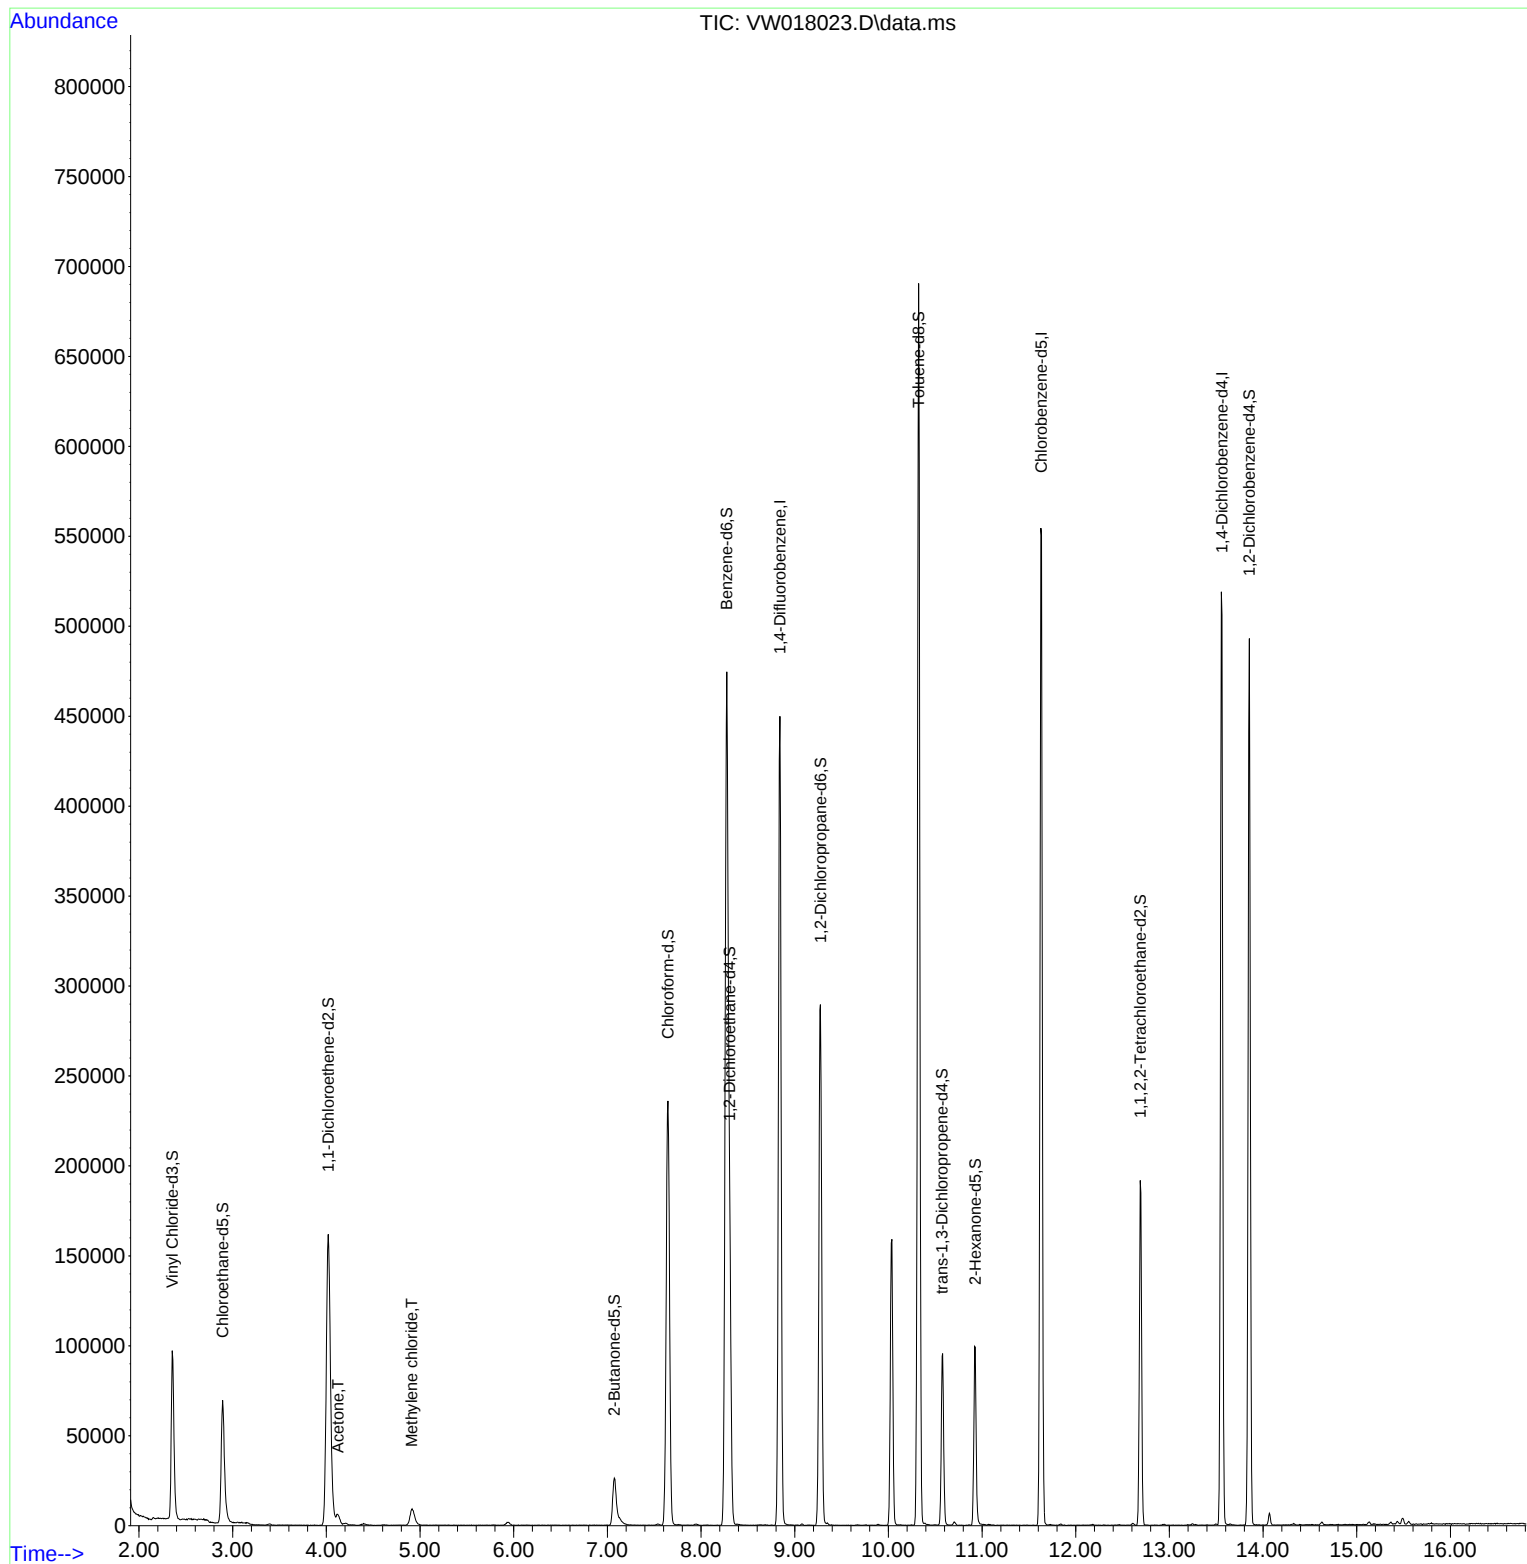


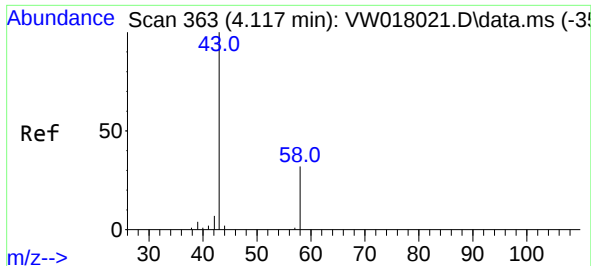

#13
Acetone
Concen: 9.74 ug/L
RT: 4.123 min Scan# 364
Delta R.T. 0.006 min
Lab File: VW018023.D
Acq: 03 Feb 2021 11:28

Instrument :
MSVOA_W
ClientSampled :
C0A37

Tgt Ion: 43 Resp: 9499
Ion Ratio Lower Upper
43 100
58 35.2 0.0 68.4

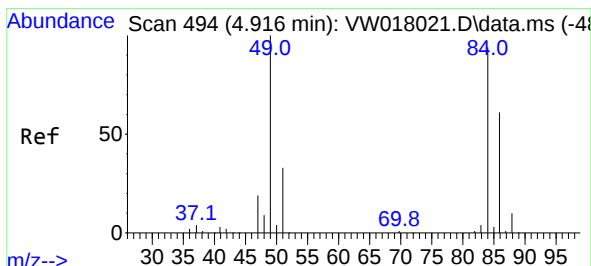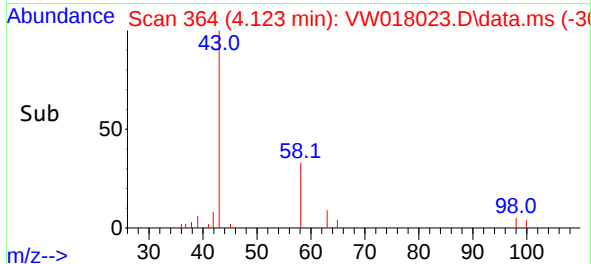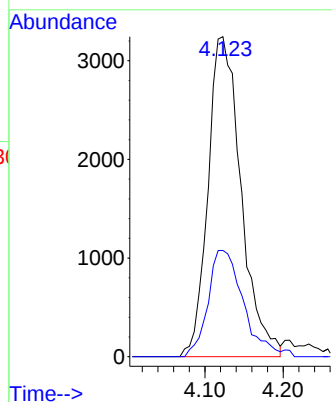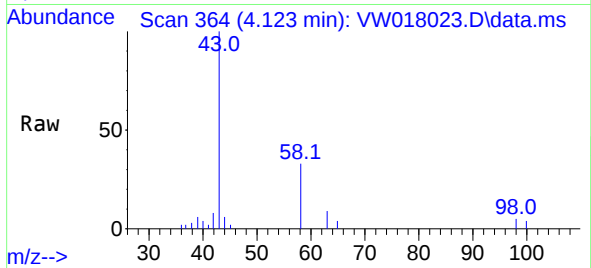

#16
Methylene chloride
Concen: 1.36 ug/L
RT: 4.909 min Scan# 493
Delta R.T. -0.006 min
Lab File: VW018023.D
Acq: 03 Feb 2021 11:28

Tgt Ion: 84 Resp: 8678
Ion Ratio Lower Upper
84 100
49 92.5 81.2 150.8
86 61.8 44.5 82.7

