

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020322\
 Data File : VW022072.D
 Acq On : 03 Feb 2022 16:51
 Operator : SY/VA
 Sample : N1353-12
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Feb 04 00:59:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 03 01:57:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	139573	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	127799	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	61938	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	43509	25.880	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.520%
7) Chloroethane-d5	2.885	69	31789	24.561	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.240%
11) 1,1-Dichloroethene-d2	4.019	63	47838	16.105	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.440%
21) 2-Butanone-d5	7.080	46	14332	48.062	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.120%
24) Chloroform-d	7.647	84	71302	21.958	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.840%
26) 1,2-Dichloroethane-d4	8.305	65	37953	23.492	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.960%
32) Benzene-d6	8.275	84	142132	22.008	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.040%
36) 1,2-Dichloropropane-d6	9.275	67	38910	22.150	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.600%
41) Toluene-d8	10.323	98	138024	21.564	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.240%
43) trans-1,3-Dichloroprop...	10.573	79	15383	19.995	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.960%
47) 2-Hexanone-d5	10.921	63	12589	49.292	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.580%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	31437	21.942	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	50061	22.405	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.600%
Target Compounds						Qvalue
37) 1,2-Dichloropropane	9.275	63	4770	3.241	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020322\
Data File : VW022072.D
Acq On : 03 Feb 2022 16:51
Operator : SY/VA
Sample : N1353-12
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Feb 04 00:59:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 03 01:57:48 2022
Response via : Initial Calibration

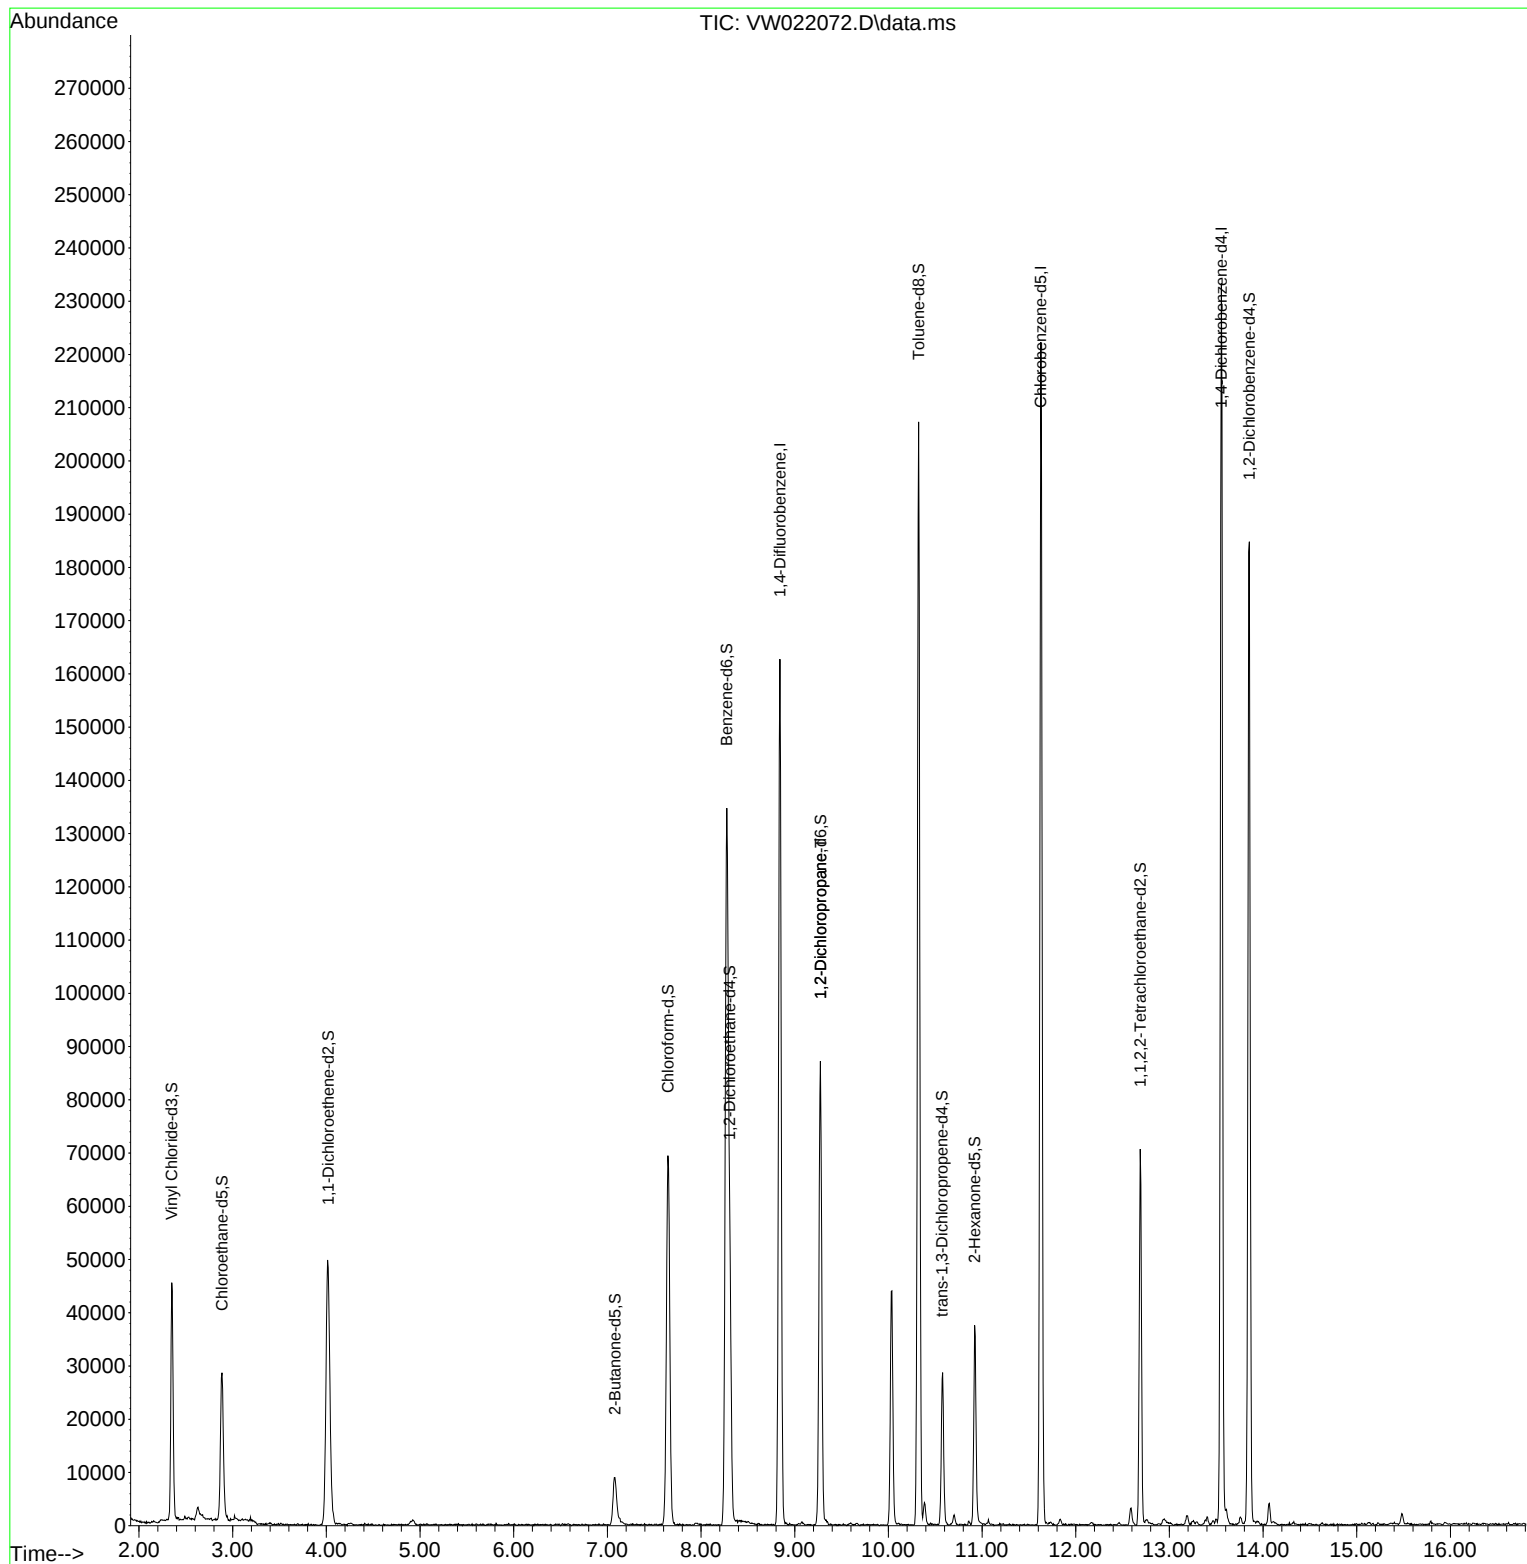

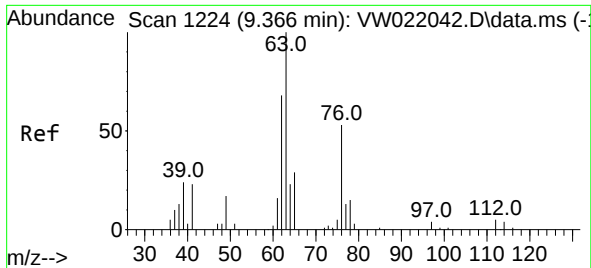

#37
 1,2-Dichloropropane
 Concen: 3.241 ug/L
 RT: 9.275 min Scan# 11
 Delta R.T. -0.091 min
 Lab File: VW022072.D
 Acq: 03 Feb 2022 16:51

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 63 Resp: 4770
 Ion Ratio Lower Upper
 63 100
 112 0.0 4.7 7.1#

