


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020322\
Data File : VW022064.D
Acq On : 03 Feb 2022 08:24
Operator : SY/VA
Sample : BFB508
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB508

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
Title : SFAM01.0
Last Update : Thu Feb 03 01:57:48 2022

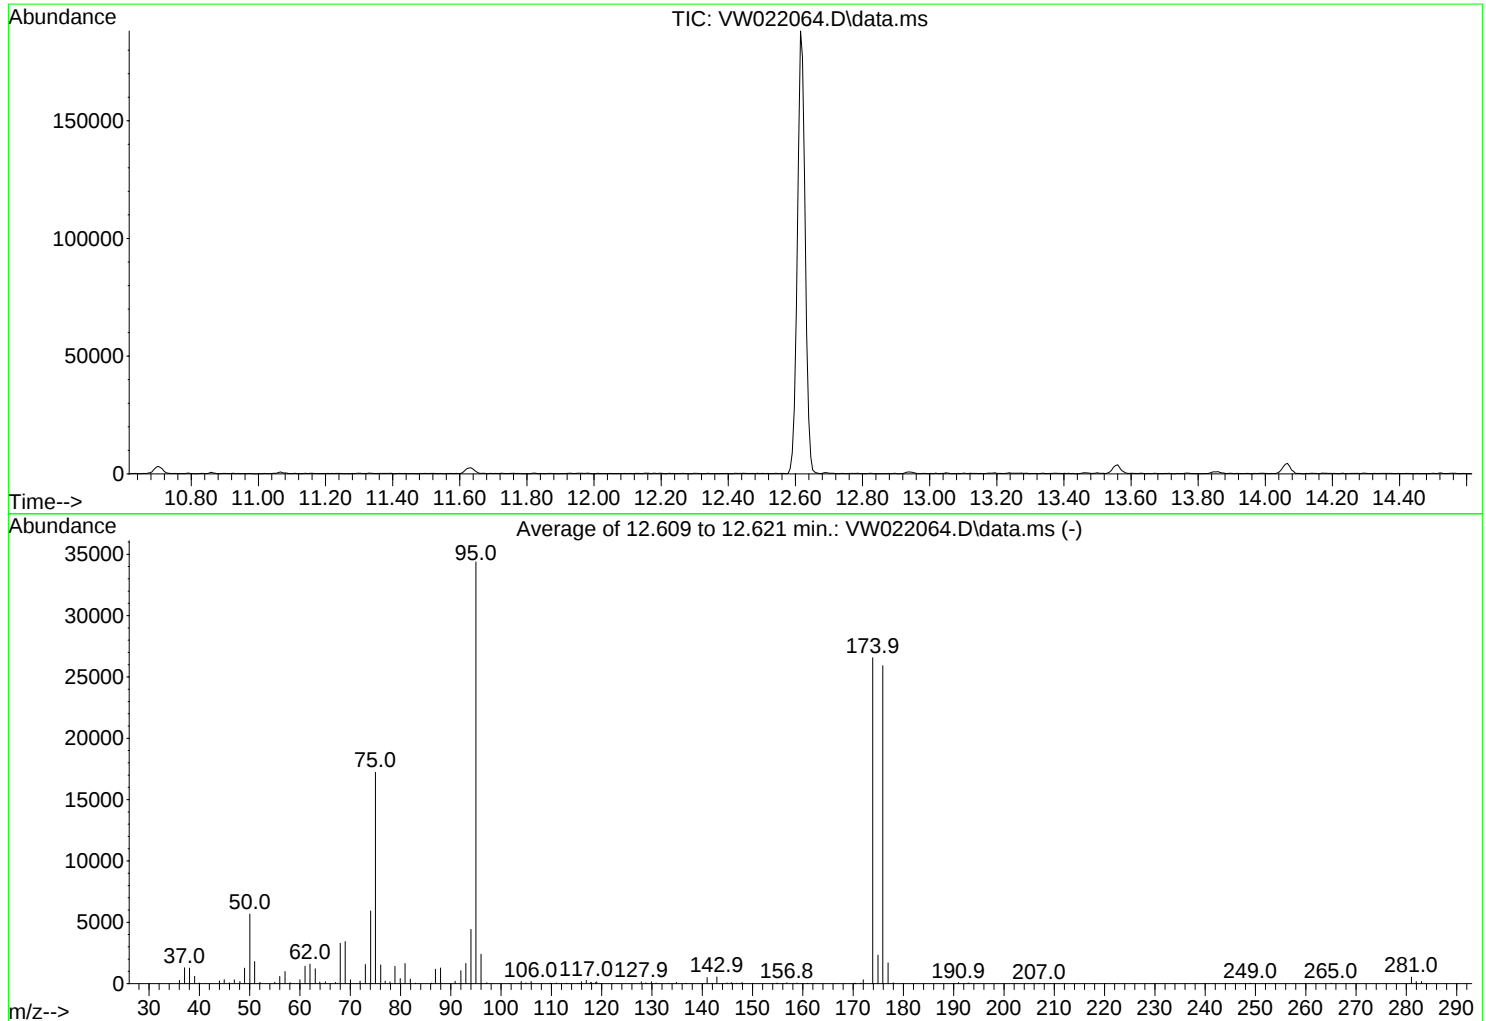

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	5677	PASS
75	95	30	80	50.1	17235	PASS
95	95	100	100	100.0	34387	PASS
96	95	5	9	7.0	2397	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.3	26576	PASS
175	174	5	9	8.7	2316	PASS
176	174	95	105	97.6	25925	PASS
177	176	5	10	6.5	1691	PASS

Scan 1749 (12.566 min): VW022064.D\data.ms
BFB508

m/z	Abundance
40.10	54.0
43.90	103.0
56.80	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB508

m/z	Abundance
36.00	228.0
37.00	1083.0
38.00	1200.0
39.10	524.0
39.90	86.0
44.00	284.0
45.00	314.0
46.00	69.0
47.00	362.0
48.00	171.0
49.00	1093.0
50.10	4978.0
51.00	1488.0
52.00	88.0
55.00	100.0
56.00	581.0
57.00	849.0
58.20	76.0
60.00	300.0
61.00	1366.0
62.00	1416.0
63.00	928.0
64.00	135.0
65.00	177.0
67.20	102.0
68.00	2636.0
69.00	2965.0
70.00	256.0
72.00	189.0
73.00	1322.0
74.10	4852.0
75.00	14890.0
76.10	1376.0
76.90	262.0
77.90	149.0
78.90	1126.0
79.90	356.0
80.90	1456.0
82.00	204.0
86.10	60.0
86.90	900.0
88.00	946.0
90.80	173.0
91.90	893.0
93.00	1319.0
94.00	3769.0
95.00	27504.0
96.00	2058.0
97.10	72.0
104.00	183.0
106.00	190.0
111.00	65.0
113.10	64.0
116.00	126.0
116.90	229.0
117.80	133.0
118.80	276.0
127.90	155.0
128.80	90.0
129.90	77.0
133.20	89.0
134.80	66.0
140.90	439.0
142.90	481.0
144.90	60.0
145.80	62.0
147.90	88.0
154.80	58.0
156.80	89.0
170.50	58.0
171.50	120.0
172.10	302.0
173.90	19992.0
174.90	1508.0
175.90	19296.0
176.90	1109.0
191.00	183.0
193.00	210.0
207.00	76.0
249.00	56.0
265.00	111.0
280.90	626.0
282.00	268.0
283.00	222.0

Instrument :
MSVOA_W
ClientSampleId :
BFB508

m/z	Abundance
36.00	273.0
37.00	1509.0
38.00	1372.0
39.00	727.0
40.20	87.0
44.00	296.0
45.00	398.0
46.00	61.0
46.90	307.0
48.10	194.0
49.00	1445.0
50.00	6204.0
51.00	2249.0
52.10	102.0
55.10	150.0
56.00	596.0
57.10	1126.0
58.00	77.0
60.00	317.0
61.00	1490.0
62.00	1651.0
63.10	1450.0
63.90	157.0
65.10	190.0
67.10	107.0
68.00	3848.0
69.00	3758.0
70.10	381.0
71.90	257.0
73.00	1680.0
74.00	6731.0
75.00	18872.0
76.00	1773.0
77.00	214.0
77.90	187.0
78.90	1674.0
80.00	452.0
80.90	1748.0
82.00	474.0
83.00	64.0
86.10	87.0
86.90	1419.0
88.00	1561.0
90.90	246.0
92.00	1215.0
93.00	1855.0
94.00	4818.0
95.00	39544.0
96.00	2773.0
97.20	64.0
104.00	183.0
105.00	97.0
105.90	191.0
109.80	69.0
111.00	96.0
113.00	53.0
115.20	50.0
115.90	191.0
117.00	304.0
118.00	244.0
119.00	266.0
128.00	189.0
128.70	54.0
130.00	158.0
130.80	59.0
134.80	110.0
136.60	76.0
140.90	546.0
142.90	594.0
144.90	70.0
145.70	112.0
146.80	63.0
147.90	129.0
150.00	76.0
154.80	80.0
156.90	66.0
158.80	60.0
160.90	78.0
170.40	78.0
172.00	274.0
173.90	30168.0
175.00	2644.0
175.90	29000.0
176.90	2125.0
178.00	70.0
190.90	113.0
192.70	92.0
249.00	58.0
281.00	638.0
282.00	161.0
283.00	203.0

Instrument :
MSVOA_W
ClientSampleId :
BFB508

m/z	Abundance
36.10	278.0
37.10	1284.0
38.10	1228.0
39.00	570.0
40.00	76.0
41.20	50.0
44.10	400.0
44.90	286.0
46.00	79.0
46.90	271.0
48.00	171.0
49.00	1256.0
50.10	5848.0
51.00	1651.0
52.00	112.0
54.90	116.0
56.00	597.0
57.00	1013.0
58.00	93.0
60.00	313.0
61.00	1419.0
62.00	1726.0
63.00	1270.0
64.00	111.0
65.00	122.0
67.00	104.0
68.00	3372.0
69.00	3584.0
70.00	310.0
72.00	180.0
73.00	1707.0
74.00	6172.0
75.00	17944.0
76.00	1430.0
76.90	165.0
77.90	100.0
78.90	1435.0
80.00	435.0
80.90	1718.0
81.90	405.0
83.00	65.0
87.00	1213.0
87.90	1328.0
90.80	168.0
92.10	1063.0
93.00	1754.0
94.00	4660.0
95.00	36112.0
96.00	2360.0
97.10	102.0
104.00	193.0
104.90	105.0
106.00	166.0
109.80	63.0
116.00	156.0
116.90	241.0
117.80	201.0
119.00	195.0
127.80	131.0
129.00	109.0
129.80	230.0
130.80	99.0
134.90	123.0
136.90	95.0
141.00	486.0
141.90	85.0
142.90	577.0
144.90	87.0
145.80	116.0
146.90	60.0
147.90	59.0
155.00	101.0
156.80	69.0
158.90	83.0
170.20	59.0
171.90	371.0
173.90	29568.0
175.00	2797.0
175.90	29480.0
177.00	1838.0
177.90	115.0
265.20	61.0
281.10	335.0
281.80	83.0
283.10	88.0

Instrument :
MSVOA_W
ClientSampleId :
BFB508