


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW020419\
Data File : VW008496.D
Acq On : 04 Feb 2019 09:32
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W012419S.M
Title : SW846 8260
Last Update : Fri Jan 25 11:07:41 2019

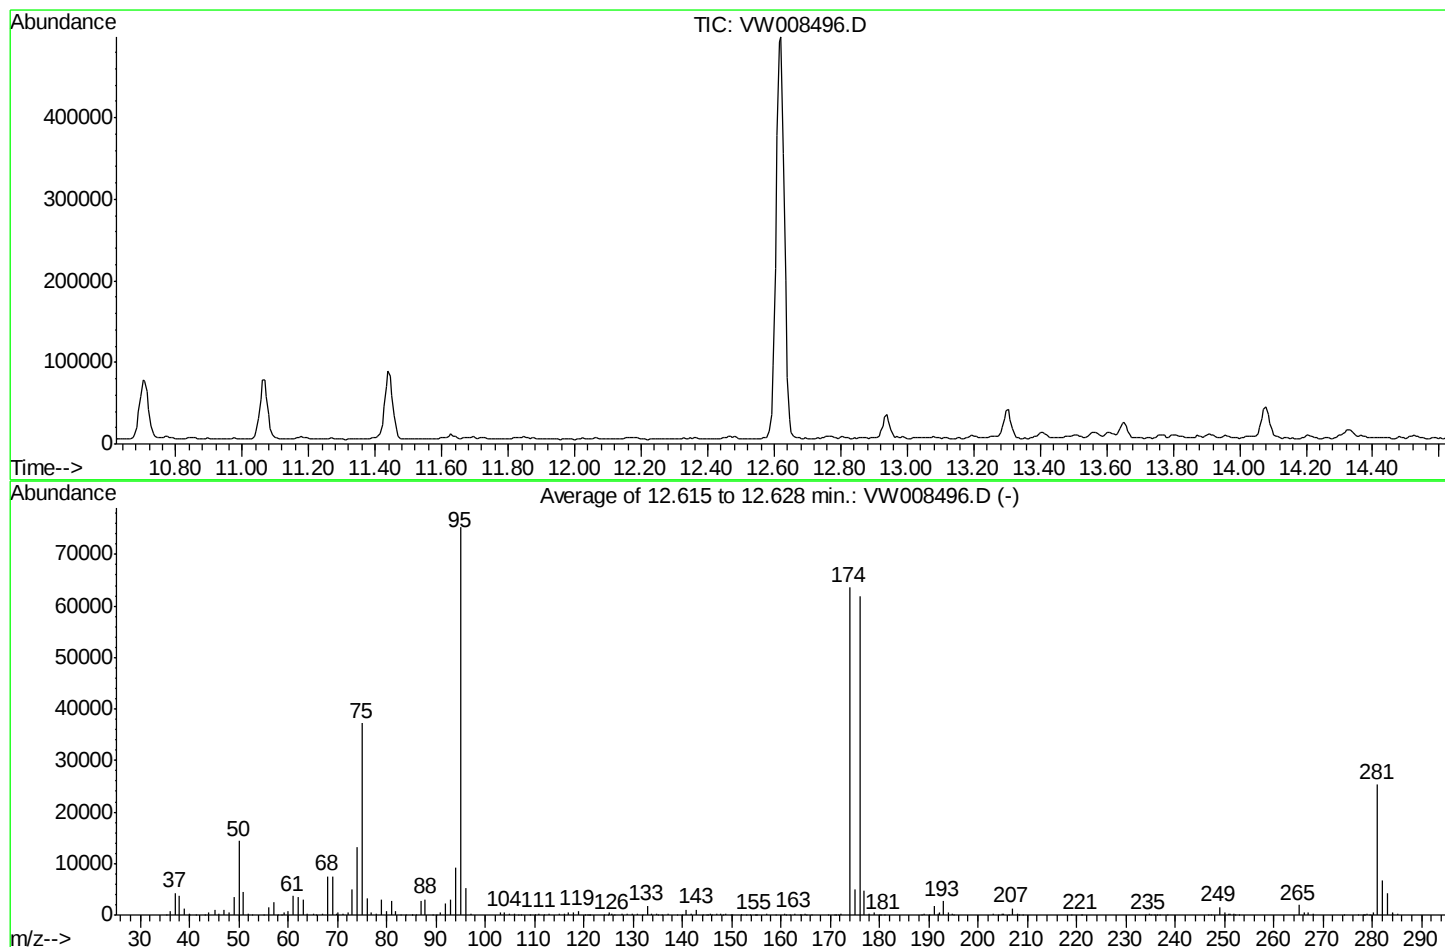

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	14369	PASS
75	95	30	60	49.5	37269	PASS
95	95	100	100	100.0	75269	PASS
96	95	5	9	6.9	5199	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.4	63546	PASS
175	174	5	9	7.9	5045	PASS
176	174	95	101	97.4	61877	PASS
177	176	5	9	7.7	4782	PASS