

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020624\
 Data File : VW027971.D
 Acq On : 06 Feb 2024 14:52
 Operator : SY/MD
 Sample : P1349-02
 Misc : 5.47g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH6W4

Quant Time: Feb 06 23:52:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 06 23:51:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	387550	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	337829	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	143801	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	83350	18.363	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.440%
7) Chloroethane-d5	2.905	69	74915	21.760	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.040%
11) 1,1-Dichloroethene-d2	4.021	65	37823	19.474	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.880%
21) 2-Butanone-d5	7.081	46	37042	52.521	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.040%
24) Chloroform-d	7.654	84	196035	21.633	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.520%
26) 1,2-Dichloroethane-d4	8.307	65	95178	23.256	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.040%
32) Benzene-d6	8.276	84	401785	22.229	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.920%
36) 1,2-Dichloropropane-d6	9.270	67	111868	22.827	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.320%
41) Toluene-d8	10.324	98	377579	21.833	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.320%
43) trans-1,3-Dichloroprop...	10.574	79	44521	22.090	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.360%
47) 2-Hexanone-d5	10.922	63	35062	52.598	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	90360	24.669	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.680%
66) 1,2-Dichlorobenzene-d4	13.854	152	116651	23.866	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.480%
Target Compounds						
16) Methylene chloride	4.917	84	12117	2.501	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020624\
Data File : VW027971.D
Acq On : 06 Feb 2024 14:52
Operator : SY/MD
Sample : P1349-02
Misc : 5.47g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH6W4


Quant Time: Feb 06 23:52:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 06 23:51:08 2024
Response via : Initial Calibration

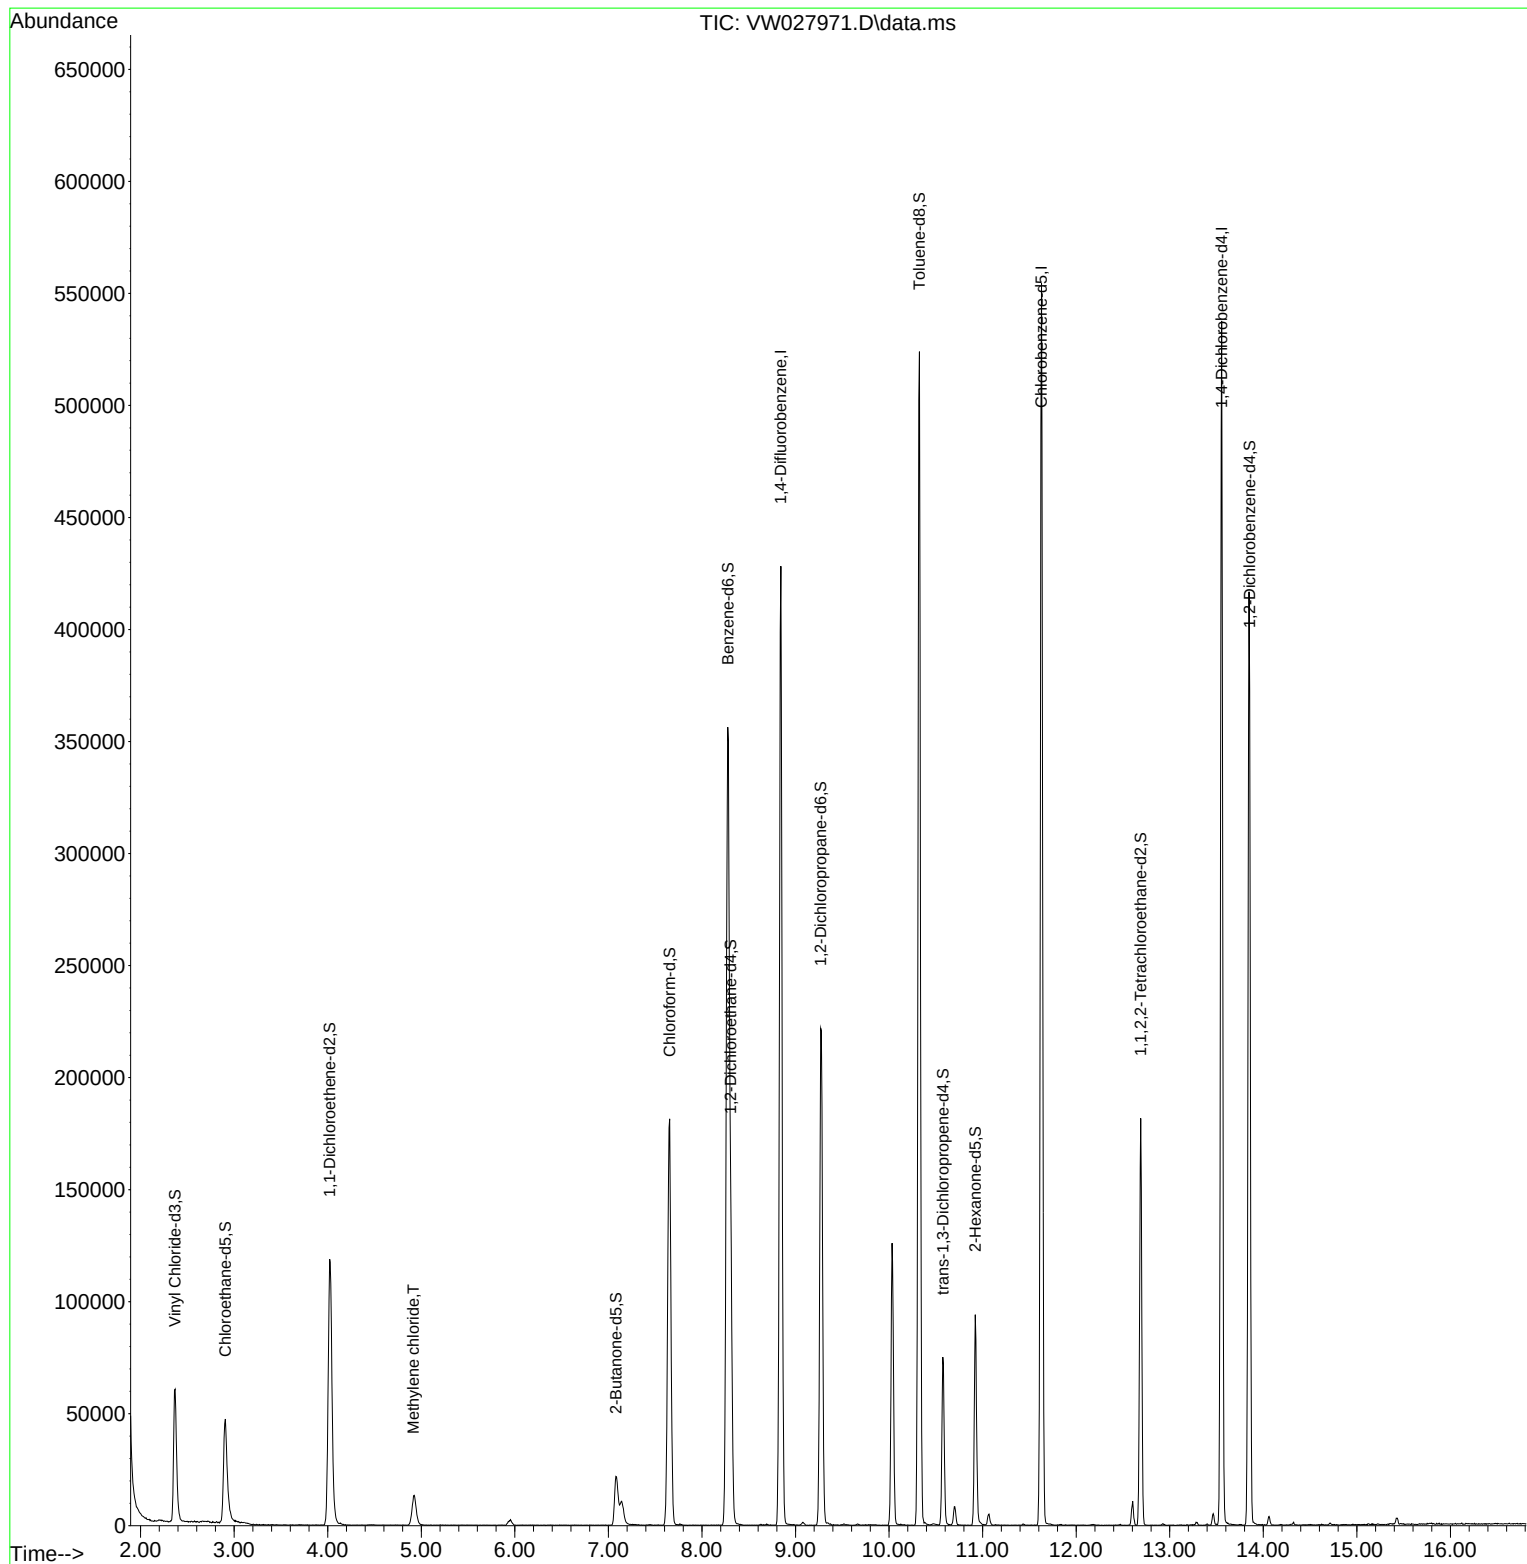

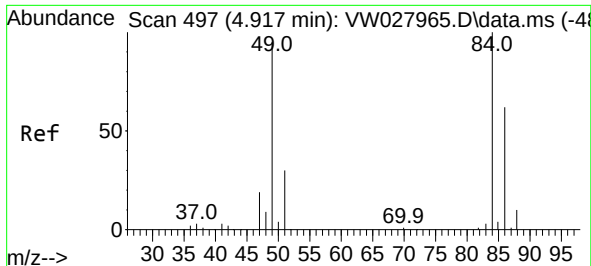

#16
Methylene chloride
Concen: 2.501 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW027971.D
Acq: 06 Feb 2024 14:52

Instrument :
MSVOA_W
ClientSampleId :
BH6W4

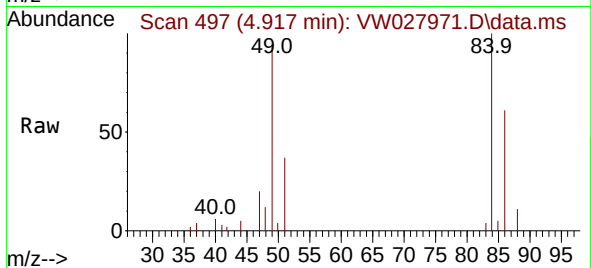

Tgt Ion: 84 Resp: 12117

Ion	Ratio	Lower	Upper
84	100		
86	60.7	45.4	84.4
49	94.3	66.3	123.1

