
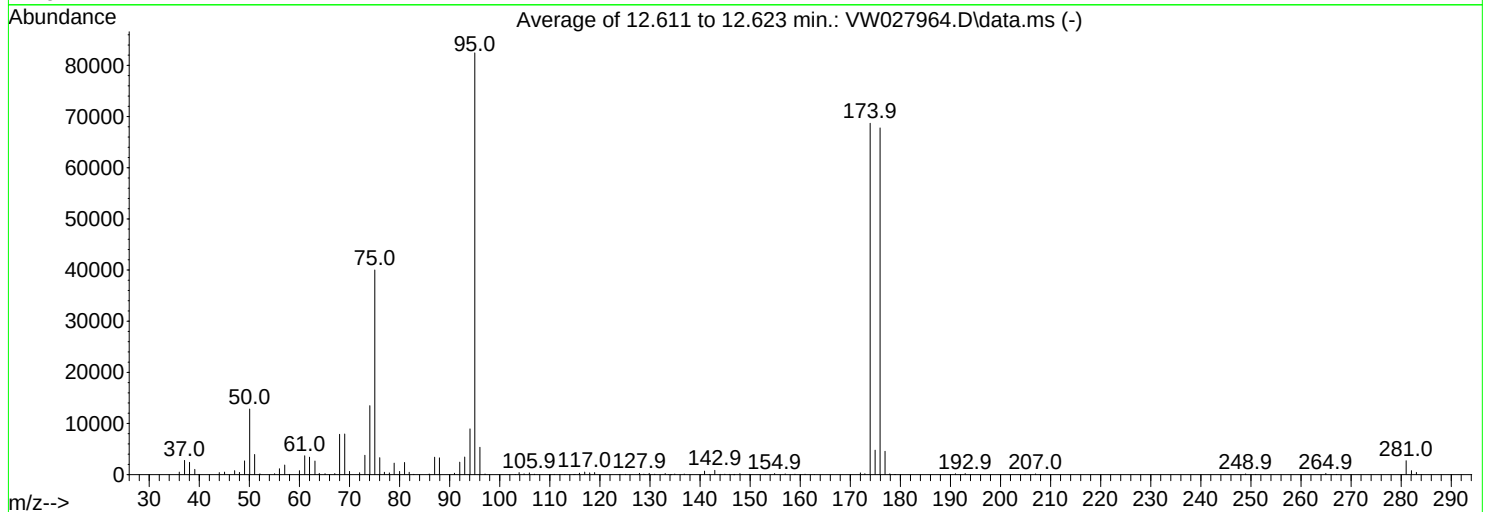


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020624\
Data File : VW027964.D
Acq On : 06 Feb 2024 08:43
Operator : SY/MD
Sample : BFB433
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB433

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Tue Feb 06 23:51:08 2024

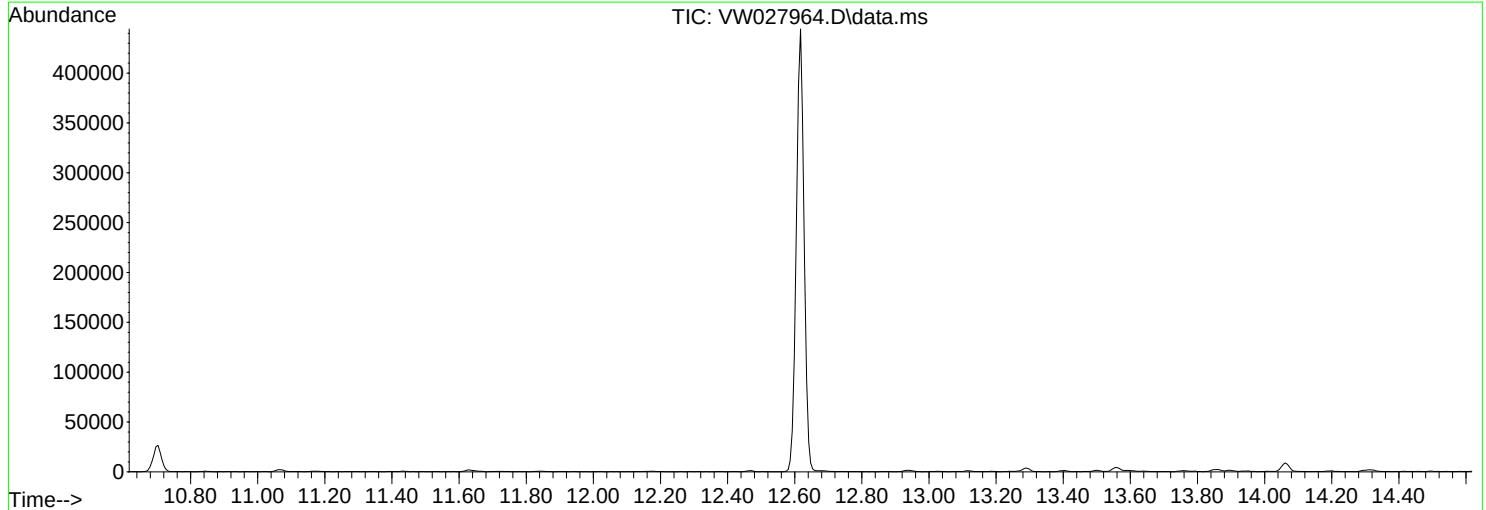

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	12825	PASS
75	95	30	80	48.5	39992	PASS
95	95	100	100	100.0	82459	PASS
96	95	5	9	6.5	5355	PASS
173	174	0.00	2	0.3	189	PASS
174	95	50	120	83.3	68680	PASS
175	174	5	9	7.0	4777	PASS
176	174	95	101	98.7	67771	PASS
177	176	5	9	6.8	4577	PASS

m/z	Abundance
40.00	132.0
43.90	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB433

m/z	Abundance
36.00	629.0
37.00	3120.0
38.10	2386.0
39.10	1104.0
40.00	204.0
44.00	529.0
45.10	592.0
47.00	736.0
48.00	383.0
49.10	3002.0
50.10	13357.0
51.10	4086.0
52.10	179.0
55.10	228.0
56.00	1188.0
57.00	1850.0
58.00	131.0
60.00	948.0
61.10	3702.0
62.00	3522.0
63.10	2638.0
63.90	305.0
65.10	192.0
67.10	182.0
68.00	7930.0
69.00	8120.0
70.00	675.0
72.00	384.0
73.00	3935.0
74.00	14092.0
75.10	40416.0
76.00	3475.0
77.00	407.0
77.90	258.0
78.90	2222.0
80.10	649.0
81.00	2369.0
81.90	551.0
82.90	83.0
86.00	137.0
87.00	3491.0
88.00	3120.0
91.00	304.0
92.00	2561.0
93.00	3698.0
94.00	8243.0
95.00	80384.0
96.10	5406.0
97.10	155.0
103.10	63.0
103.90	406.0
104.90	169.0
106.00	369.0
106.90	75.0
112.00	57.0
113.00	51.0
114.80	131.0
116.00	261.0
117.00	534.0
117.90	305.0
118.90	308.0
125.10	163.0
127.90	331.0
128.80	155.0
129.90	214.0
131.00	101.0
133.00	372.0
133.70	52.0
134.10	51.0
135.00	109.0
136.80	103.0
140.90	630.0
141.90	67.0
143.00	938.0
144.90	103.0
145.80	59.0
146.70	54.0
148.00	230.0
149.90	99.0
154.90	158.0
157.00	133.0
158.90	57.0
161.00	128.0
162.80	88.0
172.00	453.0
173.90	63440.0
175.00	4219.0
176.00	60744.0
177.00	4181.0
177.90	140.0
178.80	69.0
191.00	274.0

Instrument :
MSVOA_W
ClientSampleId :
BFB433

192.00	77.0
192.90	367.0
194.00	105.0
205.00	138.0
207.00	381.0
207.90	58.0
248.90	195.0
251.00	124.0
265.00	387.0
266.00	123.0
267.10	101.0
281.00	4031.0
282.10	1373.0
283.10	693.0
284.10	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB433

m/z	Abundance
36.00	530.0
37.00	2804.0
38.00	2784.0
39.10	1051.0
39.90	176.0
44.10	405.0
45.00	455.0
47.10	850.0
48.00	570.0
49.00	2653.0
50.00	14022.0
51.10	4440.0
52.10	100.0
55.00	216.0
56.00	1251.0
57.00	2197.0
58.00	103.0
60.00	797.0
61.00	4045.0
62.00	3811.0
63.10	2952.0
64.00	254.0
65.10	282.0
67.00	315.0
68.00	8578.0
69.10	8627.0
70.00	683.0
72.00	409.0
73.10	4048.0
74.10	14551.0
75.00	44608.0
76.10	3626.0
76.90	487.0
77.90	330.0
78.90	2609.0
80.00	654.0
81.00	2674.0
81.90	485.0
82.80	71.0
85.80	128.0
87.00	3688.0
88.00	3778.0
90.90	382.0
92.00	2691.0
93.00	3407.0
94.10	10110.0
95.00	93600.0
96.00	6172.0
97.00	150.0
103.90	404.0
104.80	158.0
105.80	332.0
106.90	91.0
109.90	57.0
110.90	103.0
112.00	63.0
115.00	113.0
115.80	347.0
116.90	491.0
118.00	406.0
118.90	564.0
124.00	75.0
125.20	59.0
127.80	223.0
128.80	171.0
129.90	292.0
130.90	56.0
133.10	162.0
133.70	80.0
134.90	149.0
136.90	109.0
140.90	800.0
141.90	80.0
142.90	807.0
144.00	53.0
145.00	120.0
145.80	77.0
146.90	102.0
147.90	209.0
149.80	88.0
153.00	59.0
154.80	274.0
156.90	174.0
158.90	112.0
160.90	112.0
172.00	372.0
174.00	75240.0
175.00	5119.0
175.90	81296.0
176.90	5450.0
177.90	213.0
179.00	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB433

191.00	219.0
193.00	196.0
204.80	93.0
207.00	132.0
249.00	248.0
250.90	78.0
264.90	218.0
267.10	52.0
281.00	3016.0
282.00	679.0
283.00	372.0

Instrument :
MSVOA_W
ClientSampleId :
BFB433

m/z	Abundance
35.90	368.0
37.10	2404.0
38.00	2071.0
39.10	981.0
39.90	199.0
44.00	407.0
45.00	491.0
47.10	748.0
48.00	366.0
49.00	2403.0
50.00	11095.0
51.00	3258.0
52.10	199.0
55.10	174.0
56.00	1009.0
57.10	1625.0
60.00	638.0
61.00	3332.0
62.00	2883.0
63.10	2397.0
64.00	182.0
65.00	115.0
67.00	150.0
68.00	7141.0
69.00	7053.0
70.00	523.0
72.00	361.0
73.00	3387.0
74.00	11809.0
75.00	34952.0
76.10	2904.0
76.90	534.0
78.00	420.0
78.90	1922.0
79.90	553.0
81.00	2126.0
81.90	416.0
85.90	78.0
87.00	3090.0
87.90	3001.0
90.90	198.0
92.00	2112.0
93.00	3231.0
94.00	8502.0
95.00	73392.0
96.00	4488.0
97.00	119.0
103.80	365.0
104.80	126.0
105.90	369.0
106.90	99.0
110.80	64.0
113.00	55.0
115.00	50.0
115.90	279.0
116.90	502.0
118.00	291.0
119.00	340.0
124.00	70.0
128.00	235.0
129.00	124.0
129.80	213.0
130.90	146.0
133.00	130.0
135.00	115.0
136.80	131.0
140.90	643.0
141.90	73.0
142.90	811.0
144.00	98.0
145.00	88.0
145.90	74.0
146.90	96.0
147.90	171.0
155.00	193.0
157.10	146.0
159.00	105.0
160.90	67.0
172.00	261.0
172.90	568.0
174.00	67360.0
174.90	4993.0
175.90	61272.0
176.90	4101.0
177.90	83.0
191.00	111.0
193.00	84.0
265.00	131.0
281.10	1135.0
282.00	305.0
283.10	223.0

Instrument :
MSVOA_W
ClientSampleId :
BFB433