

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020821\
 Data File : VW018045.D
 Acq On : 08 Feb 2021 10:58
 Operator : SY/VA
 Sample : VW0208SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK02

Manual Integrations
 APPROVED

MMDadoda
 2/9/2021 4:33:17 PM

Quant Time: Feb 09 03:24:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 09 03:23:41 2021
 Response via : Initial Calibration

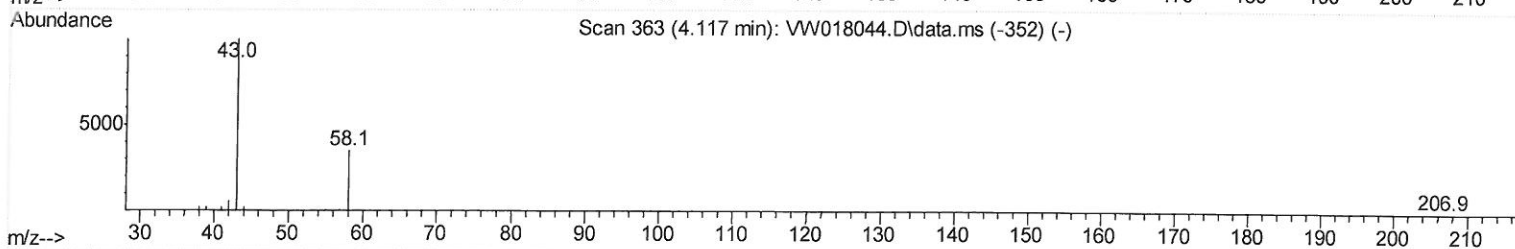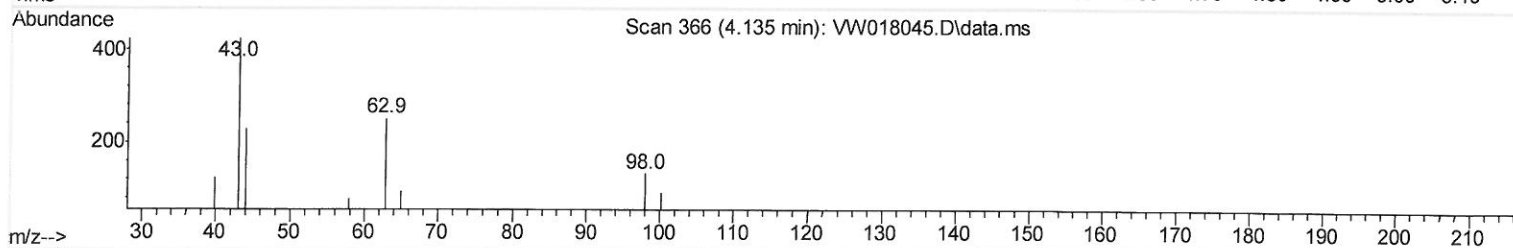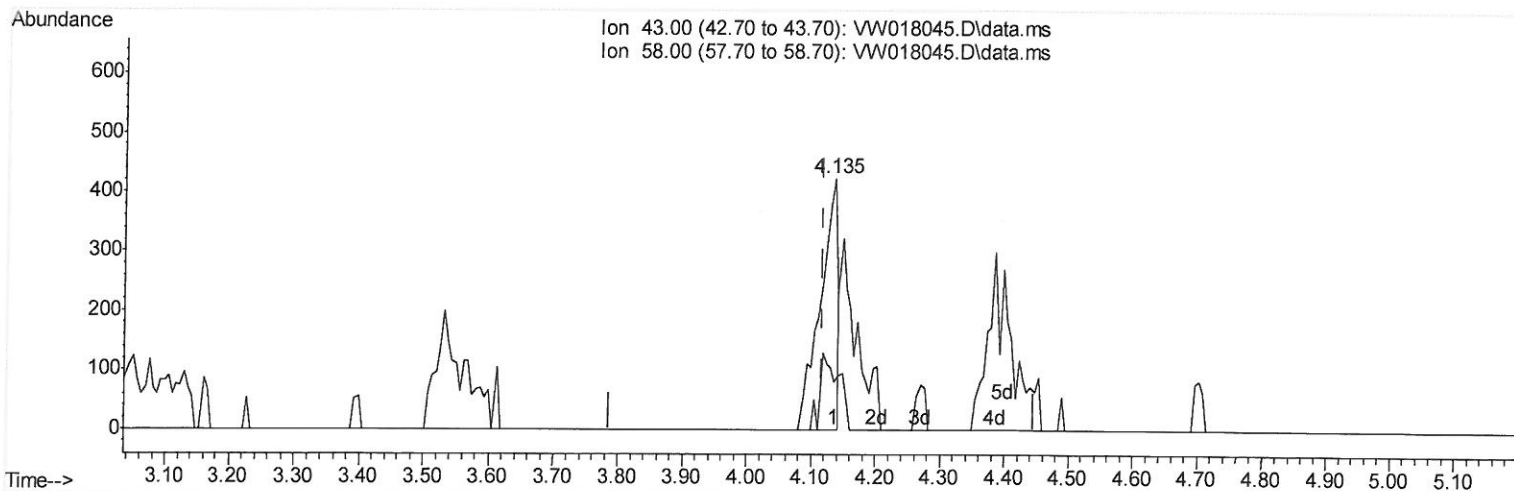

TIC: VW018045.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 0.80 ug/L

response 815

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.20	10.67
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020821\
Data File : VW018045.D
Acq On : 08 Feb 2021 10:58
Operator : SY/VA
Sample : VW0208SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK02

Manual Integrations
APPROVED

MMDadoda
2/9/2021 4:33:17 PM

Quant Time: Feb 09 03:24:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 09 03:23:41 2021
Response via : Initial Calibration

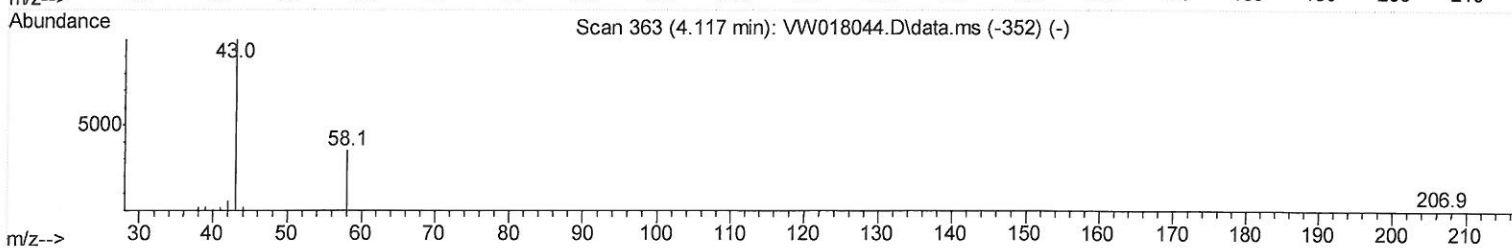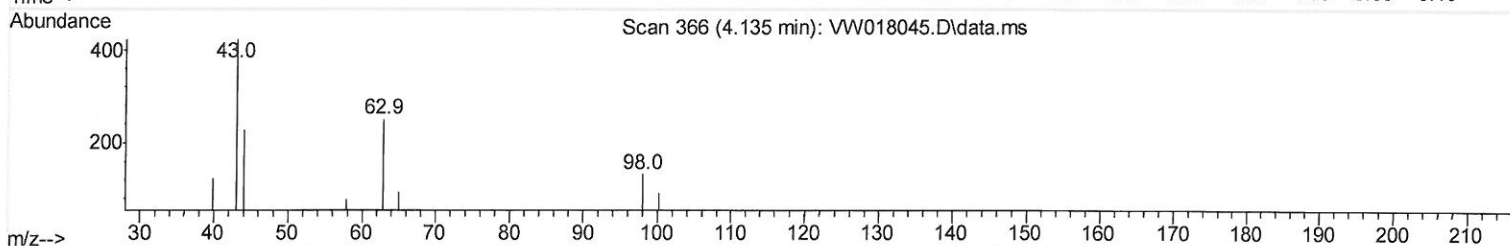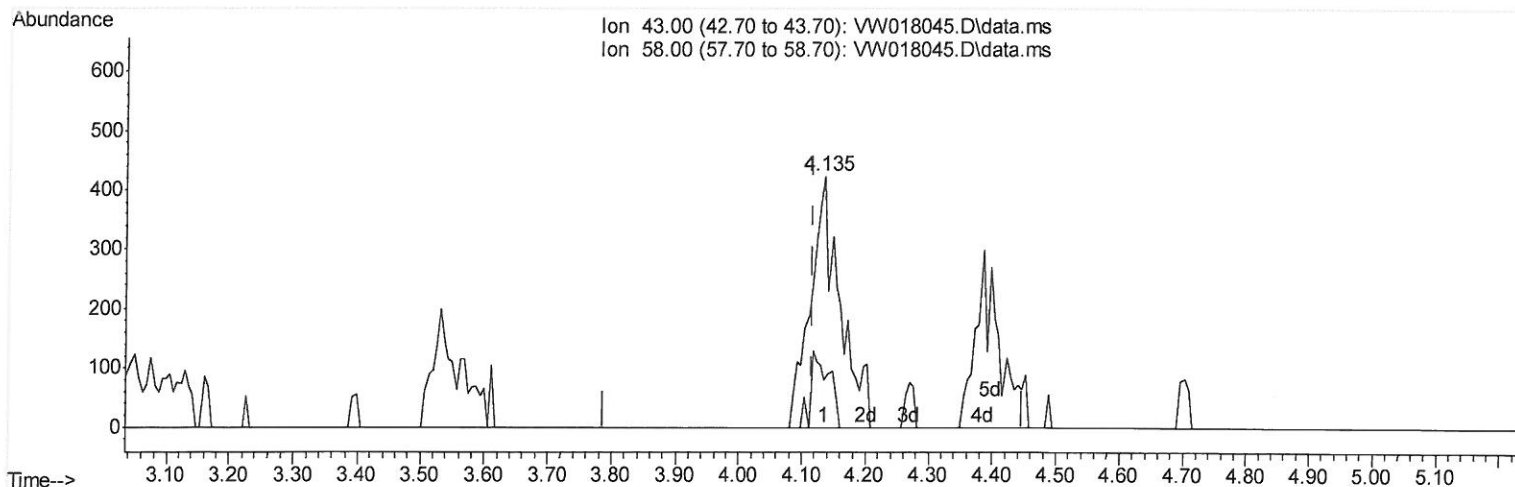

TIC: VW018045.D\data.ms

(13) Acetone (T)

4.135min (+ 0.018) 1.34 ug/L m

response 1370

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.20	6.35
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020821\
 Data File : VW018045.D
 Acq On : 08 Feb 2021 10:58
 Operator : SY/VA
 Sample : VW0208SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK02

Manual Integrations
 APPROVED

MMDadoda
 2/9/2021 4:33:17 PM

Quant Time: Feb 09 03:24:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 09 03:23:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	416629	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	369628	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	191954	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	101368	19.58	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	78.32%		
7) Chloroethane-d5	2.898	69	82928	20.18	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	80.72%		
10) 1,1-Dichloroethene-d2	4.025	63	162949	15.74	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	62.96%		
20) 2-Butanone-d5	7.080	46	47476	34.36	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	68.72%		
24) Chloroform-d	7.647	84	232902	21.30	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	85.20%		
26) 1,2-Dichloroethane-d4	8.305	65	118788	20.40	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	81.60%		
29) Benzene-d6	8.275	84	476717	23.49	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	93.96%		
33) 1,2-Dichloropropane-d6	9.274	67	128276	22.60	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	90.40%		
37) Toluene-d8	10.323	98	451827	23.40	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	93.60%		
38) trans-1,3-Dichloroprop...	10.579	79	56949	22.13	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	88.52%		
39) 2-Hexanone-d5	10.927	63	38763	35.72	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	71.44%		
48) 1,1,2,2-Tetrachloroeth...	12.695	84	97396	19.53	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	78.12%		
61) 1,2-Dichlorobenzene-d4	13.853	152	162825	23.78	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	95.12%		
Target Compounds						
13) Acetone	4.135	43	1370m	1.34	ug/L	Qvalue 82/10/21 Sy
16) Methylene chloride	4.928	84	5687	0.85	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020821\
Data File : VW018045.D
Acq On : 08 Feb 2021 10:58
Operator : SY/VA
Sample : VW0208SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK02

Manual Integrations
APPROVED

MMDadoda
2/9/2021 4:33:17 PM

Quant Time: Feb 09 03:24:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 09 03:23:41 2021
Response via : Initial Calibration

