

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020823\
 Data File : VW025311.D
 Acq On : 08 Feb 2023 10:05
 Operator : SY/MD
 Sample : VW0208SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK461

Quant Time: Feb 09 00:27:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 07 20:11:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	296251	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	263644	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	129336	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.367	65	54368	18.965	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.840%		
7) Chloroethane-d5	2.898	69	45923	18.041	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.160%		
11) 1,1-Dichloroethene-d2	4.019	63	119588	15.044	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	60.160%		
21) 2-Butanone-d5	7.080	46	33109	44.489	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.980%		
24) Chloroform-d	7.647	84	176461	22.726	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.920%		
26) 1,2-Dichloroethane-d4	8.305	65	97440	25.762	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.040%		
32) Benzene-d6	8.269	84	332082	20.782	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.120%		
36) 1,2-Dichloropropane-d6	9.274	67	94416	20.195	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	80.760%		
41) Toluene-d8	10.323	98	311252	21.791	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	87.160%		
43) trans-1,3-Dichloroprop...	10.579	79	40619	23.251	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	93.000%		
47) 2-Hexanone-d5	10.921	63	26384	50.332	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.660%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	68310	21.485	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.960%		
66) 1,2-Dichlorobenzene-d4	13.847	152	102305	22.799	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.200%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	9.274	63	12107	2.691	ug/L	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020823\
Data File : VW025311.D
Acq On : 08 Feb 2023 10:05
Operator : SY/MD
Sample : VW0208SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK461

Quant Time: Feb 09 00:27:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 07 20:11:22 2023
Response via : Initial Calibration

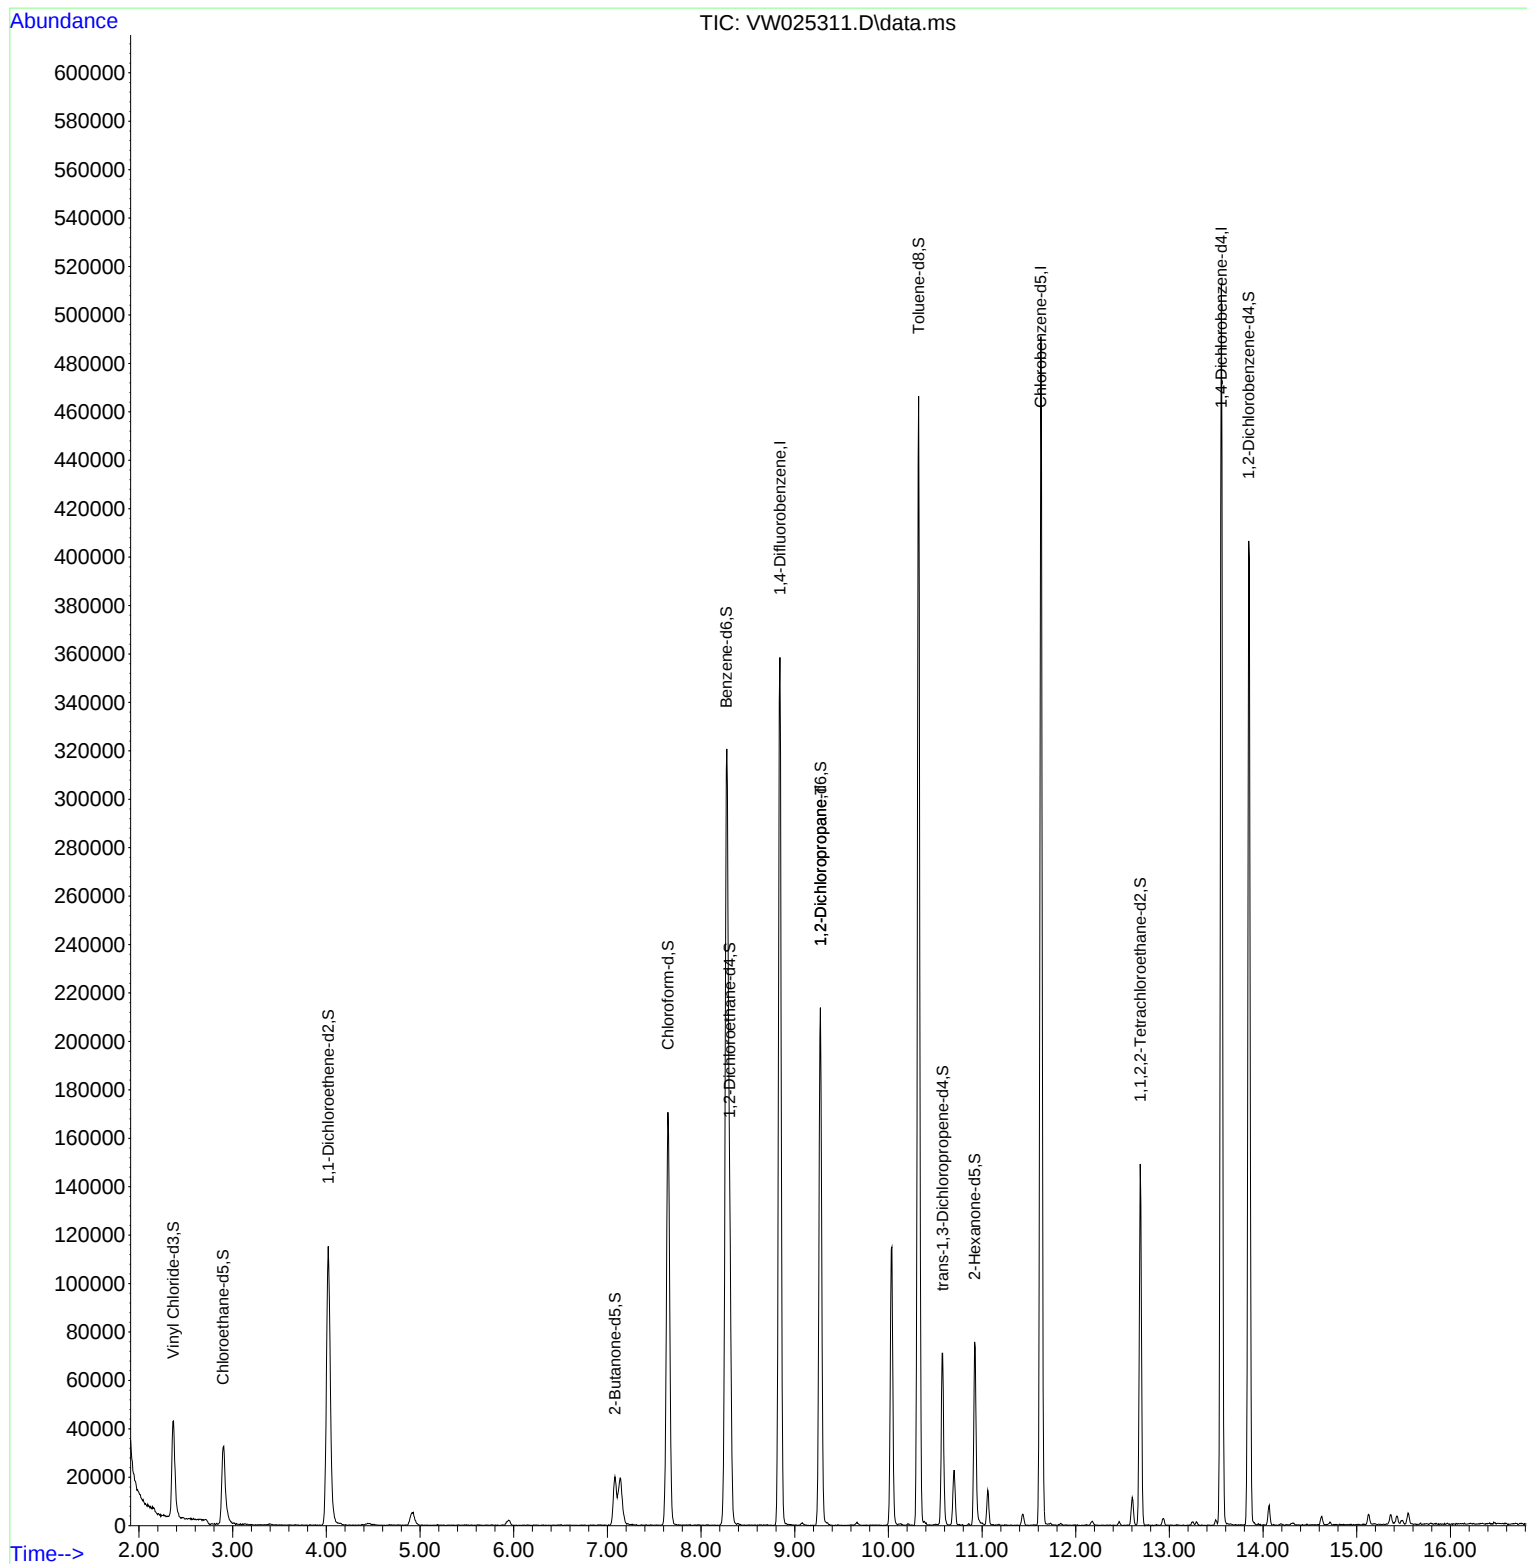

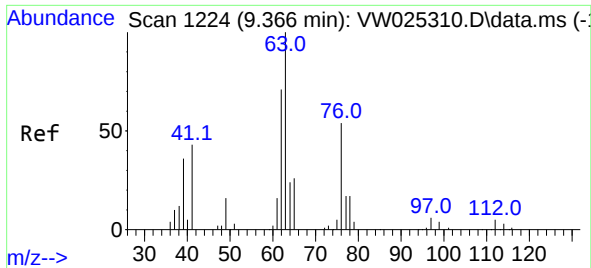

#37
1,2-Dichloropropane
Concen: 2.691 ug/L
RT: 9.274 min Scan# 11
Delta R.T. -0.091 min
Lab File: VW025311.D
Acq: 08 Feb 2023 10:05

Instrument :
MSVOA_W
ClientSampleId :
VBLK461

Tgt Ion: 63 Resp: 12107
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.8#

