

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020823\
 Data File : VW025312.D
 Acq On : 08 Feb 2023 11:38
 Operator : SY/MD
 Sample : 01422-15
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Feb 09 00:27:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Feb 07 20:11:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	286181	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	251337	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	119531	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	55498	20.040	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.160%
7) Chloroethane-d5	2.898	69	48585	19.759	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.040%
11) 1,1-Dichloroethene-d2	4.019	63	122750	15.985	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.960%
21) 2-Butanone-d5	7.171	46	305	0.424	ug/L	0.09
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.840%#
24) Chloroform-d	7.647	84	177738	23.696	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	8.305	65	95400	26.110	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.440%
32) Benzene-d6	8.275	84	334160	21.936	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.760%
36) 1,2-Dichloropropane-d6	9.275	67	93990	21.088	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.360%
41) Toluene-d8	10.323	98	314256	23.079	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.320%
43) trans-1,3-Dichloroprop...	10.579	79	40030	24.036	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.160%
47) 2-Hexanone-d5	10.921	63	25166	50.359	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.720%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	66742	22.020	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.080%
66) 1,2-Dichlorobenzene-d4	13.847	152	103794	25.028	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.120%
Target Compounds						
					Qvalue	
34) Trichloroethene	8.842	95	9740	1.999	ug/L #	5
37) 1,2-Dichloropropane	9.275	63	12237	2.853	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020823\
Data File : VW025312.D
Acq On : 08 Feb 2023 11:38
Operator : SY/MD
Sample : 01422-15
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Feb 09 00:27:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 07 20:11:22 2023
Response via : Initial Calibration

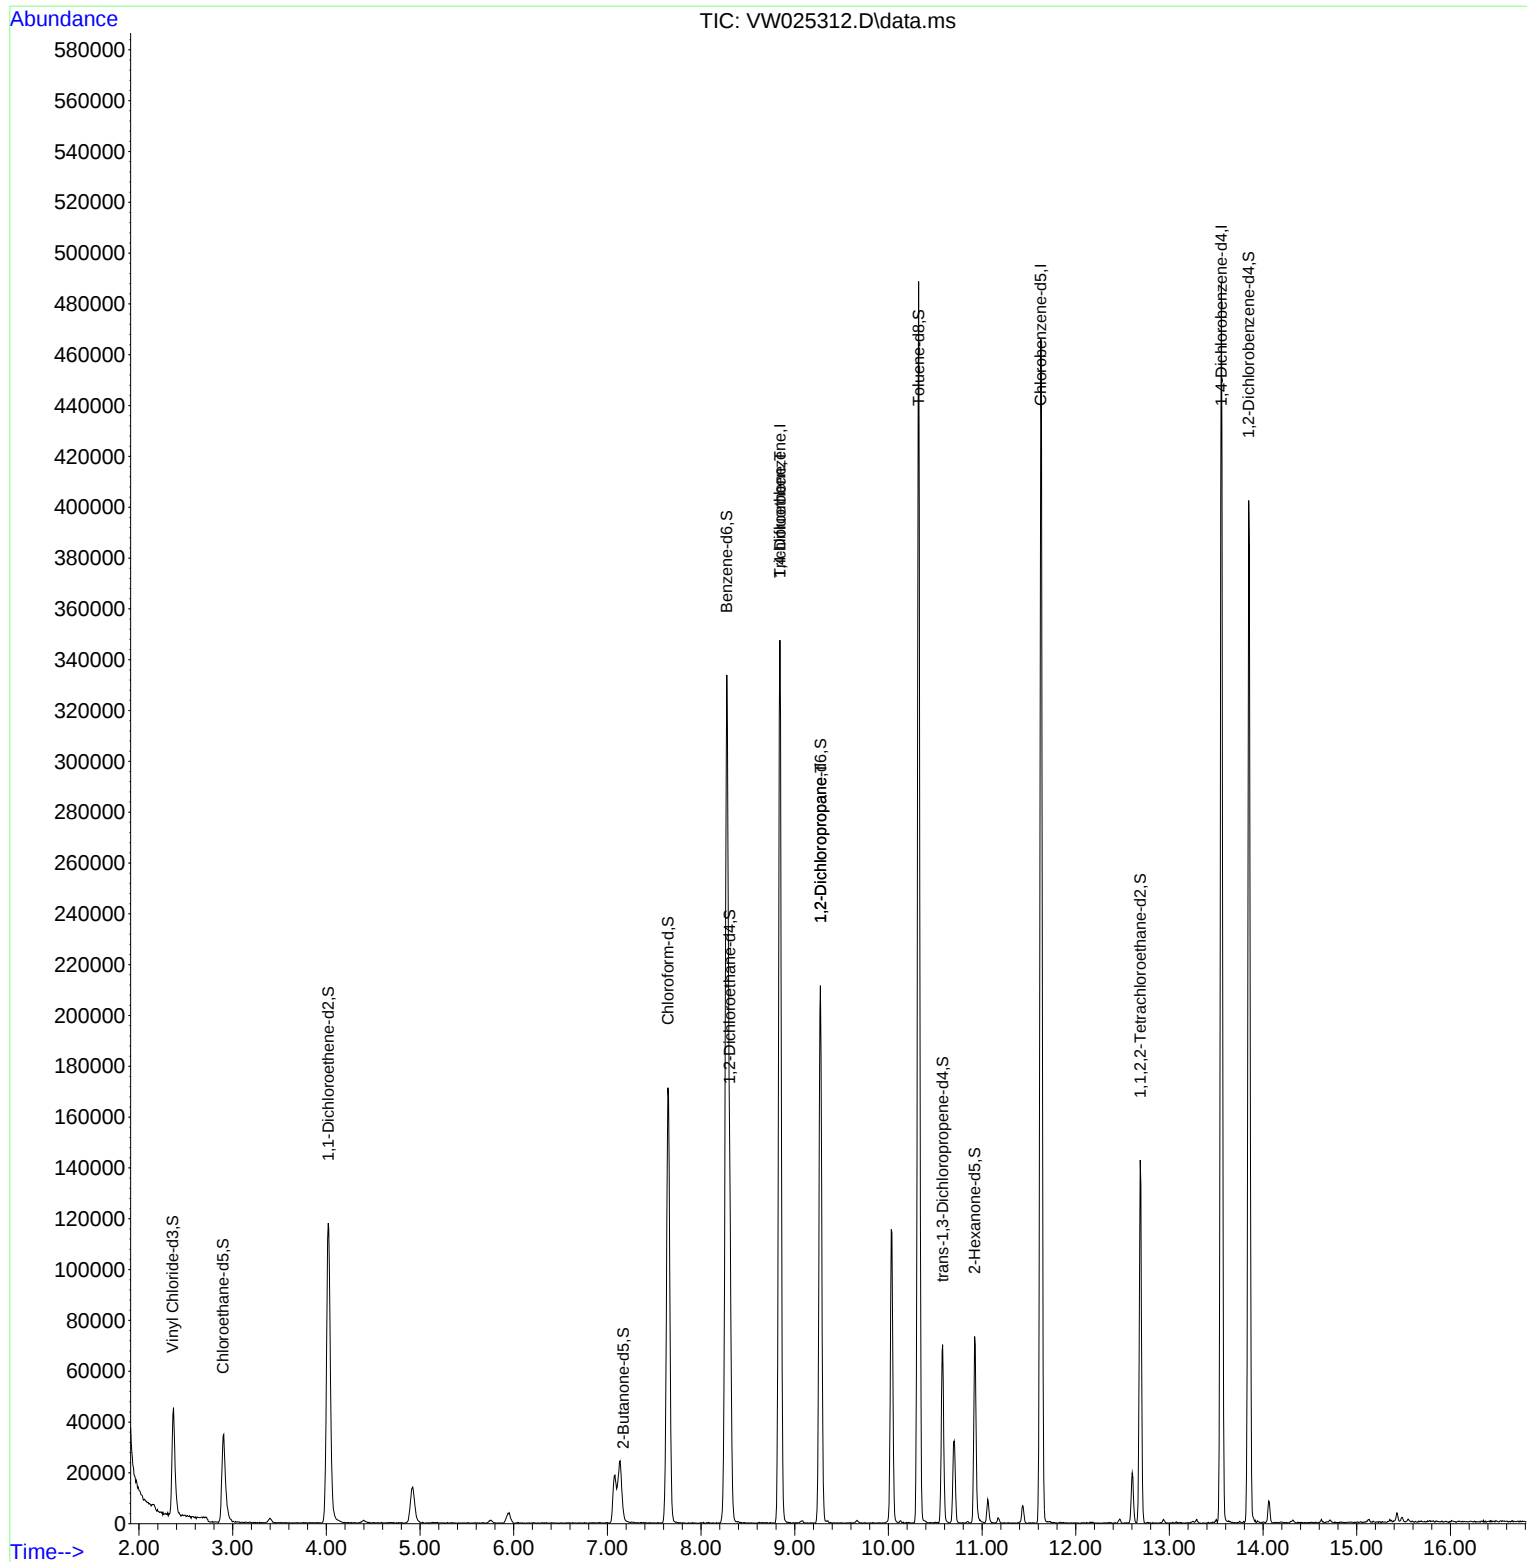




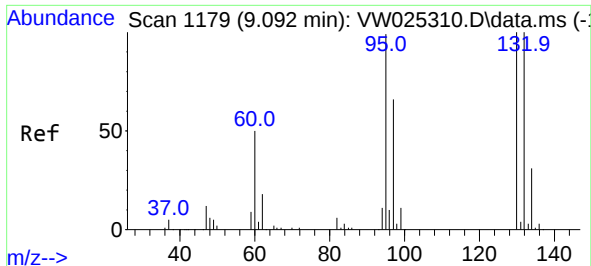


#34
Trichloroethene
Concen: 1.999 ug/L
RT: 8.842 min Scan# 1179
Delta R.T. -0.250 min
Lab File: VW025312.D
Acq: 08 Feb 2023 11:38

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Tgt Ion: 95 Resp: 9740

Ion	Ratio	Lower	Upper
95	100		
97	0.0	45.4	84.2#
132	0.0	67.1	124.5#
130	0.0	69.2	128.6#

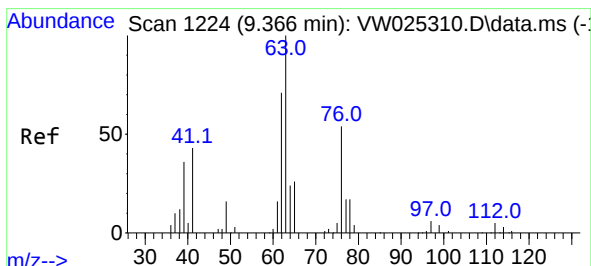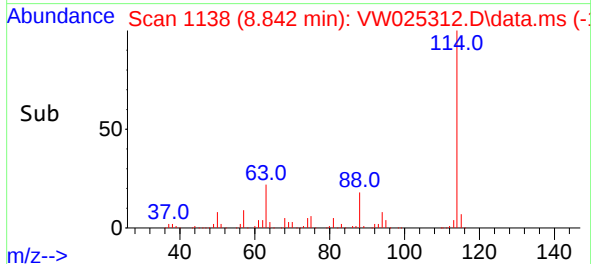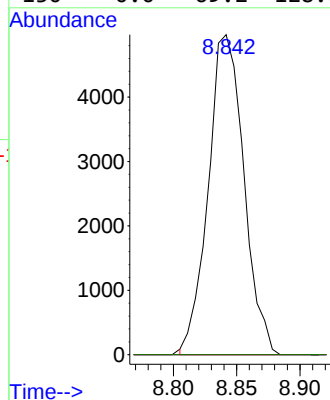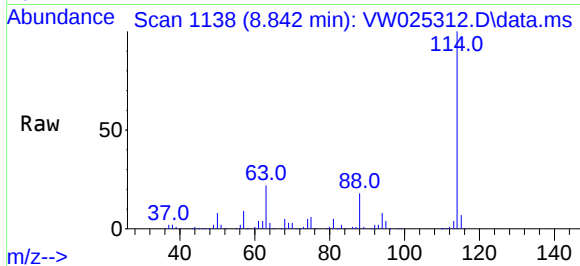

#37
1,2-Dichloropropane
Concen: 2.853 ug/L
RT: 9.275 min Scan# 1209
Delta R.T. -0.091 min
Lab File: VW025312.D
Acq: 08 Feb 2023 11:38

Tgt Ion: 63 Resp: 12237

Ion	Ratio	Lower	Upper
63	100		
112	0.0	3.8	5.8#

