
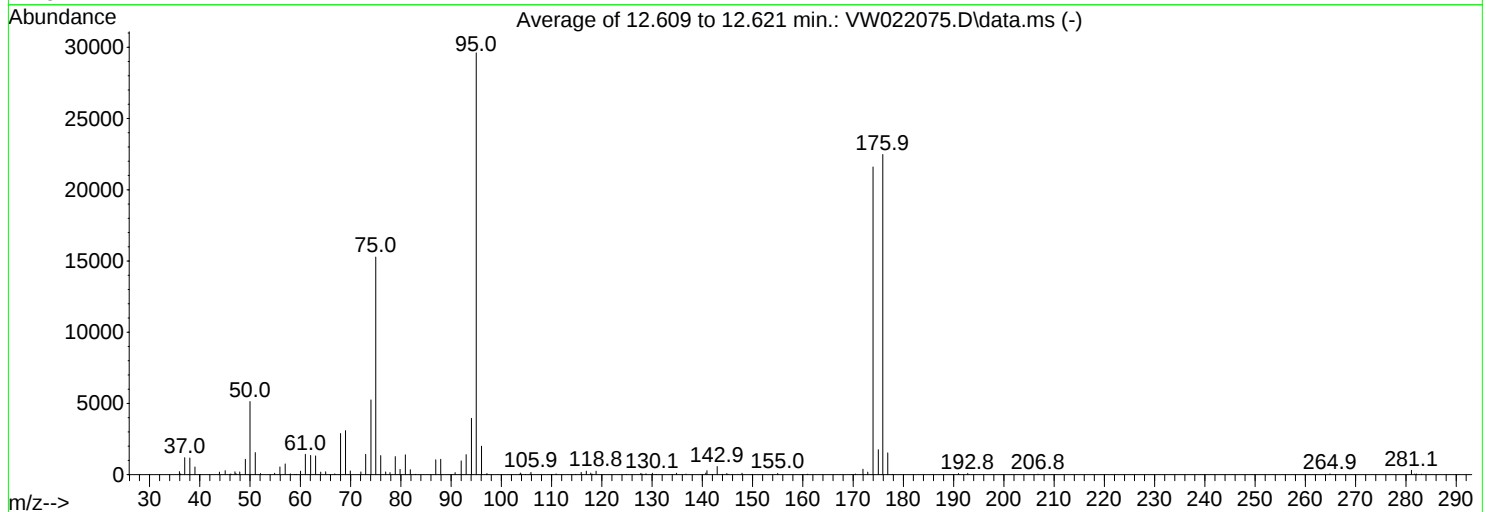


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020922\
 Data File : VW022075.D
 Acq On : 09 Feb 2022 08:13
 Operator : SY/VA
 Sample : BFB509
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB509

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
 Title : SFAM01.0
 Last Update : Thu Feb 03 01:57:48 2022

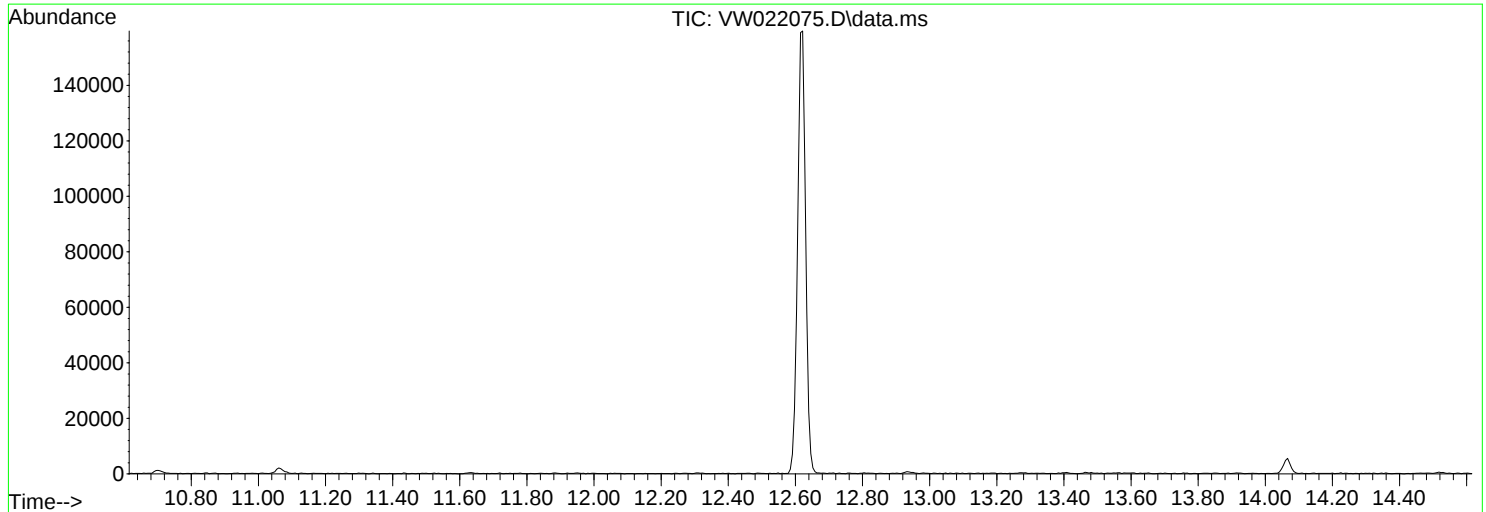

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	5131	PASS
75	95	30	80	51.6	15276	PASS
95	95	100	100	100.0	29611	PASS
96	95	5	9	6.7	1998	PASS
173	174	0.00	2	0.9	184	PASS
174	95	50	120	73.0	21605	PASS
175	174	5	9	8.1	1749	PASS
176	174	95	105	104.0	22472	PASS
177	176	5	10	6.8	1530	PASS

m/z	Abundance
40.10	91.0
43.80	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB509

m/z	Abundance
35.90	173.0
36.20	160.0
37.00	978.0
38.00	958.0
39.10	500.0
40.00	98.0
43.90	242.0
45.10	244.0
47.00	256.0
47.90	171.0
49.00	829.0
50.00	4264.0
51.00	1116.0
55.00	89.0
55.90	413.0
57.00	608.0
58.00	118.0
59.20	59.0
60.00	217.0
61.00	1221.0
62.10	1214.0
63.00	1194.0
64.00	150.0
65.00	139.0
66.80	57.0
68.00	2228.0
69.00	2276.0
69.90	226.0
72.10	193.0
73.00	1131.0
74.00	4211.0
75.00	12464.0
76.00	1135.0
76.90	124.0
77.90	158.0
78.90	1083.0
79.90	305.0
80.90	1156.0
81.90	320.0
82.90	73.0
86.90	963.0
87.90	680.0
90.80	132.0
92.00	669.0
93.00	1049.0
94.10	3142.0
95.00	24104.0
96.00	1869.0
97.00	58.0
103.70	143.0
105.70	117.0
115.90	153.0
116.90	256.0
118.10	113.0
118.80	216.0
127.80	88.0
130.20	54.0
134.90	105.0
136.80	59.0
140.70	355.0
142.90	387.0
145.10	115.0
148.00	82.0
155.00	72.0
171.90	307.0
173.90	16880.0
175.00	1230.0
175.90	15456.0
176.90	1120.0
191.00	107.0
192.80	84.0
206.80	95.0
264.90	98.0
281.10	389.0
282.10	145.0
283.10	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB509

m/z	Abundance
35.90	209.0
37.00	1338.0
38.00	1246.0
39.00	629.0
40.00	123.0
44.00	319.0
45.00	322.0
46.00	90.0
47.20	233.0
48.00	194.0
49.10	1200.0
50.00	5708.0
51.10	1679.0
52.10	116.0
54.90	101.0
55.90	562.0
57.00	904.0
58.00	62.0
58.90	55.0
60.00	277.0
61.00	1598.0
62.00	1488.0
63.00	1447.0
64.00	147.0
65.10	254.0
66.90	128.0
68.00	3390.0
69.00	3439.0
70.00	247.0
72.10	184.0
73.00	1682.0
74.10	5993.0
75.00	17016.0
76.00	1432.0
77.00	194.0
77.80	136.0
78.90	1397.0
79.90	424.0
80.90	1449.0
81.90	375.0
87.00	1087.0
88.00	1302.0
90.80	202.0
92.00	959.0
93.00	1526.0
94.00	4589.0
95.00	32416.0
96.10	2097.0
97.20	113.0
103.90	173.0
105.90	248.0
110.90	87.0
115.90	122.0
116.90	241.0
117.80	135.0
118.80	268.0
124.90	65.0
128.00	151.0
128.80	127.0
130.00	156.0
134.90	121.0
136.70	71.0
140.90	444.0
143.00	555.0
144.80	88.0
147.90	128.0
149.90	55.0
155.00	107.0
170.50	63.0
171.90	544.0
174.00	24056.0
175.00	2040.0
175.90	24368.0
176.90	1783.0
190.90	52.0
192.80	174.0
264.90	68.0
281.00	322.0
281.80	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB509

m/z	Abundance
36.00	268.0
37.00	1243.0
38.00	1286.0
39.00	489.0
40.10	94.0
43.90	253.0
45.00	292.0
46.20	121.0
47.00	361.0
48.00	206.0
49.00	1216.0
50.00	5421.0
51.00	1843.0
52.10	108.0
54.80	102.0
56.00	657.0
57.00	754.0
60.10	265.0
61.00	1447.0
62.00	1358.0
63.10	1311.0
64.10	238.0
65.00	224.0
68.00	3041.0
69.00	3553.0
70.00	314.0
72.00	203.0
73.00	1482.0
74.00	5545.0
75.00	16349.0
76.00	1452.0
77.10	244.0
77.90	136.0
78.90	1338.0
79.80	399.0
80.90	1572.0
81.90	336.0
87.00	1071.0
87.90	1240.0
90.90	105.0
92.00	1266.0
93.00	1654.0
94.00	4139.0
95.00	32312.0
96.00	2027.0
97.10	110.0
103.80	174.0
104.80	59.0
105.90	234.0
110.90	88.0
114.80	53.0
115.90	185.0
116.90	246.0
117.80	209.0
118.90	263.0
127.70	166.0
128.80	75.0
130.00	108.0
130.80	83.0
134.80	96.0
140.90	409.0
142.90	790.0
144.00	53.0
144.90	143.0
147.80	82.0
155.00	93.0
160.90	108.0
170.50	64.0
172.00	288.0
172.90	551.0
173.90	23880.0
175.00	1977.0
175.90	27592.0
176.90	1688.0
177.80	54.0
190.90	64.0
281.20	189.0
281.70	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB509