
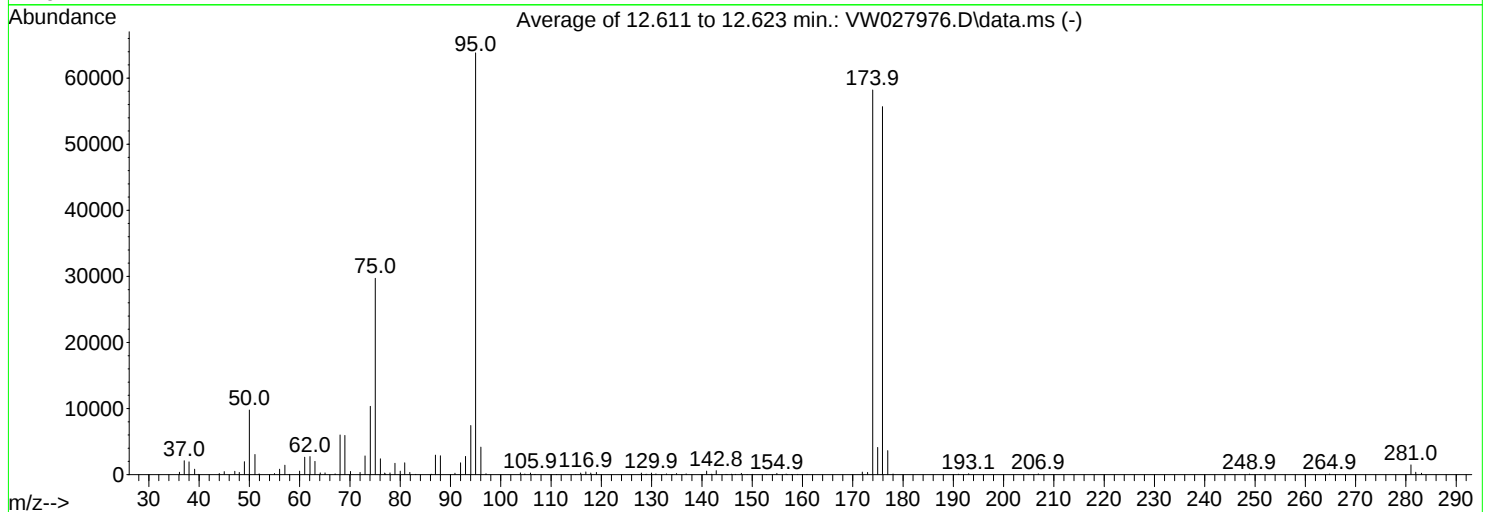


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020924\
Data File : VW027976.D
Acq On : 09 Feb 2024 09:20
Operator : SY/MD
Sample : BFB434
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB434

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Fri Feb 09 22:30:02 2024

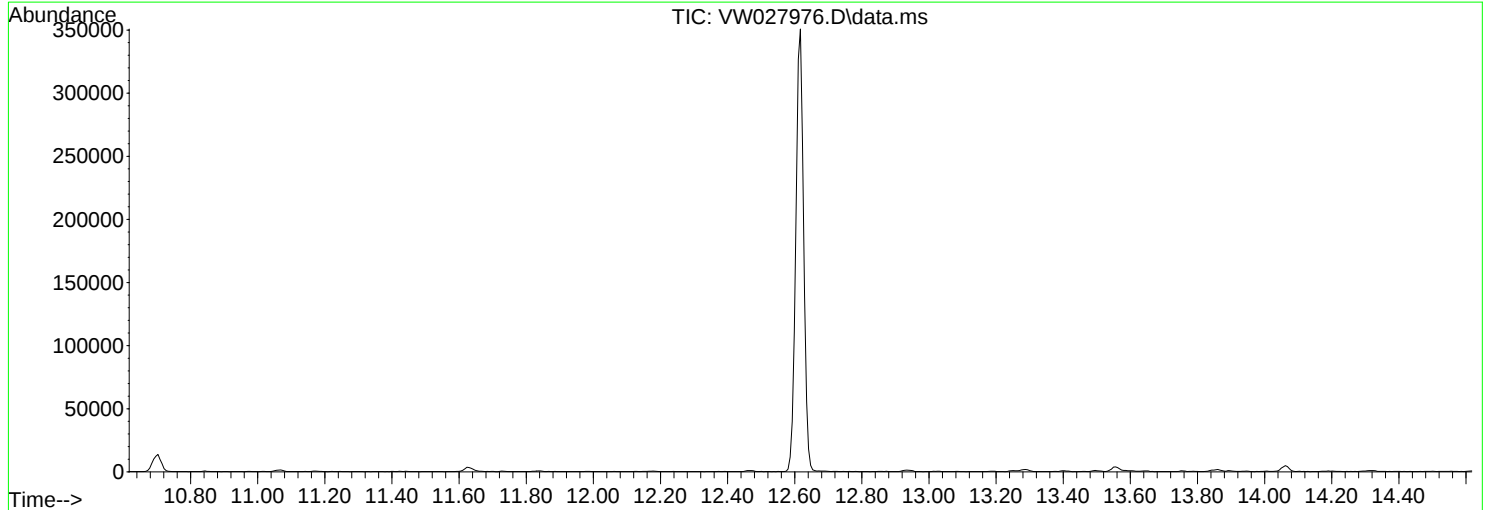

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	9783	PASS
75	95	30	80	46.6	29715	PASS
95	95	100	100	100.0	63827	PASS
96	95	5	9	6.5	4166	PASS
173	174	0.00	2	0.6	346	PASS
174	95	50	120	91.2	58208	PASS
175	174	5	9	7.1	4113	PASS
176	174	95	101	95.7	55677	PASS
177	176	5	9	6.5	3640	PASS

m/z	Abundance
40.00	95.0
44.00	200.0

Instrument :
MSVOA_W
ClientSampleId :
BFB434

m/z	Abundance
36.10	503.0
37.00	2338.0
38.00	2257.0
39.10	874.0
40.00	142.0
44.10	358.0
45.00	610.0
47.20	471.0
48.00	384.0
49.00	2187.0
50.00	11615.0
51.10	3532.0
52.00	140.0
55.00	239.0
56.00	920.0
57.00	1507.0
57.90	70.0
60.00	550.0
61.00	3111.0
62.00	2933.0
63.10	2191.0
64.10	249.0
65.00	267.0
67.00	146.0
68.10	6547.0
69.00	6457.0
70.10	553.0
71.90	376.0
73.00	3088.0
74.00	11321.0
75.00	30528.0
76.10	2849.0
76.90	476.0
78.00	273.0
78.90	1847.0
80.00	549.0
80.90	1822.0
81.90	309.0
83.10	89.0
87.00	3188.0
88.00	3087.0
90.90	252.0
92.00	1856.0
93.00	2935.0
94.00	7860.0
95.00	67352.0
96.10	4701.0
97.00	135.0
103.80	284.0
104.80	139.0
105.80	242.0
106.80	97.0
111.10	87.0
114.90	81.0
116.00	239.0
116.90	420.0
117.90	283.0
119.10	387.0
128.00	305.0
129.10	80.0
129.90	255.0
130.90	135.0
133.00	214.0
134.10	64.0
134.90	205.0
136.90	123.0
140.90	607.0
141.80	82.0
142.90	578.0
144.80	106.0
145.90	98.0
147.90	178.0
150.00	60.0
154.90	161.0
156.70	56.0
157.00	60.0
171.90	453.0
172.90	531.0
173.90	58504.0
174.90	4206.0
175.90	52872.0
176.90	3582.0
178.00	156.0
191.10	97.0
193.00	258.0
204.90	51.0
206.90	199.0
248.90	124.0
251.00	66.0
264.80	198.0
281.00	2709.0
281.90	665.0

Instrument :
MSVOA_W
ClientSampleId :
BFB434

283.10

343.0

Instrument :
MSVOA_W
ClientSampleId :
BFB434

m/z	Abundance
36.10	343.0
37.10	2379.0
38.00	2179.0
39.10	949.0
39.90	184.0
44.00	496.0
45.00	510.0
47.10	669.0
47.90	375.0
49.00	2268.0
50.00	10647.0
51.10	3308.0
51.90	141.0
55.00	172.0
56.00	891.0
57.10	1643.0
58.00	97.0
60.00	524.0
61.00	2926.0
62.00	3208.0
63.00	2263.0
64.10	282.0
65.00	274.0
67.10	158.0
68.00	6669.0
69.00	6810.0
70.10	588.0
72.00	295.0
73.00	3053.0
74.00	11530.0
75.10	34224.0
76.00	2535.0
77.10	290.0
78.00	322.0
78.90	1947.0
80.00	672.0
80.90	2027.0
81.90	379.0
83.10	78.0
86.10	96.0
87.00	3367.0
88.00	2855.0
90.90	181.0
92.00	2179.0
93.00	3139.0
94.10	8271.0
95.00	70720.0
96.00	4665.0
97.00	156.0
103.90	346.0
104.80	94.0
105.90	258.0
106.80	75.0
115.90	344.0
116.90	374.0
117.90	271.0
118.90	416.0
128.00	202.0
129.00	136.0
129.90	297.0
130.80	140.0
133.00	125.0
135.00	173.0
136.80	87.0
140.90	534.0
141.90	88.0
142.80	709.0
145.00	98.0
145.90	79.0
146.70	70.0
147.90	202.0
149.00	67.0
150.10	93.0
154.90	178.0
156.80	89.0
157.80	52.0
159.00	76.0
160.90	124.0
171.90	329.0
173.90	65632.0
175.00	4143.0
175.90	64272.0
176.90	4339.0
178.00	154.0
191.00	111.0
193.10	97.0
206.90	76.0
248.90	123.0
264.90	120.0
281.00	1182.0
282.00	272.0
283.10	254.0

Instrument :
MSVOA_W
ClientSampleId :
BFB434

m/z	Abundance
36.00	245.0
37.00	1570.0
38.10	1379.0
39.10	626.0
40.00	112.0
44.00	293.0
45.00	263.0
47.00	396.0
48.10	228.0
49.00	1463.0
50.10	7086.0
51.10	2347.0
52.00	83.0
55.00	136.0
56.00	699.0
57.00	1137.0
60.00	565.0
61.00	1905.0
62.10	2058.0
63.00	1605.0
64.10	240.0
65.10	242.0
67.10	89.0
68.00	4817.0
69.00	4549.0
70.10	354.0
72.10	348.0
73.00	2335.0
74.10	8136.0
75.10	24392.0
76.00	1849.0
76.90	258.0
77.90	243.0
79.00	1334.0
79.90	355.0
80.90	1565.0
81.90	315.0
86.20	155.0
87.00	2311.0
88.00	2651.0
90.90	209.0
92.10	1337.0
93.00	2246.0
94.00	6208.0
95.00	53408.0
96.00	3131.0
97.10	119.0
104.00	190.0
104.80	96.0
106.00	214.0
115.80	146.0
116.90	447.0
118.00	182.0
119.00	236.0
127.90	205.0
128.80	126.0
130.00	207.0
130.90	123.0
132.80	64.0
134.90	144.0
136.90	127.0
141.00	455.0
141.90	88.0
142.90	501.0
144.80	80.0
145.90	75.0
146.70	58.0
147.80	182.0
152.80	55.0
154.90	217.0
156.80	121.0
159.10	50.0
171.90	368.0
173.00	507.0
174.00	50488.0
174.90	3989.0
175.90	49888.0
177.00	2999.0
193.00	66.0
206.90	74.0
248.90	77.0
281.00	562.0
281.90	178.0
283.10	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB434