


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021119\
Data File : VW008588.D
Acq On : 11 Feb 2019 09:47
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W012419S.M
Title : SW846 8260
Last Update : Fri Jan 25 11:07:41 2019

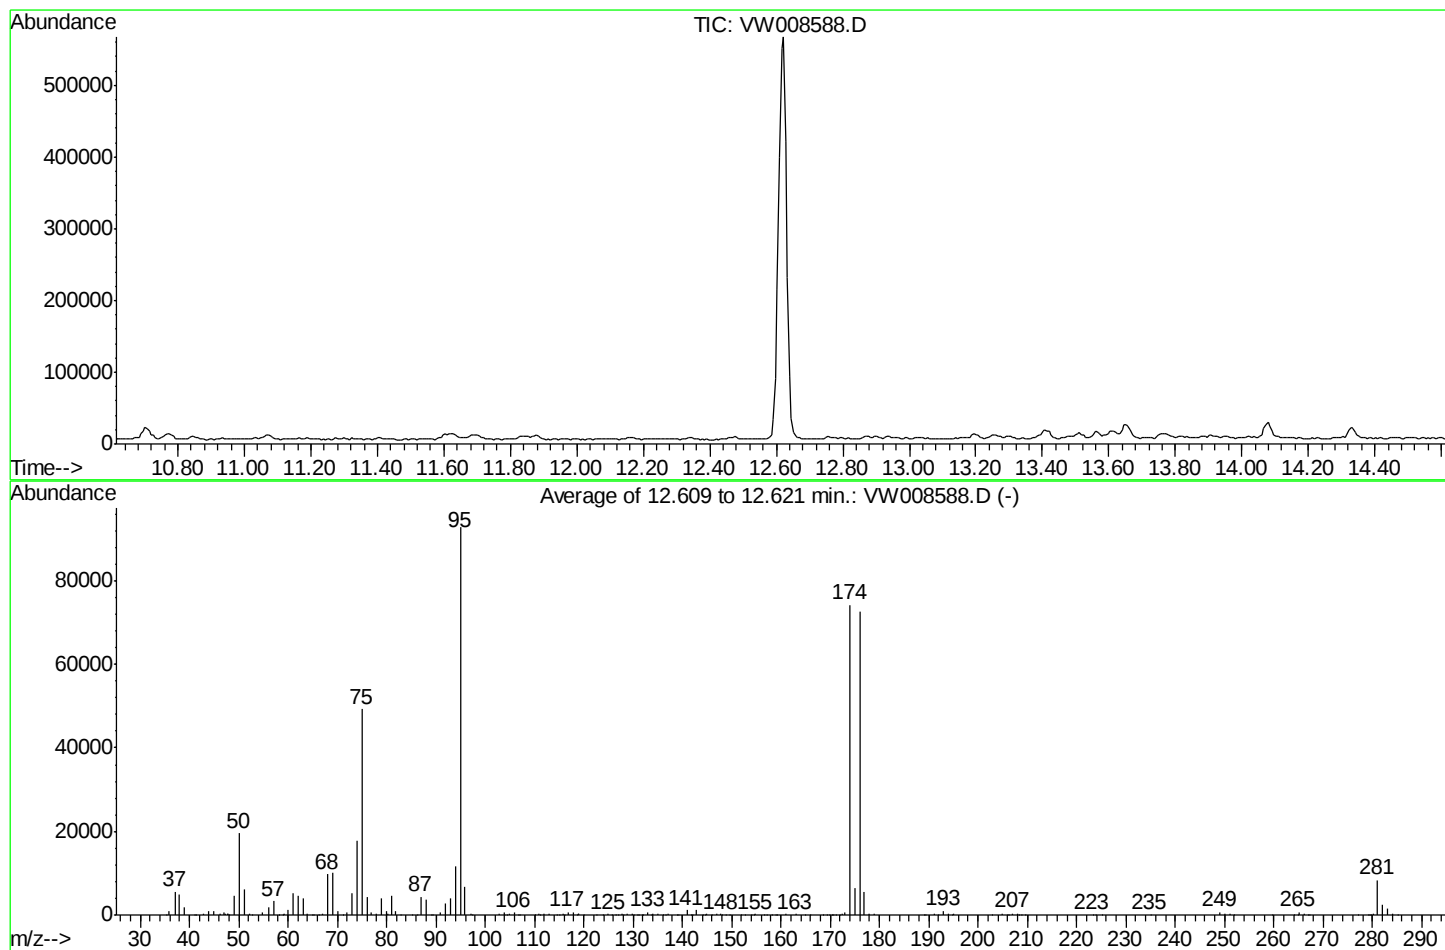

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	19579	PASS
75	95	30	60	53.1	49293	PASS
95	95	100	100	100.0	92802	PASS
96	95	5	9	7.1	6629	PASS
173	174	0.00	2	0.8	624	PASS
174	95	50	100	80.1	74309	PASS
175	174	5	9	8.6	6386	PASS
176	174	95	101	97.9	72720	PASS
177	176	5	9	7.4	5414	PASS