

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021323\
 Data File : VW025329.D
 Acq On : 13 Feb 2023 13:09
 Operator : SY/MD
 Sample : 01512-06
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Feb 13 23:32:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Feb 13 23:31:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	348338	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	334909	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	161624	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	69363	20.578	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.320%
7) Chloroethane-d5	2.899	69	68314	22.825	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.280%
11) 1,1-Dichloroethene-d2	4.021	63	147182	15.747	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.000%
21) 2-Butanone-d5	7.069	46	48333	55.234	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.460%
24) Chloroform-d	7.648	84	216858	23.752	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	8.307	65	117986	26.530	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.120%
32) Benzene-d6	8.276	84	430969	21.232	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.920%
36) 1,2-Dichloropropane-d6	9.270	67	126129	21.237	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.960%
41) Toluene-d8	10.325	98	387532	21.358	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.440%
43) trans-1,3-Dichloroprop...	10.575	79	51505	23.209	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.840%
47) 2-Hexanone-d5	10.922	63	37199	55.863	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	96137	23.803	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	126026	22.475	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.880%
Target Compounds						Qvalue
34) Trichloroethene	8.837	95	10688	1.646	ug/L	# 5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021323\
Data File : VW025329.D
Acq On : 13 Feb 2023 13:09
Operator : SY/MD
Sample : 01512-06
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Feb 13 23:32:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Feb 13 23:31:51 2023
Response via : Initial Calibration

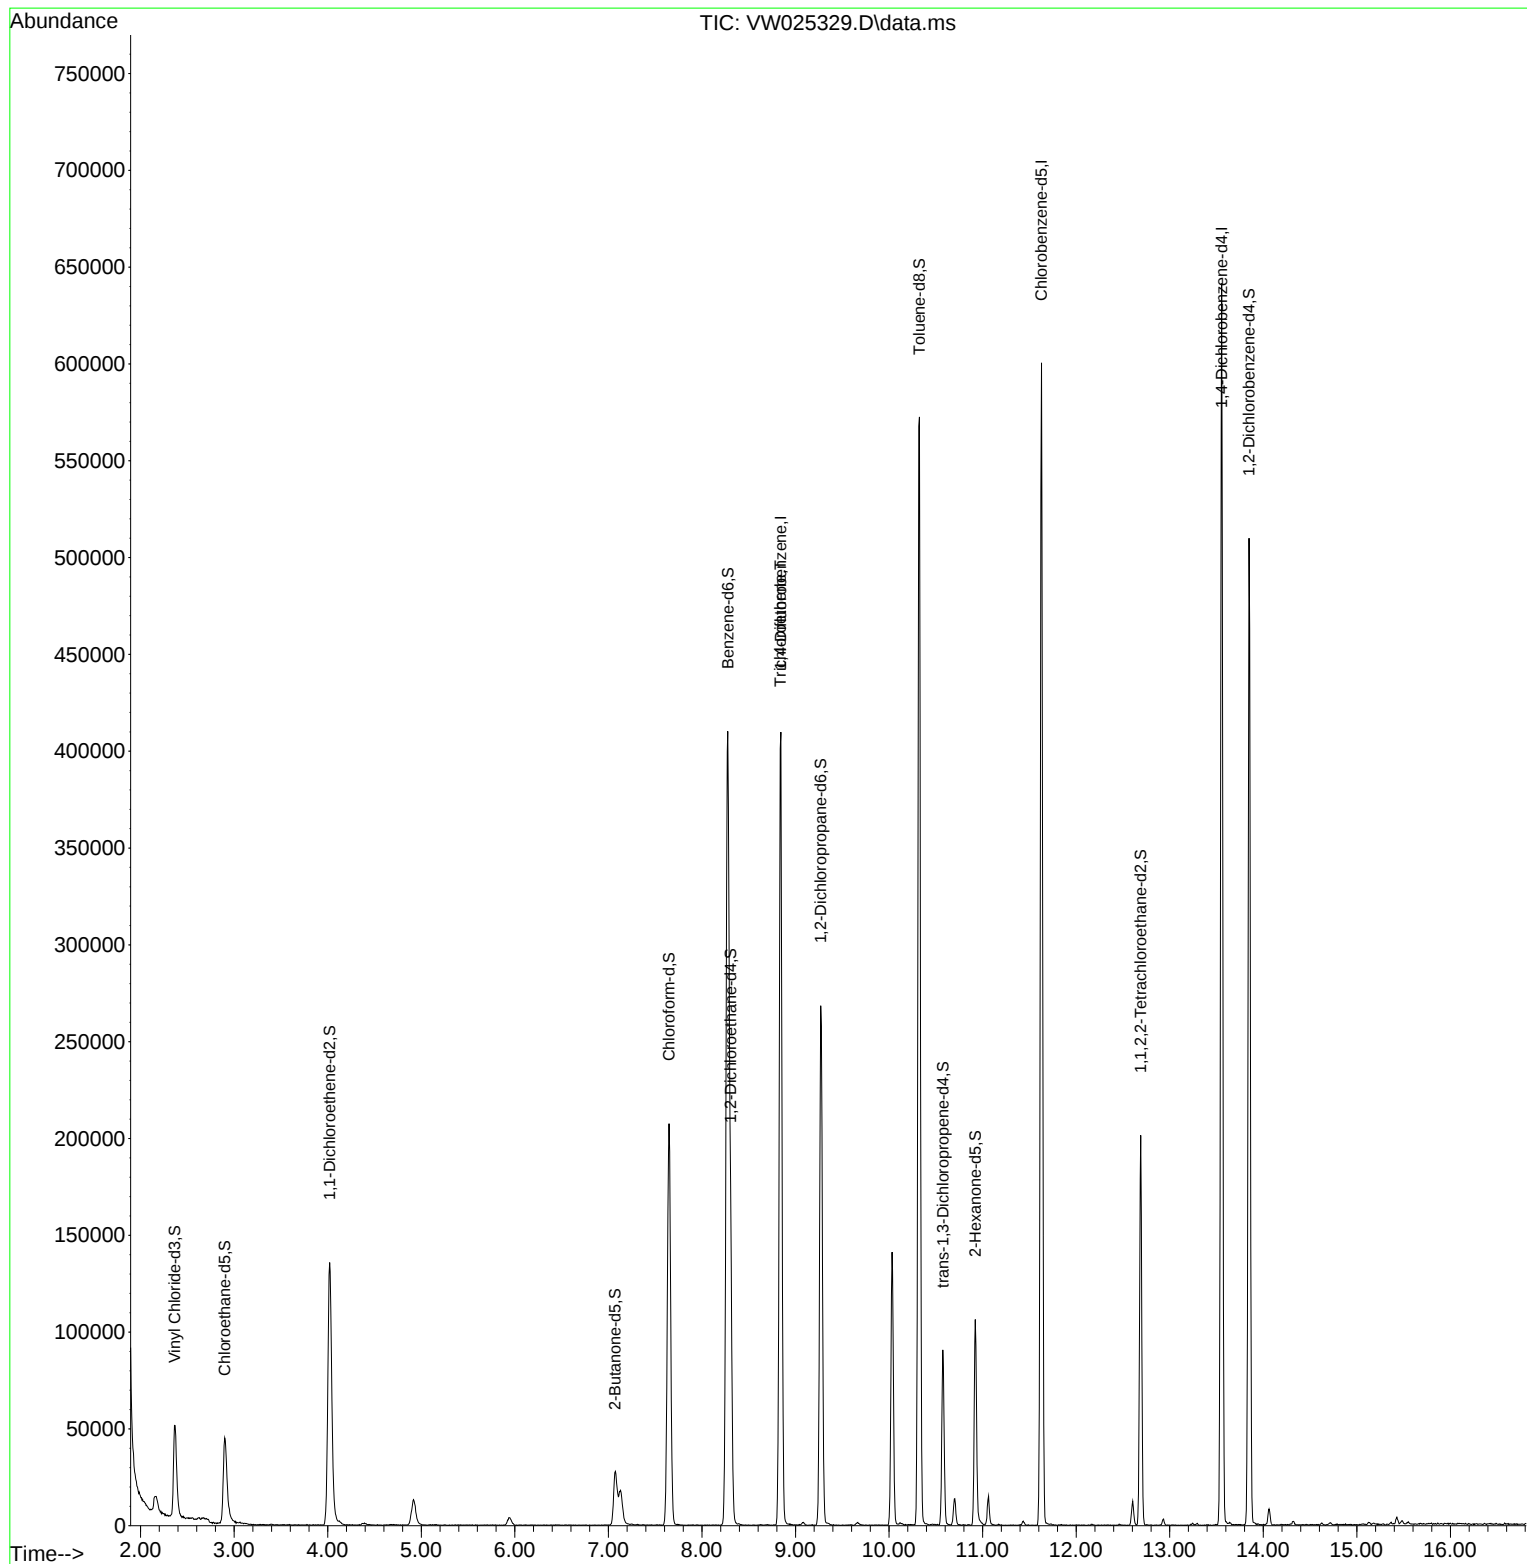

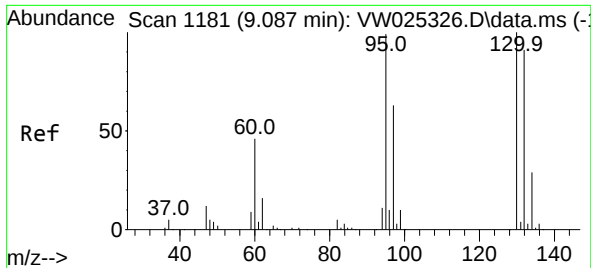

#34

Trichloroethene

Concen: 1.646 ug/L

RT: 8.837 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW025329.D


Acq: 13 Feb 2023 13:09

Instrument :

MSVOA_W

ClientSampleId :

VHBLK002

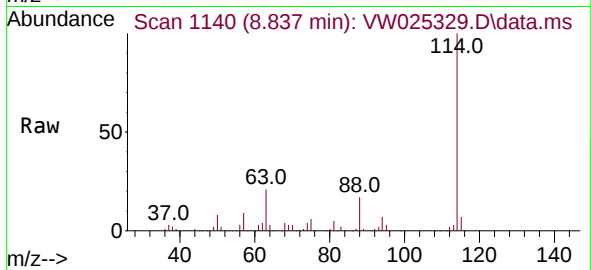

Tgt Ion: 95 Resp: 10688

Ion Ratio Lower Upper

95 100

97 0.0 45.4 84.2#

132 0.0 67.1 124.5#

130 0.0 69.2 128.6#

