
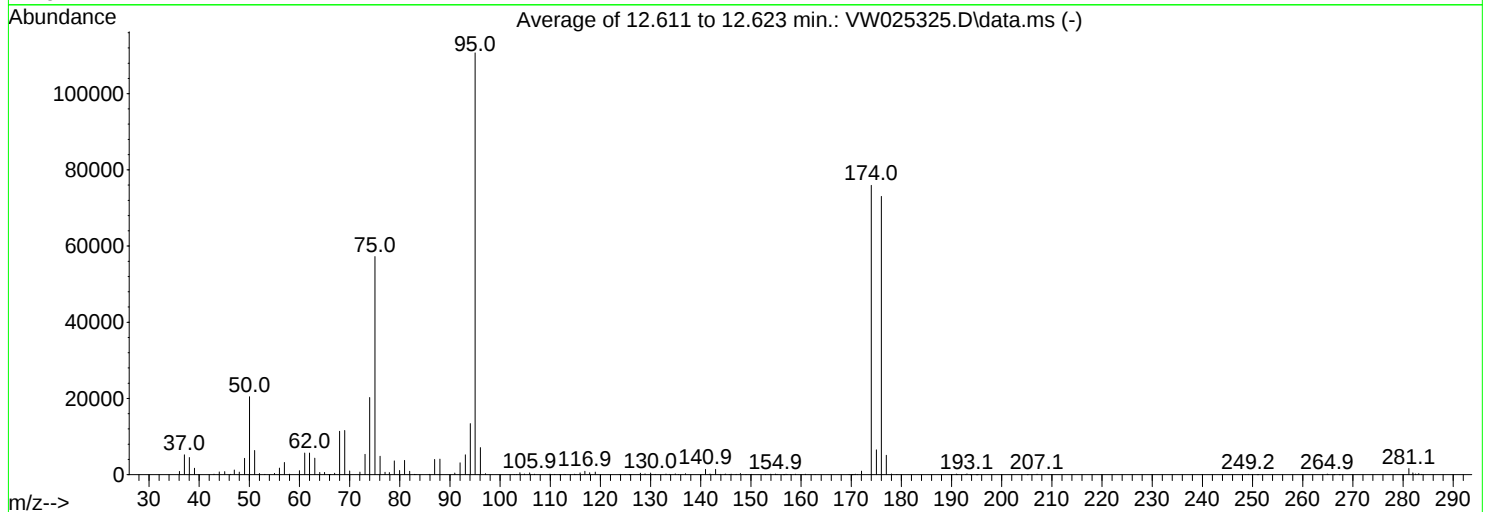


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021323\
Data File : VW025325.D
Acq On : 13 Feb 2023 08:05
Operator : SY/MD
Sample : BFB480
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB480

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Title : SFAM01.0
Last Update : Mon Feb 13 23:31:51 2023

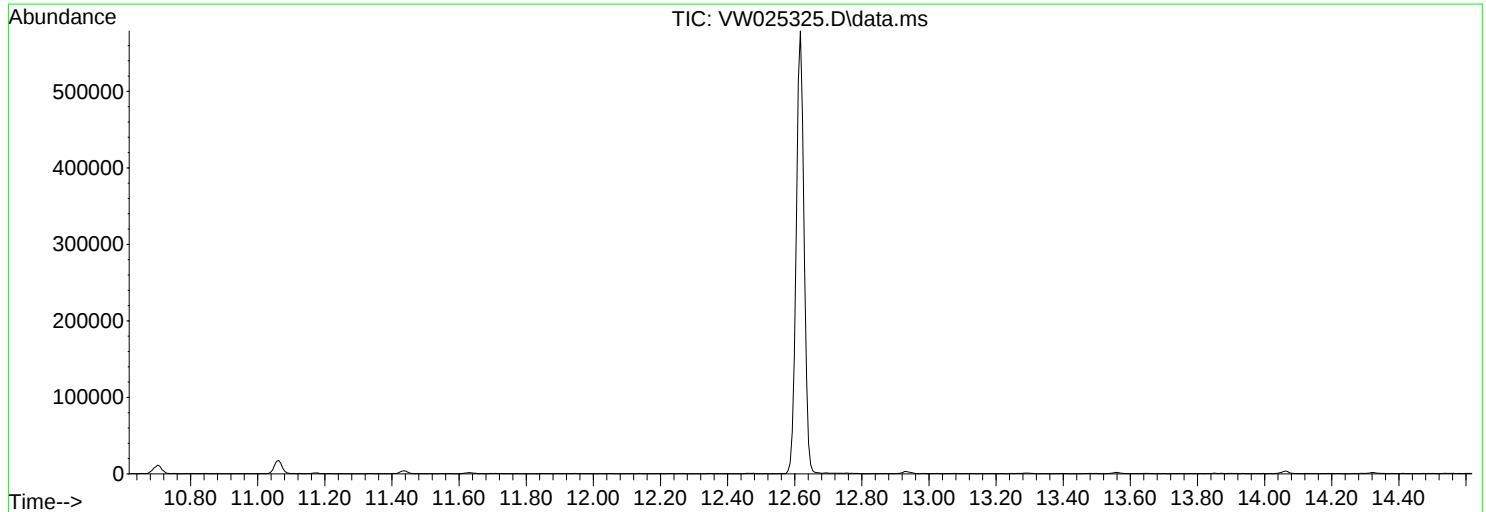

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	20464	PASS
75	95	30	80	51.7	57248	PASS
95	95	100	100	100.0	110717	PASS
96	95	5	9	6.4	7092	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.6	75955	PASS
175	174	5	9	8.6	6534	PASS
176	174	95	105	96.2	73040	PASS
177	176	5	10	7.0	5106	PASS

m/z	Abundance
40.00	174.0
44.00	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB480

m/z	Abundance
36.00	800.0
37.10	5972.0
38.00	4780.0
39.00	1724.0
40.10	168.0
42.90	120.0
44.00	859.0
45.10	796.0
46.20	106.0
47.00	1421.0
47.90	737.0
49.00	4815.0
50.10	21144.0
51.10	6460.0
52.00	288.0
53.20	133.0
55.00	372.0
56.00	1805.0
57.00	3295.0
58.10	149.0
60.00	1129.0
61.00	5893.0
62.00	5686.0
63.00	4776.0
64.00	632.0
65.00	560.0
65.90	70.0
67.10	388.0
68.00	11538.0
69.00	11779.0
70.00	993.0
72.00	673.0
73.00	5219.0
74.00	20072.0
75.00	58432.0
76.00	5094.0
77.00	771.0
77.90	552.0
78.90	3588.0
80.00	1253.0
80.90	3788.0
82.00	902.0
83.00	158.0
86.00	144.0
87.00	3949.0
88.00	4030.0
90.90	469.0
92.00	2877.0
93.00	5218.0
94.10	12771.0
95.00	110288.0
96.00	7323.0
97.00	270.0
102.80	113.0
103.90	651.0
104.90	175.0
106.00	370.0
106.80	120.0
109.90	85.0
110.80	85.0
111.90	61.0
112.70	108.0
114.80	127.0
115.10	140.0
116.00	476.0
116.90	855.0
117.90	574.0
118.90	759.0
124.90	85.0
125.80	64.0
128.00	355.0
129.00	165.0
130.10	297.0
130.90	102.0
133.10	247.0
133.80	159.0
134.80	215.0
137.00	292.0
141.00	1455.0
141.90	138.0
143.00	1323.0
143.90	106.0
144.80	235.0
146.00	219.0
147.10	131.0
147.90	306.0
149.90	126.0
152.90	55.0
153.90	171.0
155.20	206.0
157.00	212.0
159.00	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB480

160.90	125.0
162.80	124.0
170.60	83.0
171.20	123.0
172.10	1028.0
174.00	69504.0
175.00	5504.0
176.00	67400.0
177.00	4422.0
178.00	188.0
179.10	93.0
190.90	258.0
193.00	213.0
193.70	52.0
194.90	54.0
195.10	53.0
205.10	50.0
207.00	208.0
248.70	123.0
249.20	130.0
251.00	64.0
264.90	466.0
266.20	60.0
281.10	2541.0
282.00	732.0
282.50	502.0
283.10	465.0
283.70	204.0

Instrument :
MSVOA_W
ClientSampleId :
BFB480

m/z	Abundance
36.00	1033.0
37.10	5334.0
38.00	5066.0
39.10	2058.0
39.90	321.0
43.00	174.0
44.10	737.0
45.10	1055.0
46.30	103.0
47.00	1117.0
48.00	745.0
49.10	4967.0
50.00	23352.0
51.00	7411.0
52.00	317.0
53.00	64.0
55.00	396.0
56.00	1723.0
57.00	3310.0
58.00	223.0
60.00	1273.0
61.00	6067.0
62.00	6618.0
63.00	4682.0
64.10	583.0
65.00	812.0
66.10	87.0
67.00	328.0
68.00	12881.0
69.00	12850.0
70.00	943.0
72.00	726.0
73.10	6092.0
74.00	21808.0
75.10	62744.0
76.10	5418.0
77.00	632.0
77.90	588.0
78.90	3887.0
79.90	1024.0
80.90	4220.0
82.00	920.0
83.20	95.0
86.90	4885.0
88.00	4795.0
90.90	471.0
92.00	4112.0
93.00	5852.0
94.00	15773.0
95.00	123448.0
96.00	8189.0
97.10	317.0
103.30	129.0
104.00	540.0
104.80	167.0
105.90	549.0
106.90	93.0
110.00	166.0
110.90	149.0
112.80	170.0
114.90	139.0
116.00	528.0
116.90	998.0
117.80	425.0
119.00	738.0
123.90	136.0
126.10	55.0
127.90	408.0
128.90	236.0
129.90	480.0
130.90	102.0
133.00	137.0
133.80	72.0
134.90	255.0
135.60	57.0
137.00	318.0
140.90	1633.0
141.90	217.0
143.00	1246.0
143.90	94.0
145.00	262.0
145.70	128.0
147.00	102.0
147.90	278.0
150.10	129.0
152.90	68.0
154.00	168.0
154.90	341.0
156.50	56.0
157.00	151.0
157.90	54.0
159.00	133.0

Instrument :
MSVOA_W
ClientSampleId :
BFB480

160.80	97.0
162.80	52.0
169.60	56.0
170.80	268.0
172.00	1079.0
174.00	84744.0
175.00	7471.0
176.00	81032.0
177.00	5668.0
177.90	172.0
191.00	208.0
193.10	277.0
207.10	98.0
248.60	57.0
249.10	167.0
265.10	62.0
267.30	60.0
281.20	1822.0
281.90	426.0
283.20	397.0

Instrument :
MSVOA_W
ClientSampleId :
BFB480

m/z	Abundance
36.10	728.0
37.00	4358.0
38.10	3650.0
39.10	1303.0
40.00	172.0
43.00	57.0
44.00	810.0
45.10	567.0
47.00	1122.0
48.10	559.0
49.00	3094.0
50.00	16896.0
51.00	5177.0
52.00	305.0
53.00	81.0
55.10	210.0
56.00	1609.0
57.00	2956.0
57.90	81.0
60.00	799.0
61.10	5057.0
62.00	4739.0
63.10	3547.0
64.00	506.0
65.10	366.0
66.90	402.0
68.00	9692.0
69.00	10147.0
70.00	1001.0
72.10	667.0
73.00	4757.0
74.00	18872.0
75.00	50568.0
76.10	3976.0
77.10	470.0
77.90	467.0
78.90	3344.0
80.00	1010.0
81.00	3152.0
81.90	888.0
82.90	119.0
85.80	118.0
87.00	3204.0
88.00	3361.0
91.00	381.0
92.00	2364.0
93.10	4599.0
94.00	11713.0
95.00	98416.0
96.10	5764.0
97.20	221.0
104.00	356.0
104.90	131.0
105.80	534.0
106.90	114.0
109.90	127.0
111.00	71.0
113.00	132.0
114.80	106.0
115.90	445.0
116.90	791.0
117.90	481.0
118.90	532.0
123.90	96.0
126.00	55.0
128.00	344.0
128.80	240.0
130.00	499.0
130.90	93.0
133.10	87.0
133.80	65.0
135.00	232.0
135.60	51.0
136.80	156.0
140.90	1128.0
141.80	159.0
142.90	1558.0
143.90	115.0
144.90	221.0
146.10	211.0
147.10	82.0
147.90	303.0
149.00	79.0
150.00	140.0
152.90	58.0
154.90	227.0
157.20	149.0
157.90	62.0
158.80	148.0
160.80	158.0
169.60	68.0
170.20	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB480

170.90	122.0
172.00	699.0
174.00	73616.0
175.00	6626.0
176.00	70688.0
177.00	5227.0
178.10	104.0
191.20	78.0
192.80	101.0
193.10	101.0
207.00	60.0
265.00	79.0
281.10	483.0
282.00	256.0
282.80	125.0

Instrument :
MSVOA_W
ClientSampleId :
BFB480