


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW021419\
Data File : VW008658.D
Acq On : 14 Feb 2019 10:32
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W021319S.M
Title : SW846 8260
Last Update : Thu Feb 14 04:06:50 2019

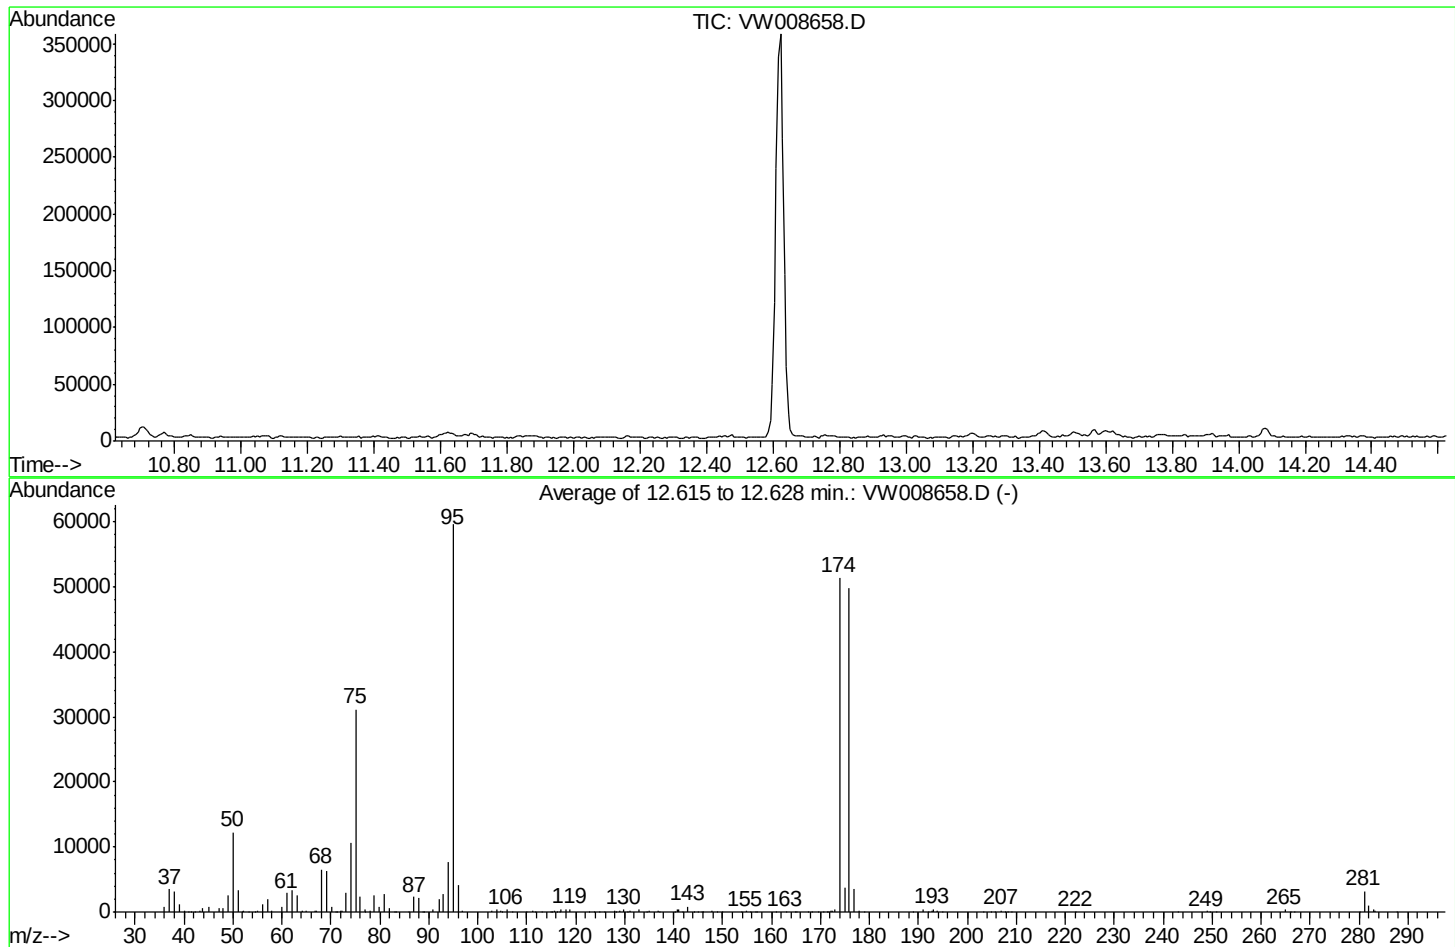

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	12281	PASS
75	95	30	60	52.2	31088	PASS
95	95	100	100	100.0	59586	PASS
96	95	5	9	6.9	4098	PASS
173	174	0.00	2	0.8	437	PASS
174	95	50	100	86.4	51453	PASS
175	174	5	9	7.4	3796	PASS
176	174	95	101	96.9	49874	PASS
177	176	5	9	7.0	3473	PASS