

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021519\
 Data File : VW008681.D
 Acq On : 15 Feb 2019 13:43
 Operator : SY/VA
 Sample : K1500-01
 Misc : 8.05G/5ML/MSVOA W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 G-021419

Quant Time: Feb 16 01:00:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W021319S.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 14 04:06:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	362350	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	547653	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	489266	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	242331	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	208868	55.45	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.90%	
35) Dibromofluoromethane	7.88	113	173315	50.97	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.94%	
50) Toluene-d8	10.32	98	645010	49.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.40%	
62) 4-Bromofluorobenzene	12.62	95	232170	47.02	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.04%	
Target Compounds						
16) Acetone	4.12	43	19487	22.732	ug/l	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW021519\
Data File : VW008681.D
Acq On : 15 Feb 2019 13:43
Operator : SY/VA
Sample : K1500-01
Misc : 8.05G/5ML/MSVOA W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
G-021419

Quant Time: Feb 16 01:00:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W021319S.M
Quant Title : SW846 8260
QLast Update : Thu Feb 14 04:06:50 2019
Response via : Initial Calibration

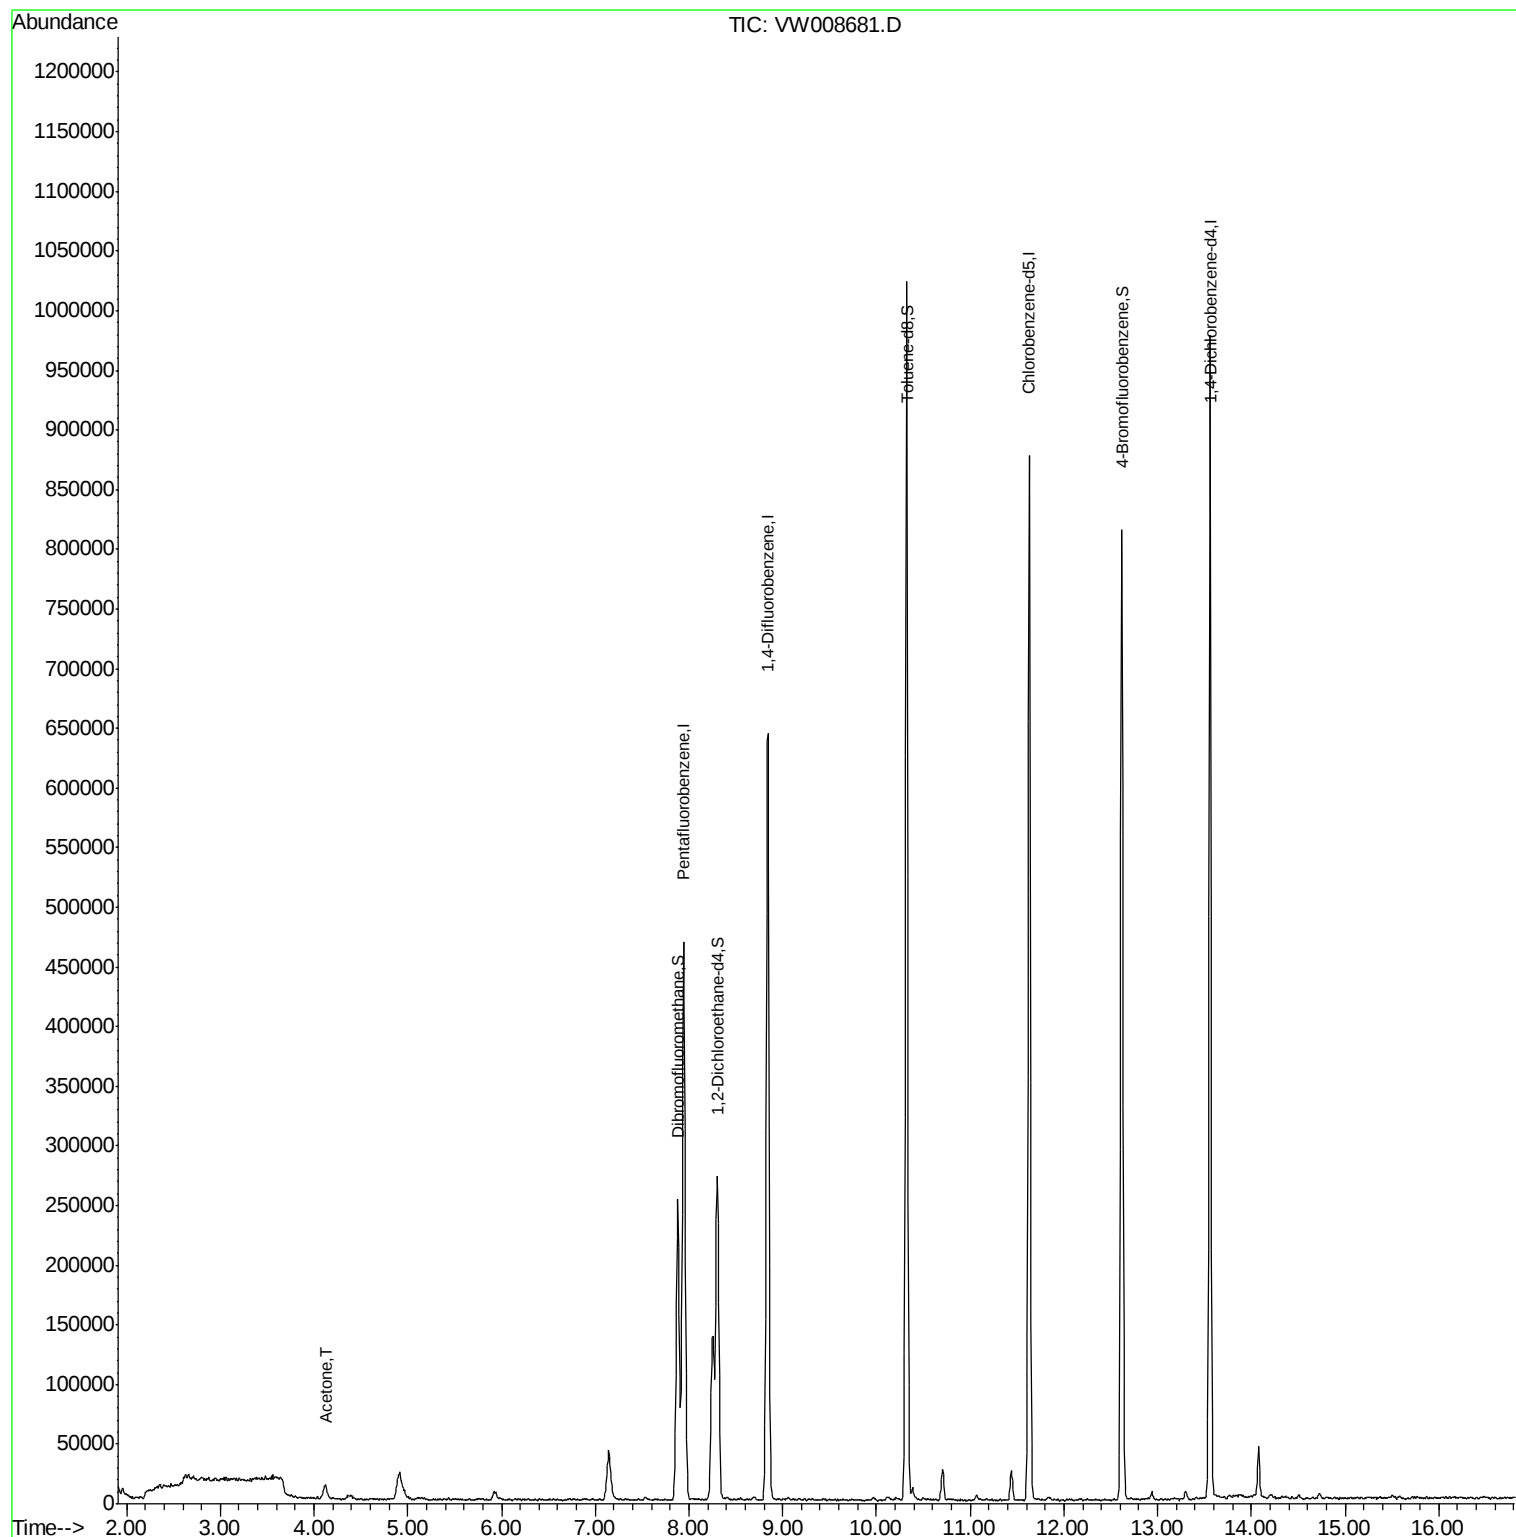

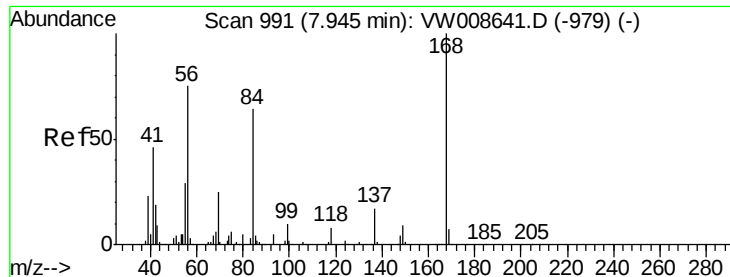

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW008681.D

Acq: 15 Feb 2019 13:43


Instrument :
MSVOA_W
ClientSampleId :
G-021419

Tot Ion:168 Resp: 362350

Ion Ratio Lower Upper




168 100

99 53.6 42.8 64.2

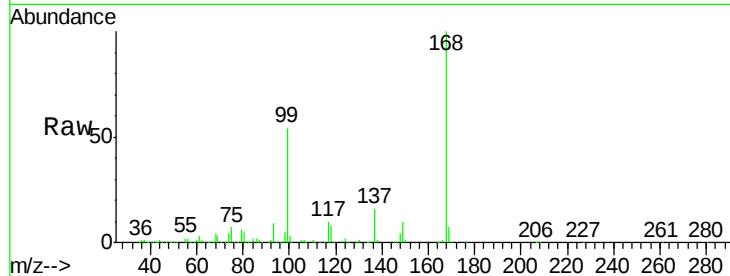

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

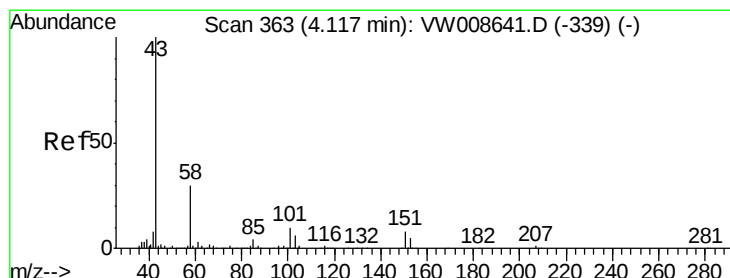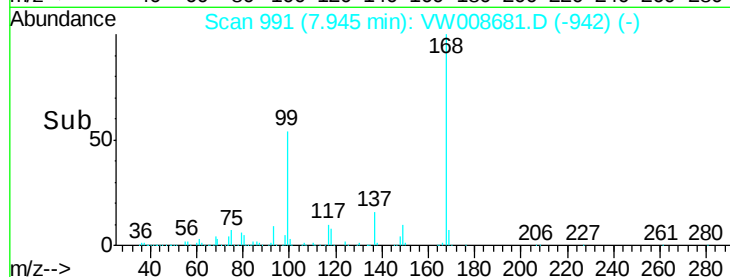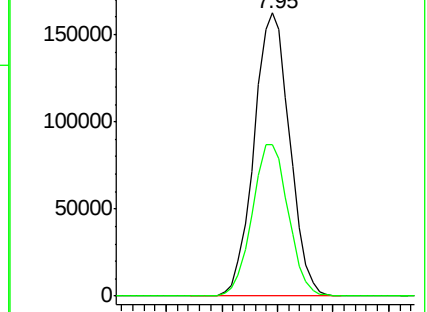

#16

Acetone

Concen: 22.732 ug/l

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW008681.D


Acq: 15 Feb 2019 13:43

Tgt Ion: 43 Resp: 19487

Ion Ratio Lower Upper



43 100


58 24.9 24.1 36.1

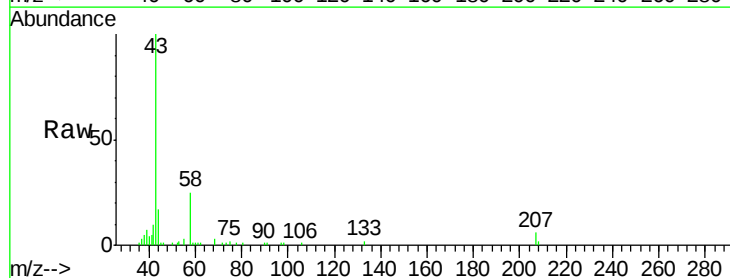

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

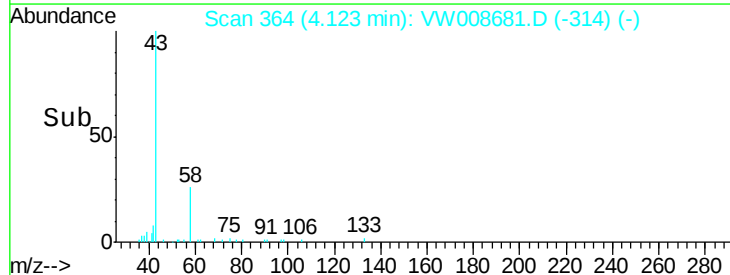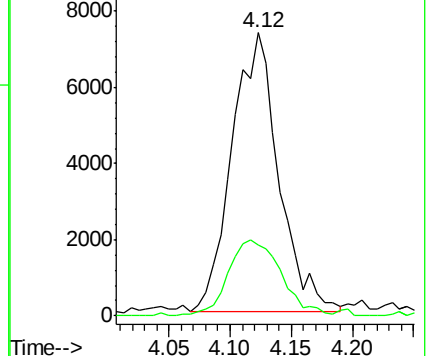

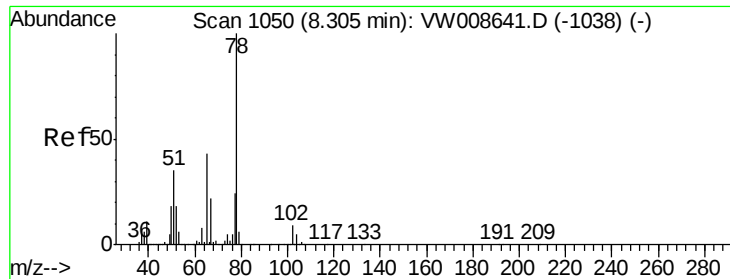

#33

1,2-Dichloroethane-d4

Concen: 55.445 ug/l

RT: 8.30 min Scan# 1049

Delta R.T. -0.01 min

Lab File: VW008681.D

Acq: 15 Feb 2019 13:43

Instrument :

MSVOA_W

ClientSampled :


G-021419

Tot Ion: 65 Resp: 208868

Ion Ratio Lower Upper




65 100

67 51.2 0.0 102.0

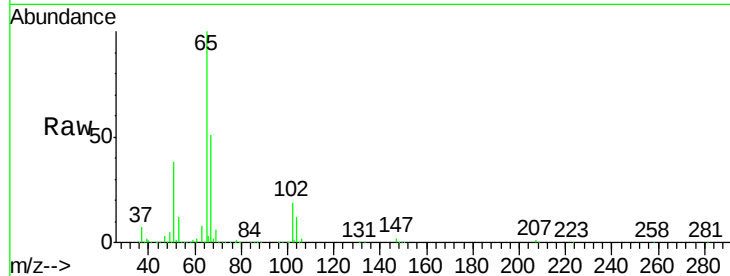

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

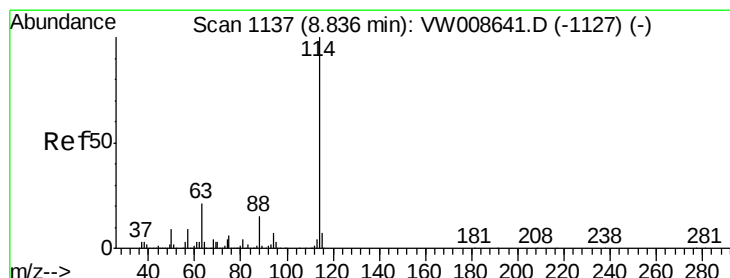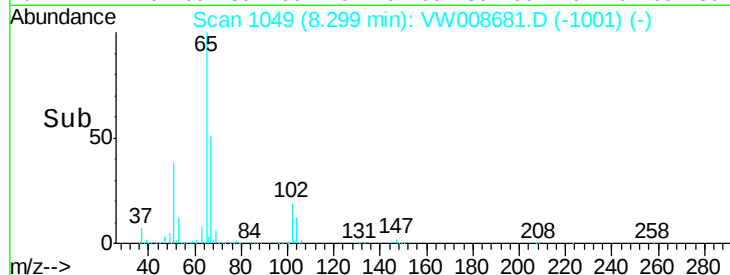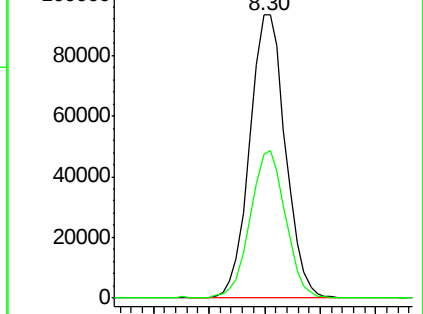

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. 0.01 min

Lab File: VW008681.D

Acq: 15 Feb 2019 13:43


Tgt Ion: 114 Resp: 547653

Ion Ratio Lower Upper

114 100

63 19.6 0.0 41.2



88 15.2 0.0 29.6

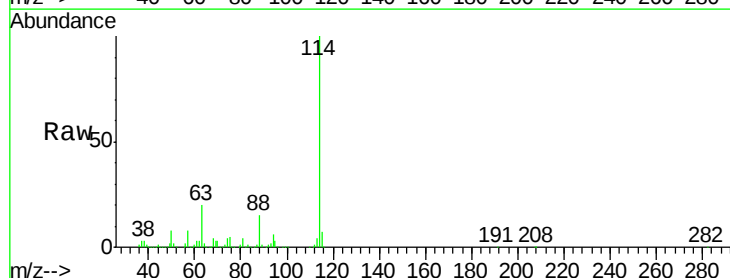


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW



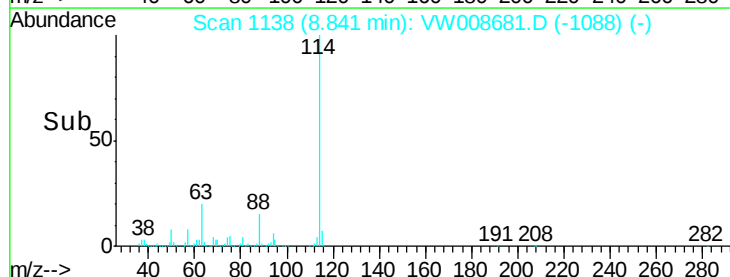
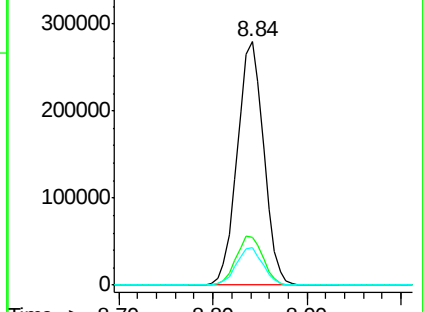


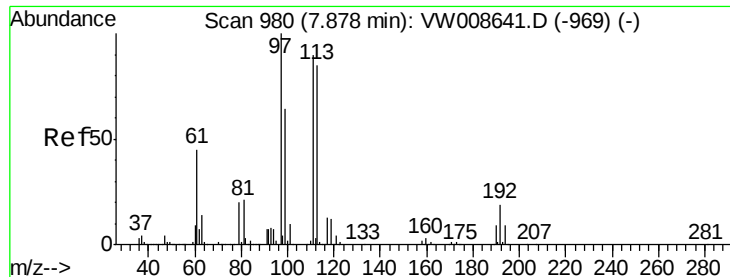

#35
 Dibromofluoromethane
 Concen: 50.966 ug/l
 RT: 7.88 min Scan# 980
 Delta R.T. -0.00 min
 Lab File: VW008681.D
 Acq: 15 Feb 2019 13:43




Instrument :
 MSVOA_W
 ClientSampleId :
 G-021419


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.4	84.0	126.0
192	21.3	17.4	26.2

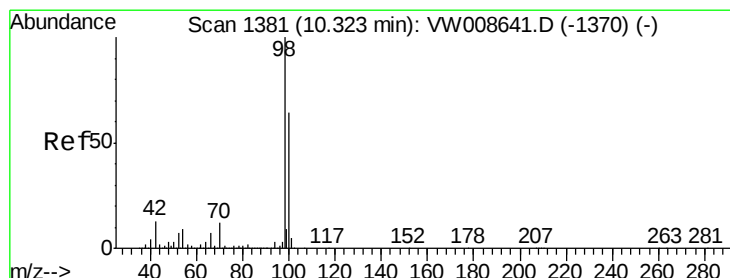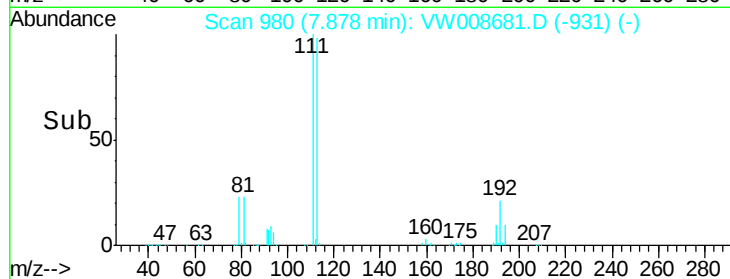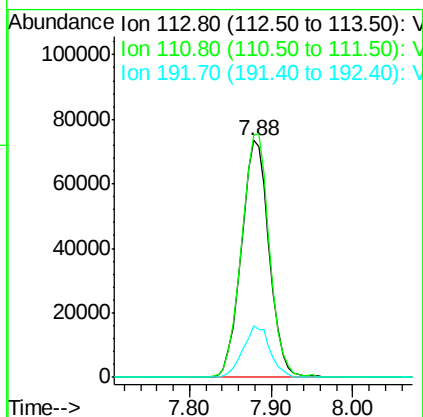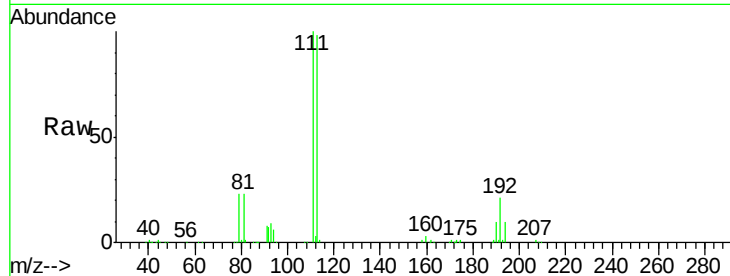

#50
 Toluene-d8
 Concen: 49.204 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. -0.00 min
 Lab File: VW008681.D
 Acq: 15 Feb 2019 13:43

Tgt Ion	Ratio	Lower	Upper
98	100		
100	66.0	52.2	78.4

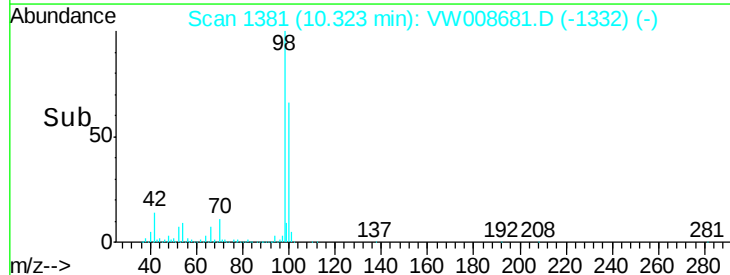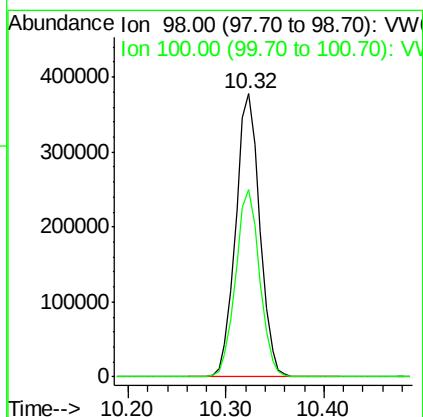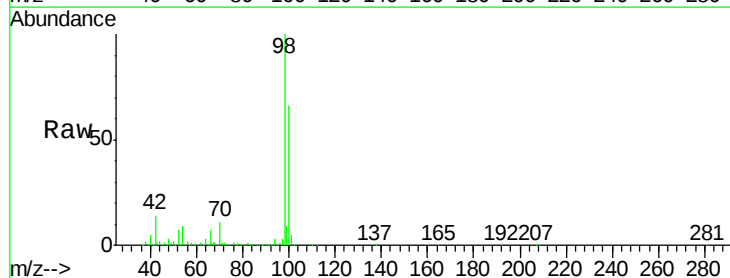

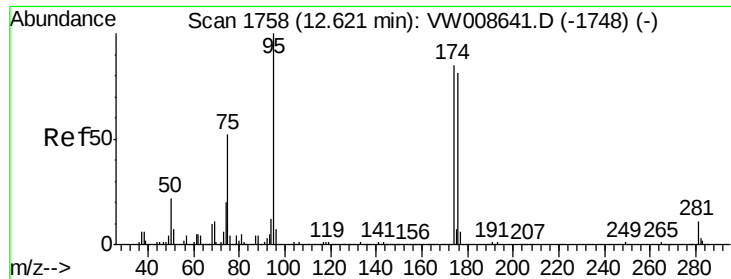

#62

4-Bromofluorobenzene

Concen: 47.020 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW008681.D

Acq: 15 Feb 2019 13:43

Instrument :

MSVOA_W

ClientSampleId :

G-021419





Tot Ion: 95 Resp: 232170

Ion Ratio Lower Upper

95 100

174 85.8 0.0 163.2

176 82.6 0.0 158.0

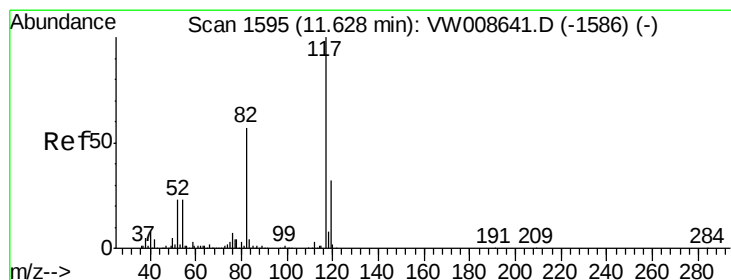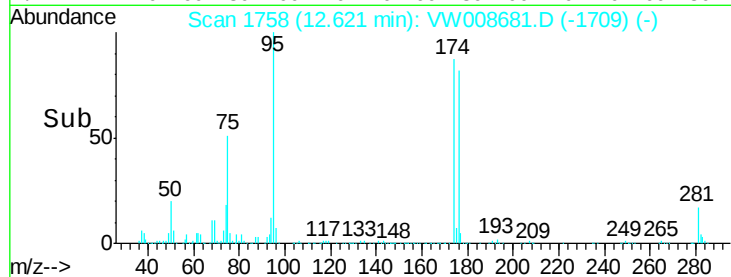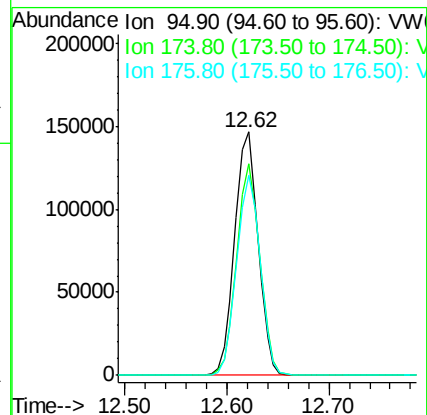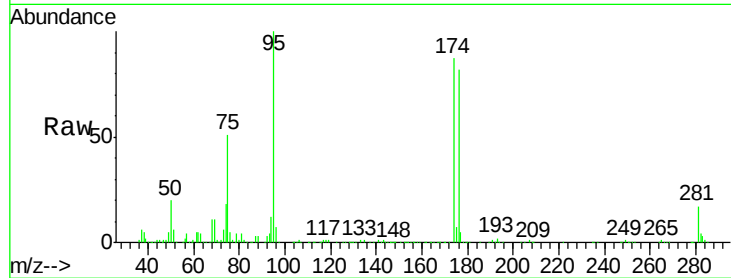

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. 0.01 min

Lab File: VW008681.D

Acq: 15 Feb 2019 13:43




Tgt Ion: 117 Resp: 489266


Ion Ratio Lower Upper

117 100

82 53.8 45.6 68.4

119 32.5 25.7 38.5

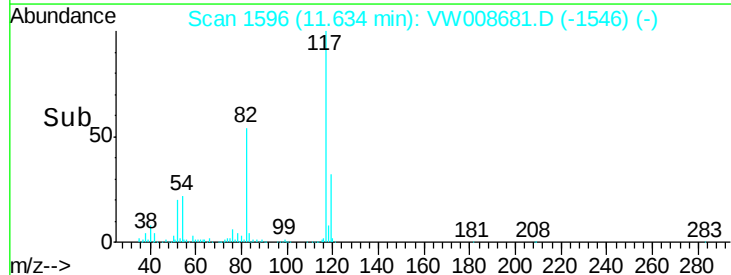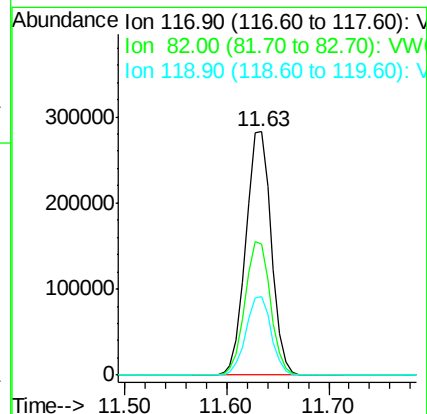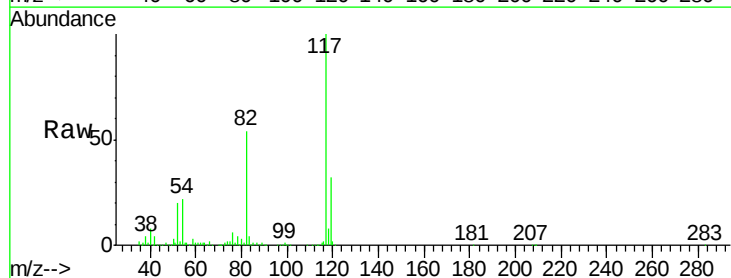

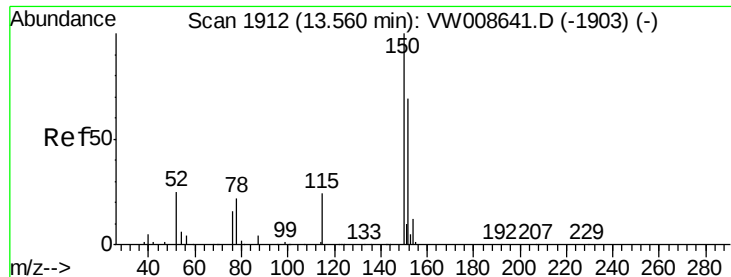

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. -0.00 min

Lab File: VW008681.D

Acq: 15 Feb 2019 13:43

Instrument :

MSVOA_W

ClientSampleId :

G-021419


Tot Ion:152 Resp: 242331

Ion Ratio Lower Upper

152 100

115 57.8 29.3 87.8

150 157.0 0.0 352.8

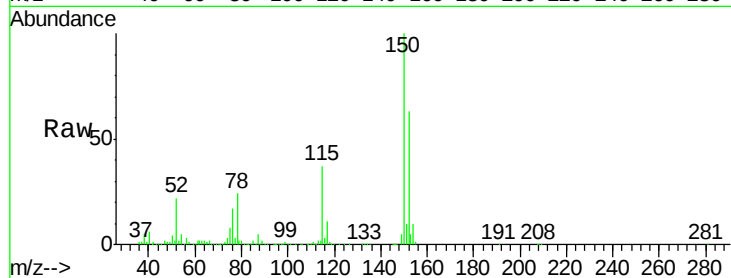

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

