


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW021519\  
 Data File : VW008699.D  
 Acq On : 15 Feb 2019 22:12  
 Operator : SY/VA  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA W/SOIL  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W021319S.M  
 Title : SW846 8260  
 Last Update : Thu Feb 14 04:06:50 2019

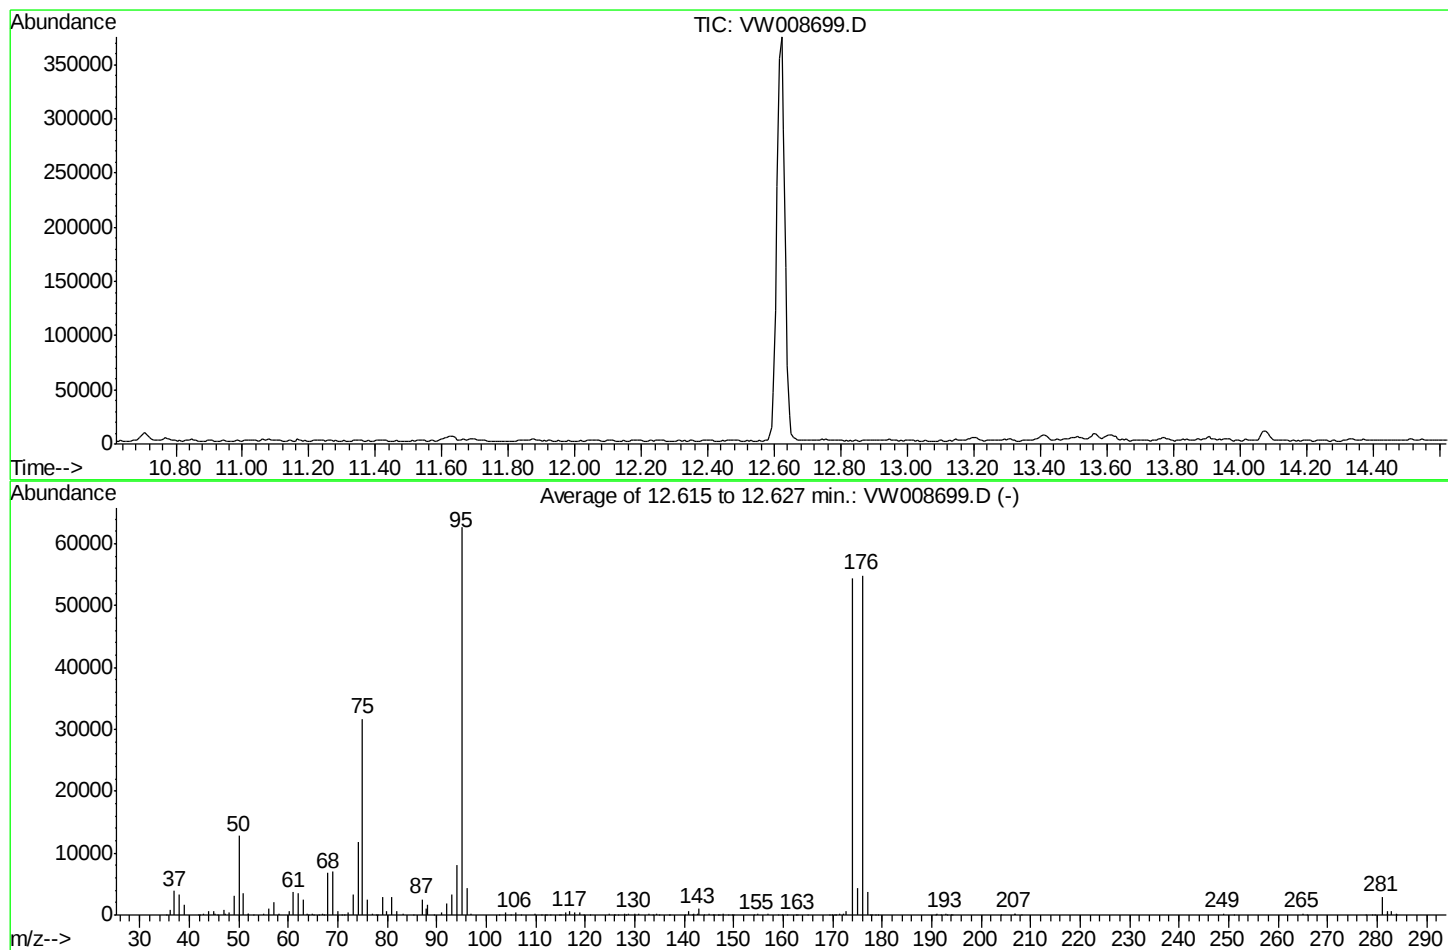

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.4      | 12761   | PASS             |
| 75          | 95           | 30           | 60           | 50.6      | 31693   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 62650   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 4269    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 567     | PASS             |
| 174         | 95           | 50           | 100          | 86.9      | 54474   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 4372    | PASS             |
| 176         | 174          | 95           | 101          | 100.7     | 54856   | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 3739    | PASS             |