


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021521\
Data File : VW018140.D
Acq On : 15 Feb 2021 17:04
Operator : SY/VA
Sample : M1370-16
Misc : 7.04G/10ML/MSVOA_W/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBGZ2

Quant Time: Feb 16 02:26:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
Quant Title : VOC Analysis
QLast Update : Tue Feb 16 02:20:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
2/17/2021 10:35:30 AM

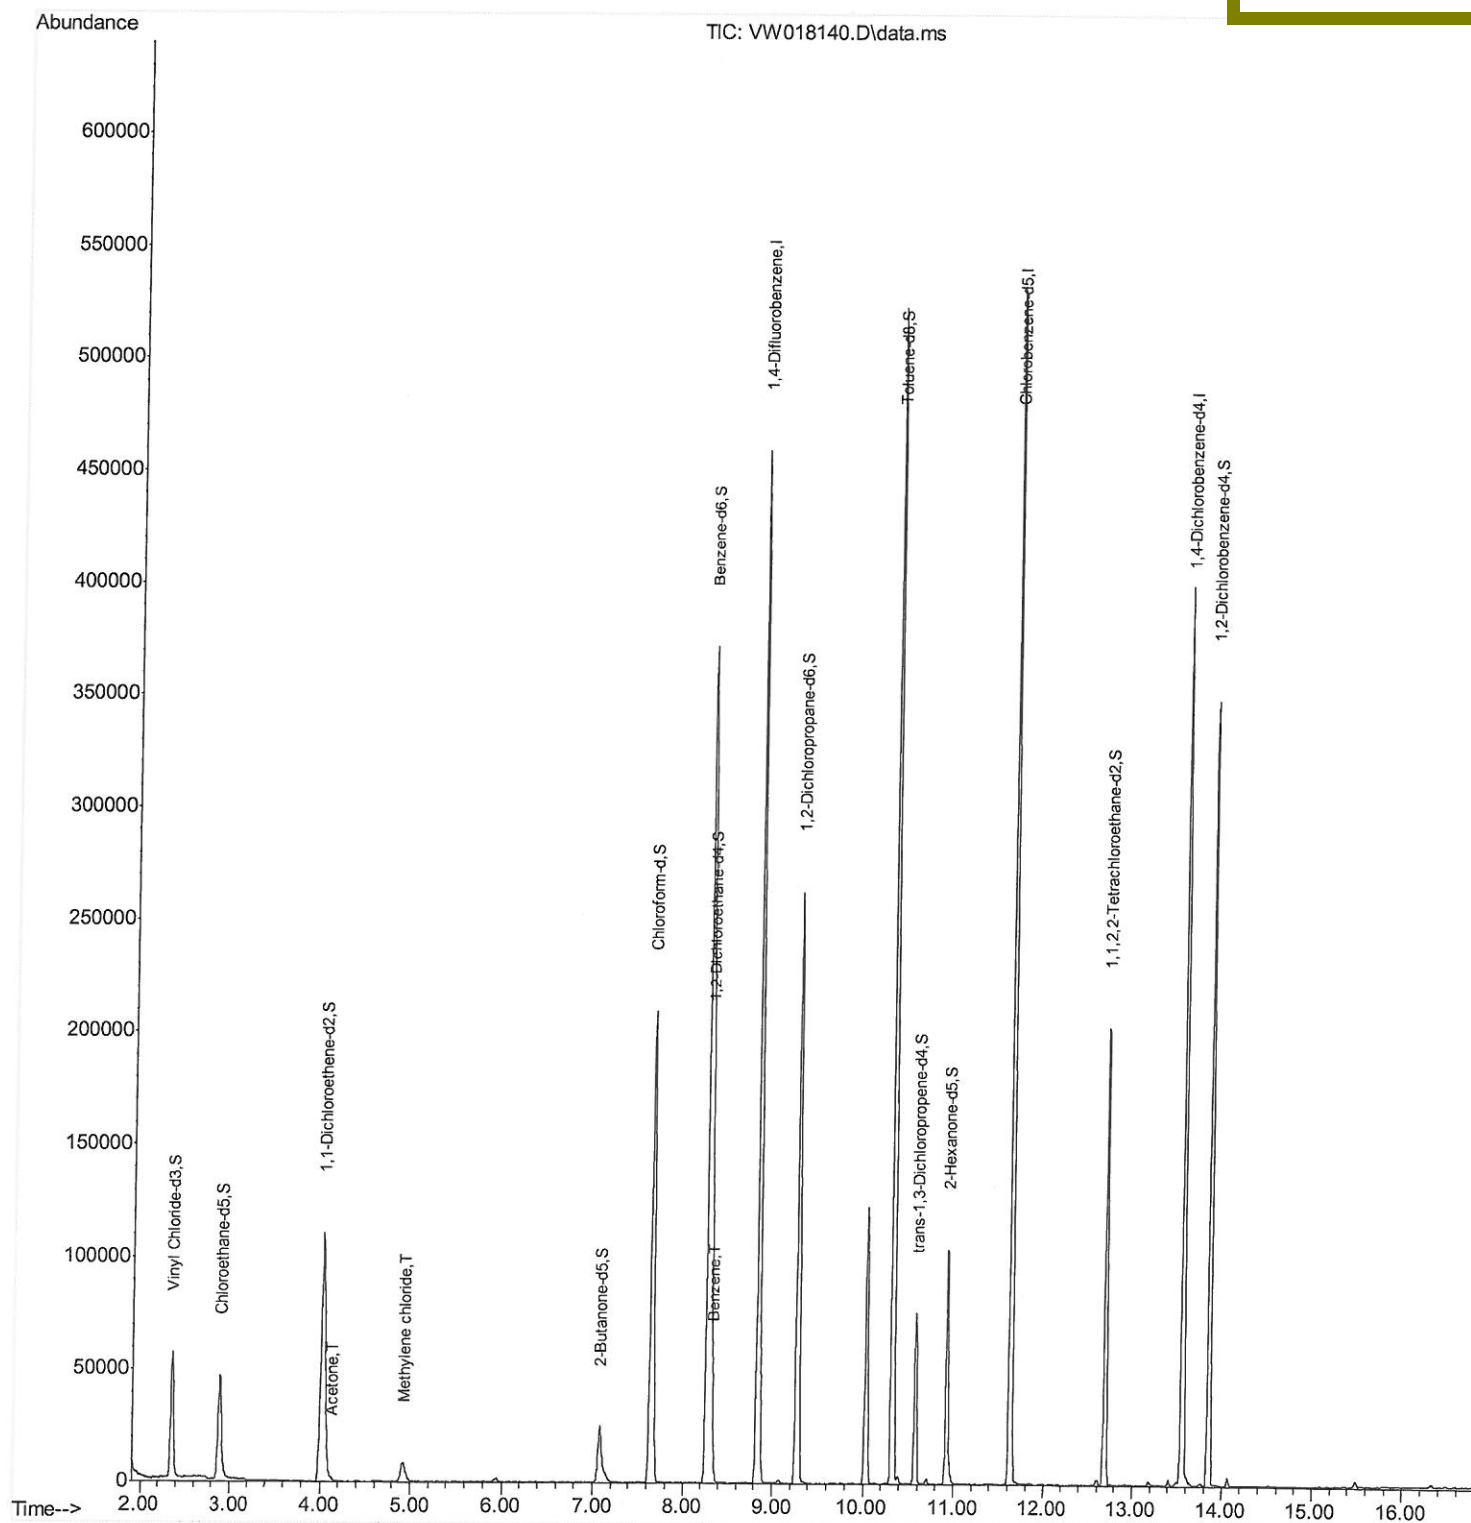

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021521\
 Data File : VW018140.D
 Acq On : 15 Feb 2021 17:04
 Operator : SY/VA
 Sample : M1370-16
 Misc : 7.04G/10ML/MSVOA_W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBGZ2

Quant Time: Feb 16 02:26:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 16 02:20:15 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 2/17/2021 10:35:30 AM

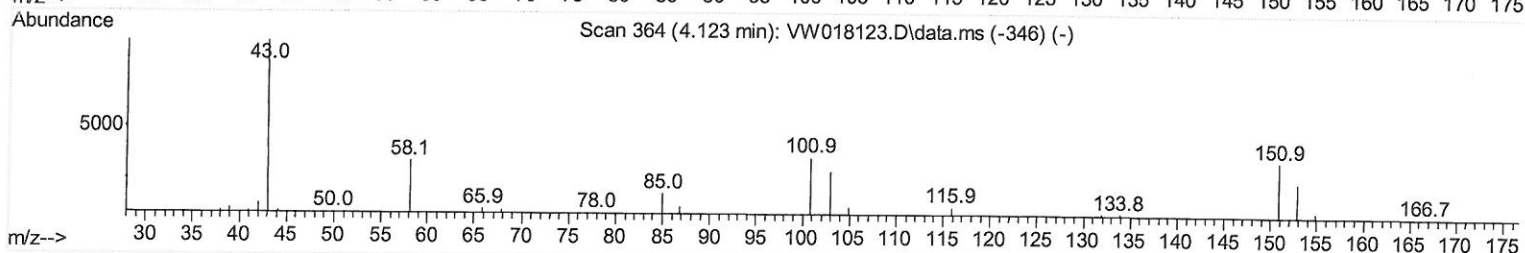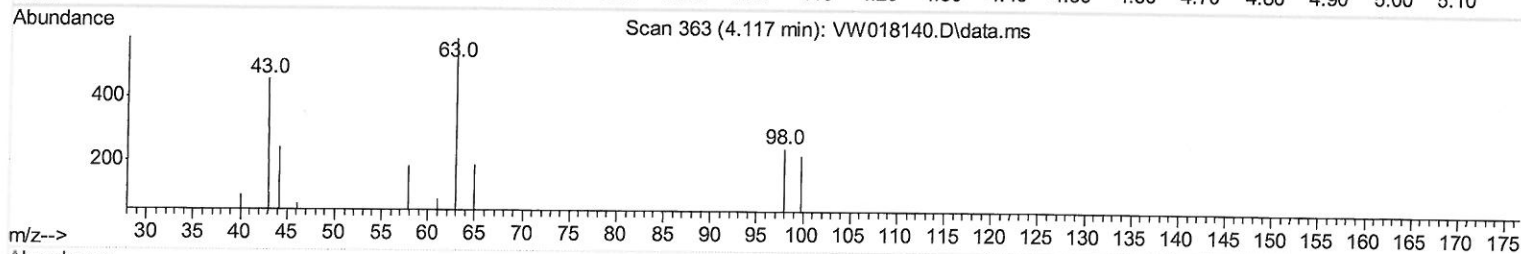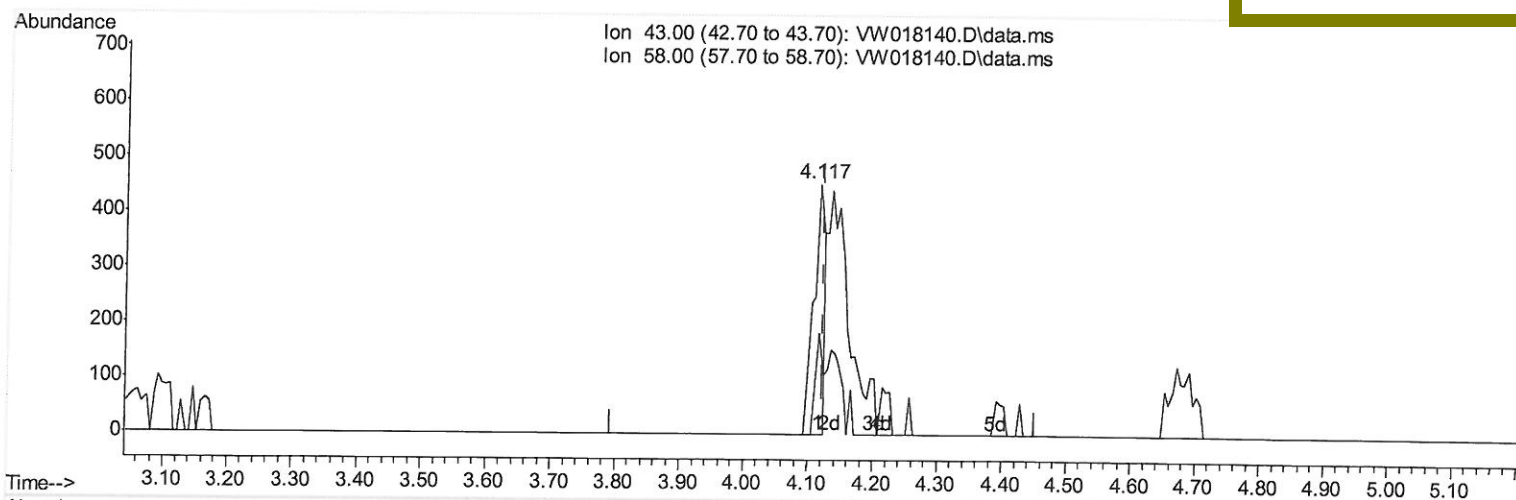

TIC: VW018140.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 0.51 ug/L

response 518

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.20	27.03
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021521\
 Data File : VW018140.D
 Acq On : 15 Feb 2021 17:04
 Operator : SY/VA
 Sample : M1370-16
 Misc : 7.04G/10ML/MSVOA_W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBGZ2

Quant Time: Feb 16 02:26:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 16 02:20:15 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 2/17/2021 10:35:30 AM

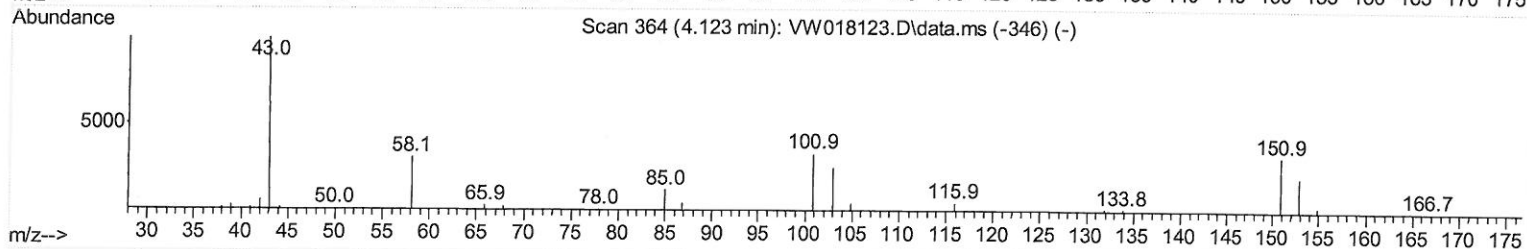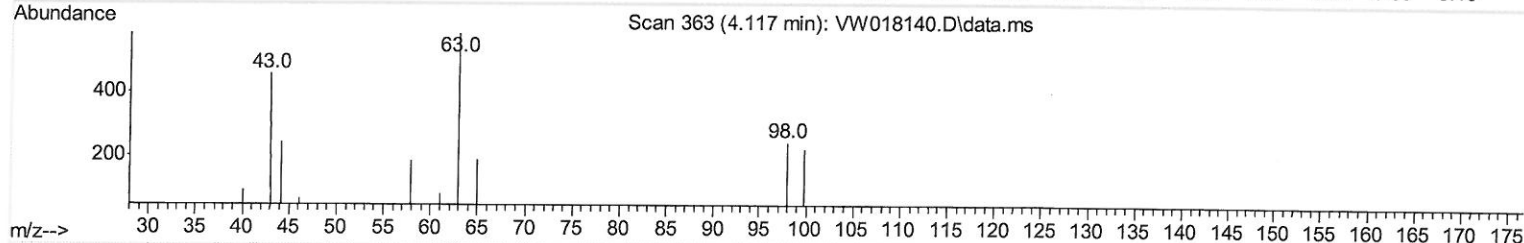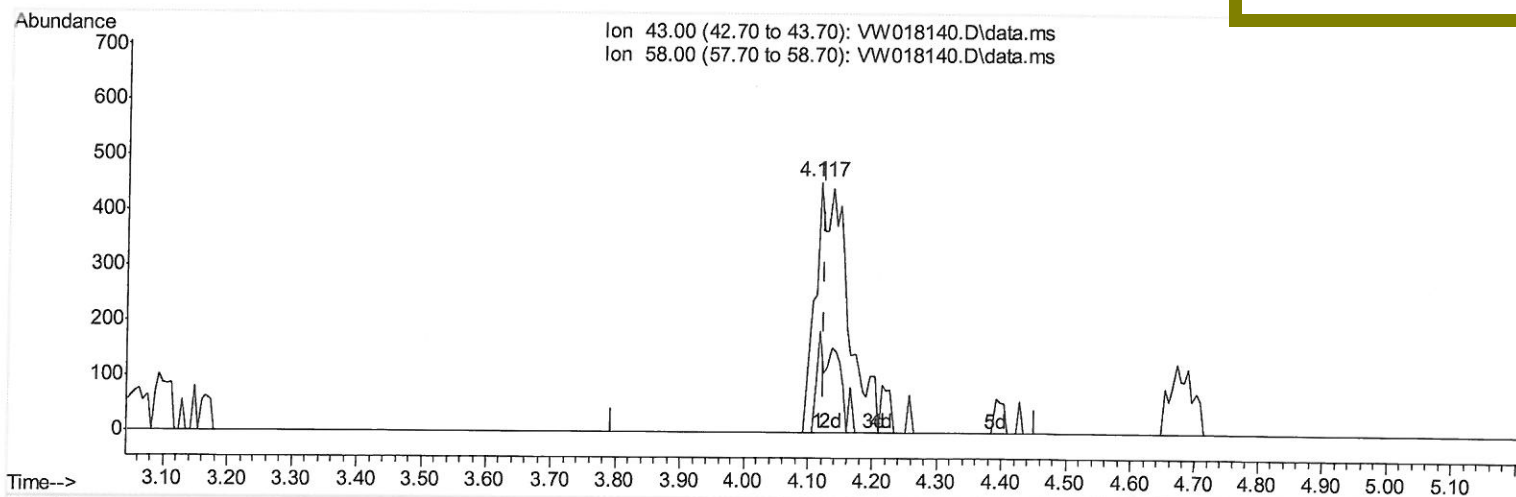

TIC: VW018140.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 1.53 ug/L m

response 1556

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.20	9.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021521\
 Data File : VW018140.D
 Acq On : 15 Feb 2021 17:04
 Operator : SY/VA
 Sample : M1370-16
 Misc : 7.04G/10ML/MSVOA_W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 DBGZ2

Quant Time: Feb 16 02:26:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Feb 16 02:20:15 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 2/17/2021 10:35:30 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	415615	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	321917	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	114766	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	70020	13.56	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.24%		
7) Chloroethane-d5	2.891	69	67080	16.36	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	65.44%		
10) 1,1-Dichloroethene-d2	4.025	63	121508	11.77	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	47.08%		
20) 2-Butanone-d5	7.074	46	43018	31.21	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	62.42%		
24) Chloroform-d	7.647	84	224429	20.58	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.32%		
26) 1,2-Dichloroethane-d4	8.305	65	113689	19.57	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.28%		
29) Benzene-d6	8.275	84	408588	23.11	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.44%		
33) 1,2-Dichloropropane-d6	9.274	67	125402	25.37	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.48%		
37) Toluene-d8	10.323	98	354190	21.06	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.24%		
38) trans-1,3-Dichloroprop...	10.579	79	44667	19.93	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.72%		
39) 2-Hexanone-d5	10.921	63	38229	40.45	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.90%		
48) 1,1,2,2-Tetrachloroeth...	12.688	84	99741	22.97	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	91.88%		
61) 1,2-Dichlorobenzene-d4	13.853	152	97590	23.84	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	95.36%		
Target Compounds						
13) Acetone	4.117	43	1556m	1.53	ug/L	Qvalue
16) Methylene chloride	4.928	84	8851	1.33	ug/L	86
34) Benzene	8.330	78	10953	0.58	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed