

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
 Data File : VW025335.D
 Acq On : 15 Feb 2023 13:25
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK413

Quant Time: Feb 15 22:07:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 15 22:06:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	346882	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	309410	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	153547	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	60562	18.042	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.160%		
7) Chloroethane-d5	2.893	69	63467	21.294	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.160%		
11) 1,1-Dichloroethene-d2	4.027	63	136724	14.689	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	58.760%		
21) 2-Butanone-d5	7.075	46	59852	68.685	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	137.360%#		
24) Chloroform-d	7.648	84	215127	23.661	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.640%		
26) 1,2-Dichloroethane-d4	8.301	65	120500	27.209	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	108.840%		
32) Benzene-d6	8.276	84	418479	22.315	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.280%		
36) 1,2-Dichloropropane-d6	9.270	67	125292	22.835	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.320%		
41) Toluene-d8	10.325	98	377643	22.528	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	90.120%		
43) trans-1,3-Dichloroprop...	10.575	79	51503	25.120	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	100.480%		
47) 2-Hexanone-d5	10.922	63	46044	74.845	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	149.680%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	107270	28.748	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	115.000%		
66) 1,2-Dichlorobenzene-d4	13.848	152	131421	24.669	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.680%		
Target Compounds					Qvalue	
34) Trichloroethene	8.837	95	11202	1.868	ug/L #	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
Data File : VW025335.D
Acq On : 15 Feb 2023 13:25
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK413


Quant Time: Feb 15 22:07:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 15 22:06:10 2023
Response via : Initial Calibration

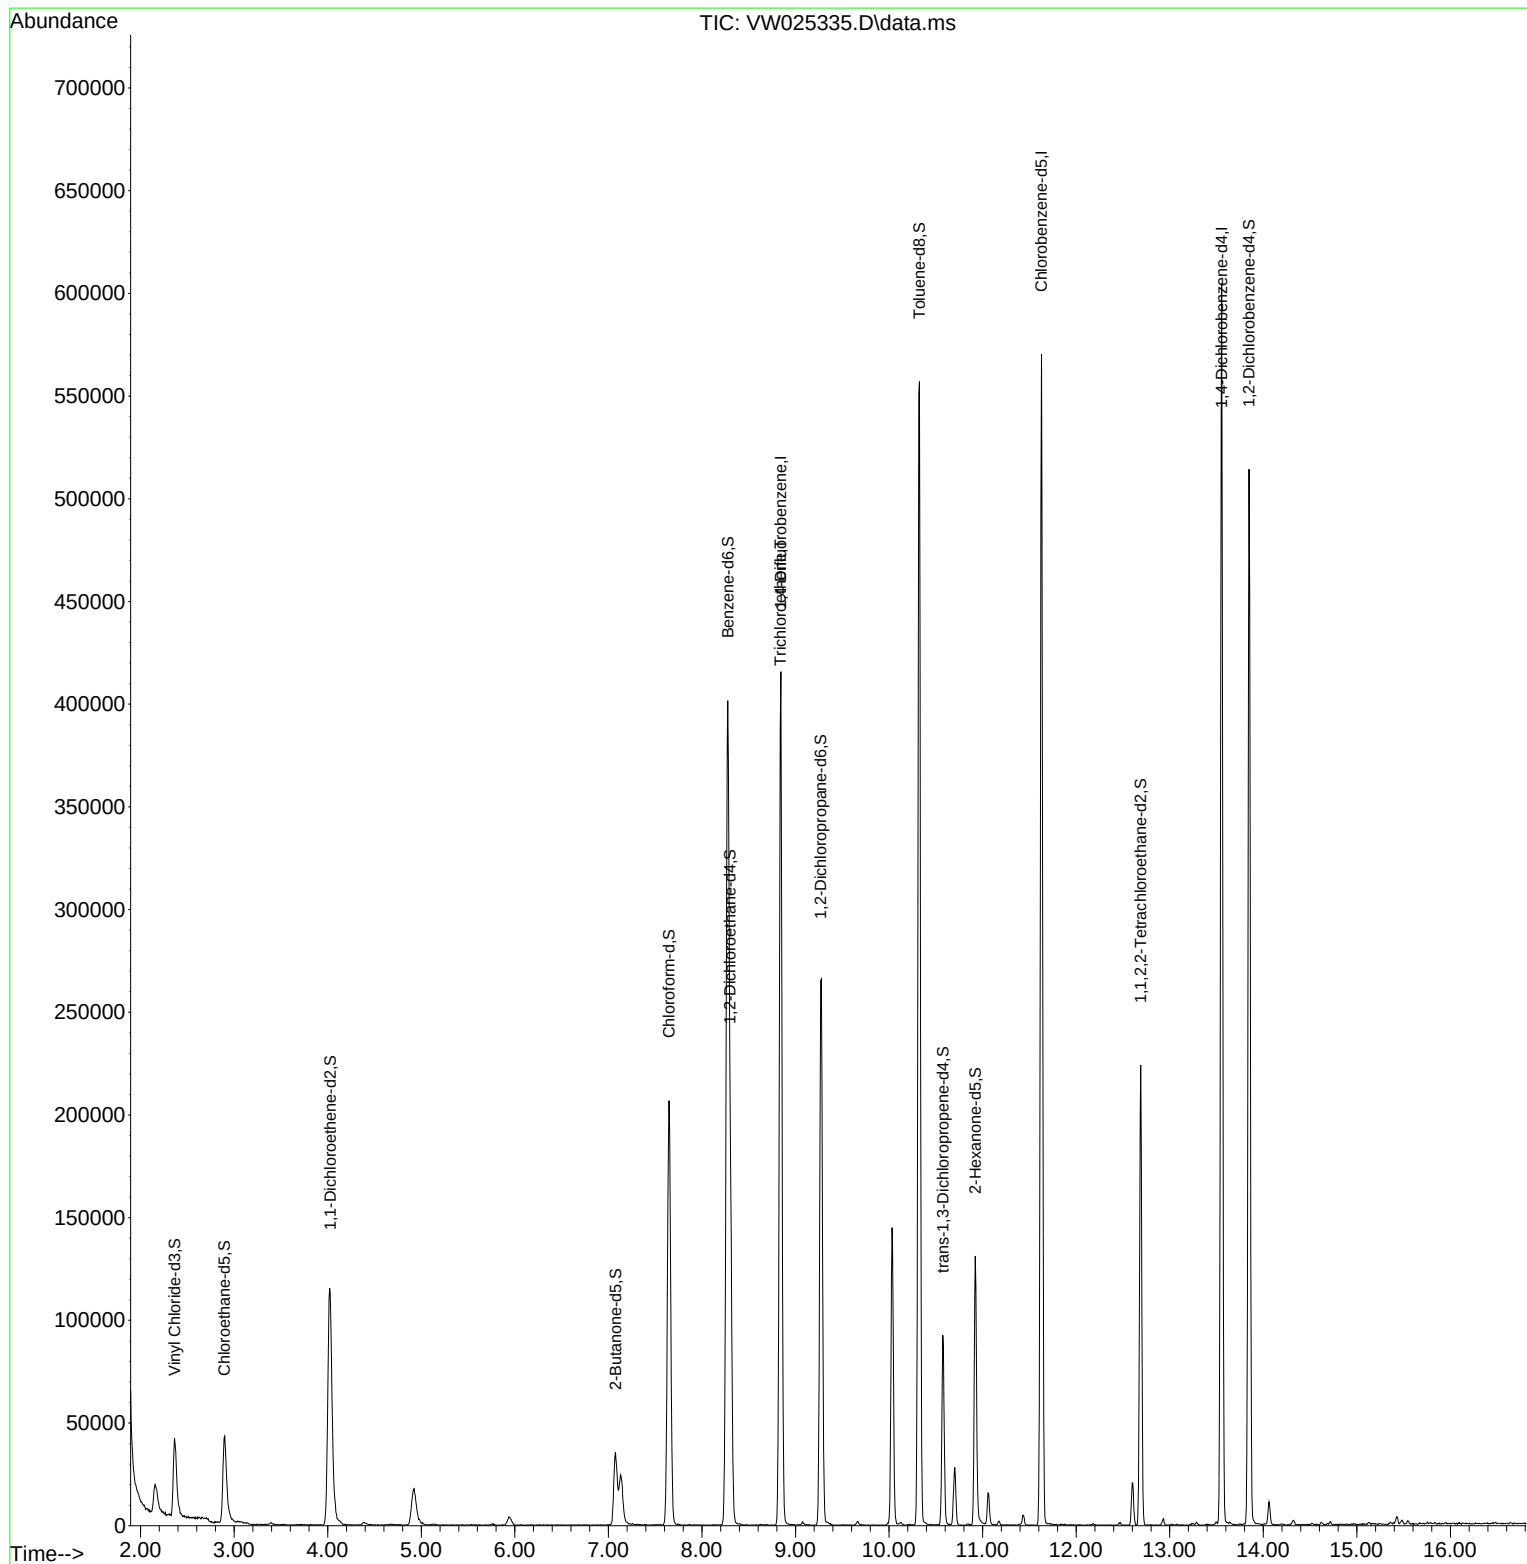

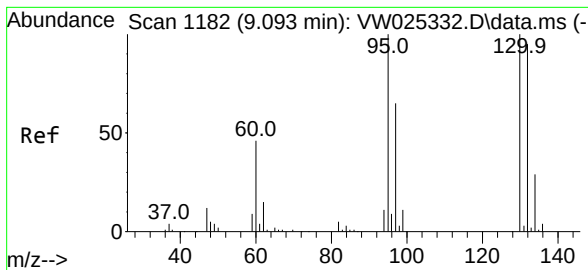

#34
 Trichloroethene
 Concen: 1.868 ug/L
 RT: 8.837 min Scan# 11
 Delta R.T. -0.256 min
 Lab File: VW025335.D
 Acq: 15 Feb 2023 13:25

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK413

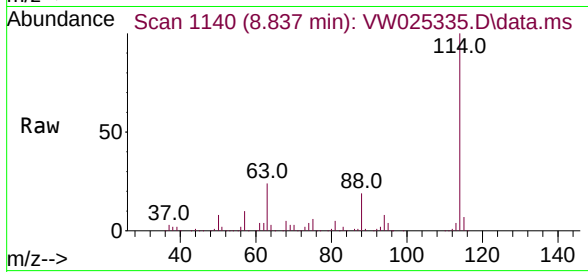

Tgt Ion: 95 Resp: 11202

Ion	Ratio	Lower	Upper
95	100		
97	0.0	45.4	84.2#
132	0.0	67.1	124.5#
130	0.0	69.2	128.6#

