

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
 Data File : VW025336.D
 Acq On : 15 Feb 2023 13:48
 Operator : SY/MD
 Sample : 01557-02
 Misc : 5.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1166

Quant Time: Feb 15 22:07:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 15 22:06:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	439223	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	389520	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	146660	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	60806	14.306	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.240%
7) Chloroethane-d5	2.899	69	61130	16.198	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.800%
11) 1,1-Dichloroethene-d2	4.021	63	129830	11.016	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	44.080%#
21) 2-Butanone-d5	7.075	46	61976	56.170	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.340%
24) Chloroform-d	7.648	84	213871	18.578	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.320%
26) 1,2-Dichloroethane-d4	8.307	65	121567	21.679	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.720%
32) Benzene-d6	8.270	84	411051	17.411	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.640%
36) 1,2-Dichloropropane-d6	9.270	67	125193	18.124	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	72.480%
41) Toluene-d8	10.319	98	370299	17.547	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.200%
43) trans-1,3-Dichloroprop...	10.575	79	53215	20.617	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.480%
47) 2-Hexanone-d5	10.922	63	49303	63.660	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.320%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	113136	24.085	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	104081	20.455	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.800%
Target Compounds					Qvalue	
13) Acetone	4.125	43	12396	10.189	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
Data File : VW025336.D
Acq On : 15 Feb 2023 13:48
Operator : SY/MD
Sample : 01557-02
Misc : 5.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C1166

Quant Time: Feb 15 22:07:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 15 22:06:10 2023
Response via : Initial Calibration

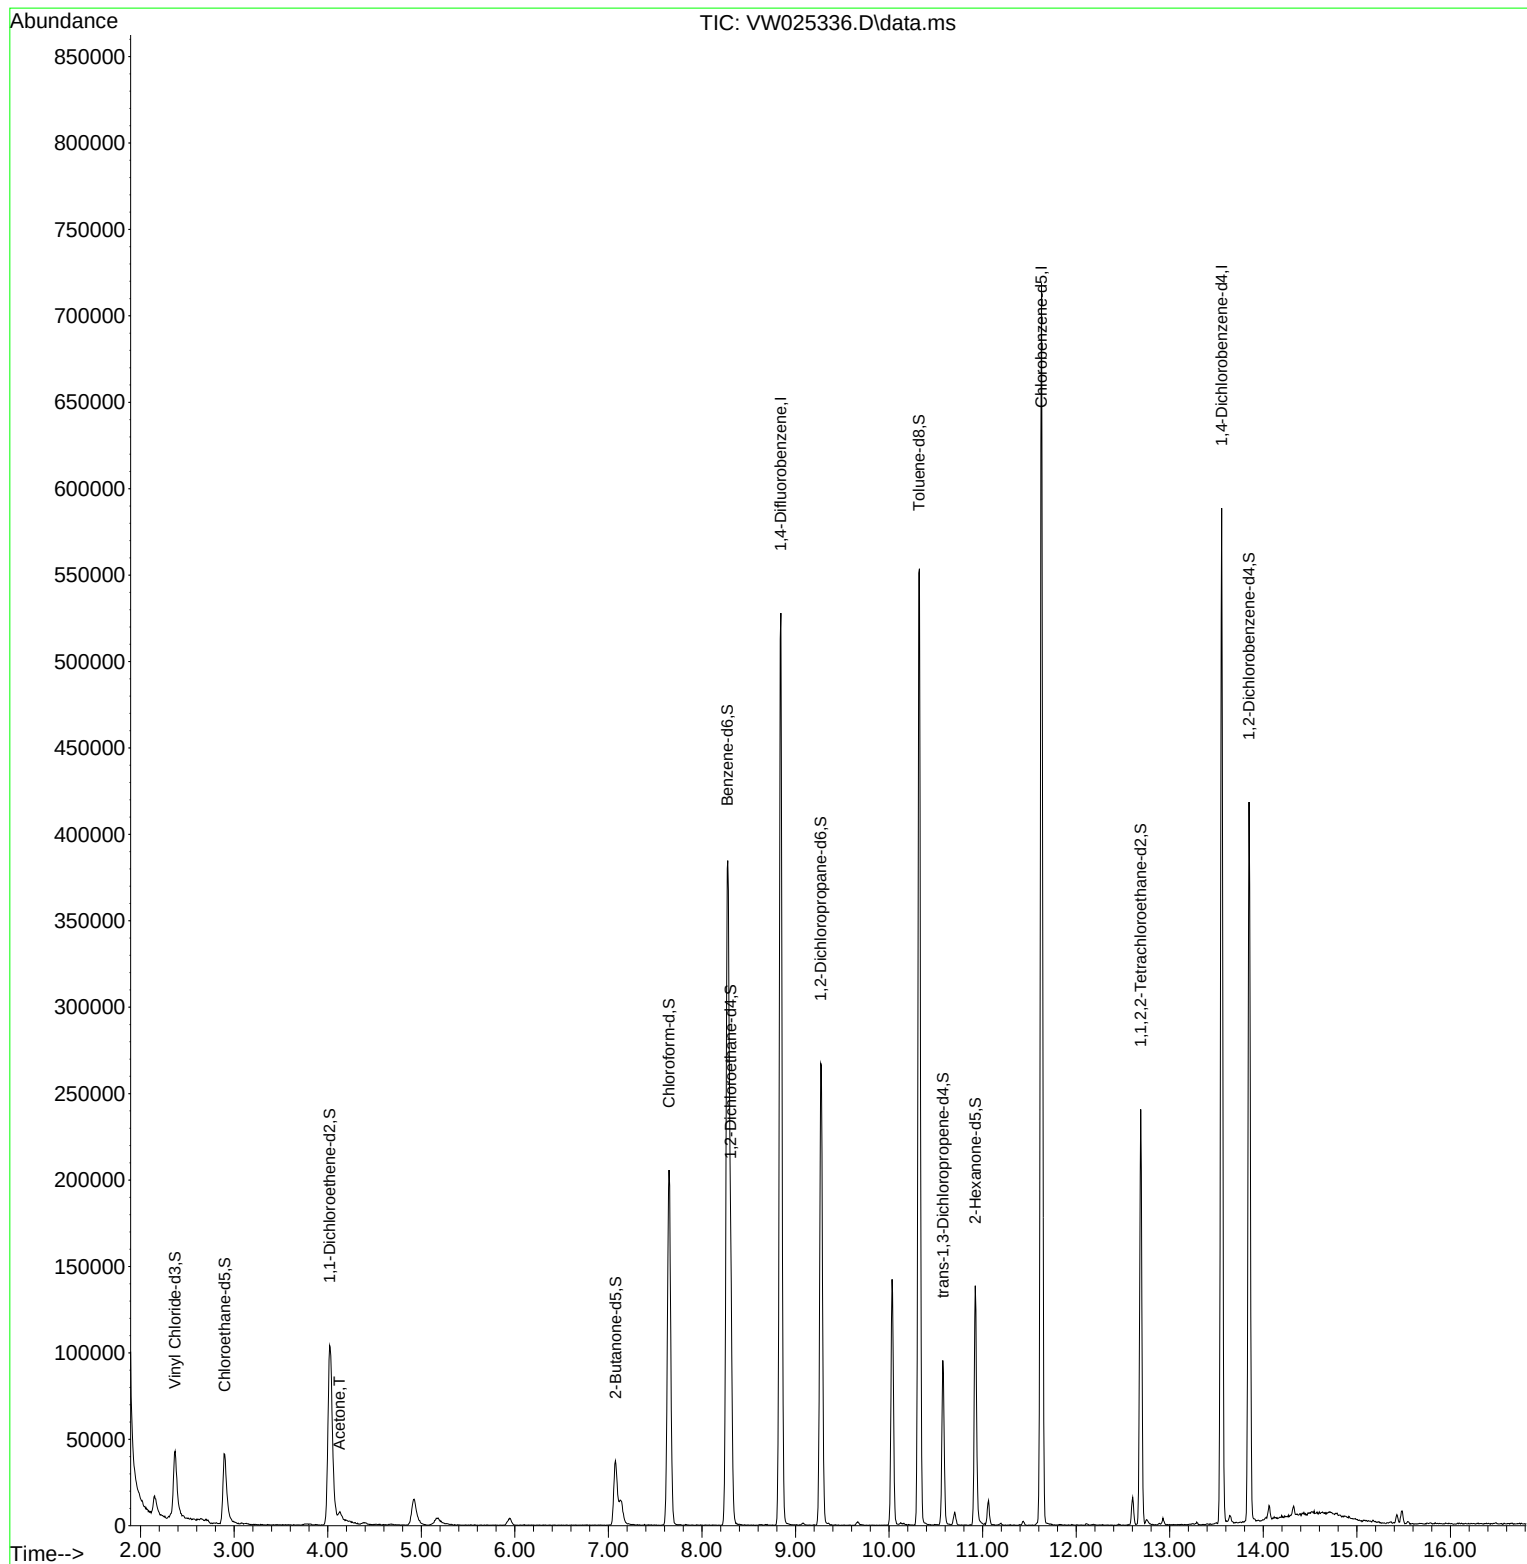

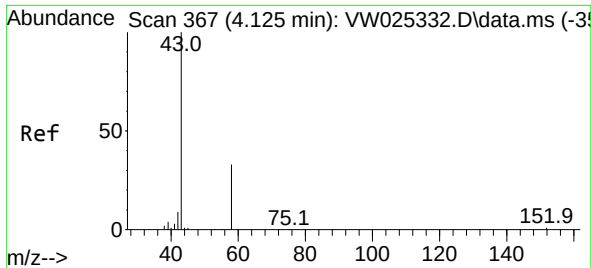

#13

Acetone

Concen: 10.189 ug/L

RT: 4.125 min Scan# 3

Delta R.T. -0.000 min

Lab File: VW025336.D


Acq: 15 Feb 2023 13:48

Instrument :

MSVOA_W

ClientSampleId :

C1166

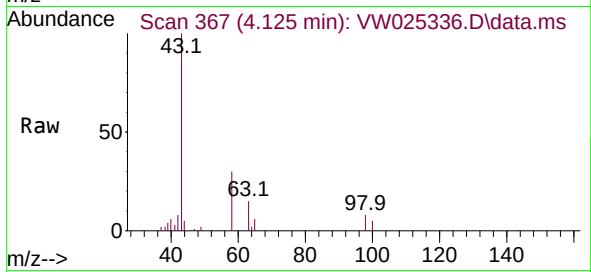

Tgt Ion: 43 Resp: 12396

Ion Ratio Lower Upper

43 100

58 23.9 0.0 63.0

