




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
Data File : VW025336.D
Acq On : 15 Feb 2023 13:48
Operator : SY/MD
Sample : 01557-02
Misc : 5.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C1166

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/16/2023
Supervised By :Mahesh Dadoda 02/20/2023

Quant Time: Feb 15 22:07:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 15 22:06:10 2023
Response via : Initial Calibration

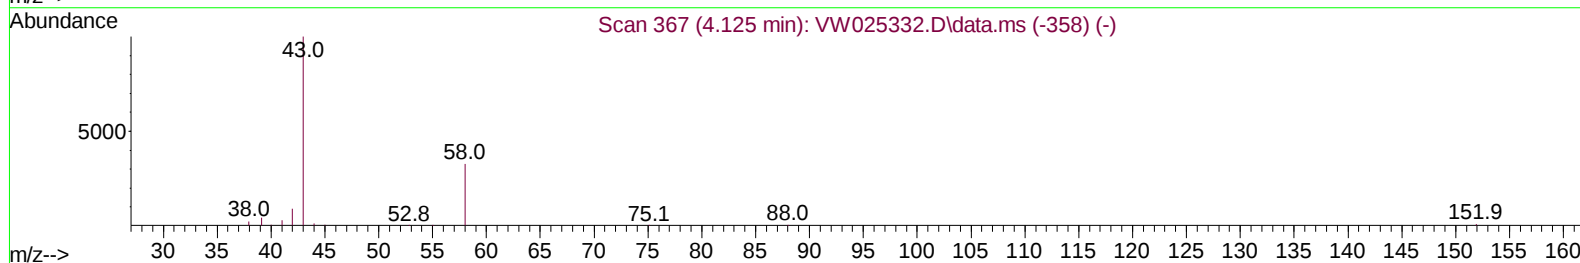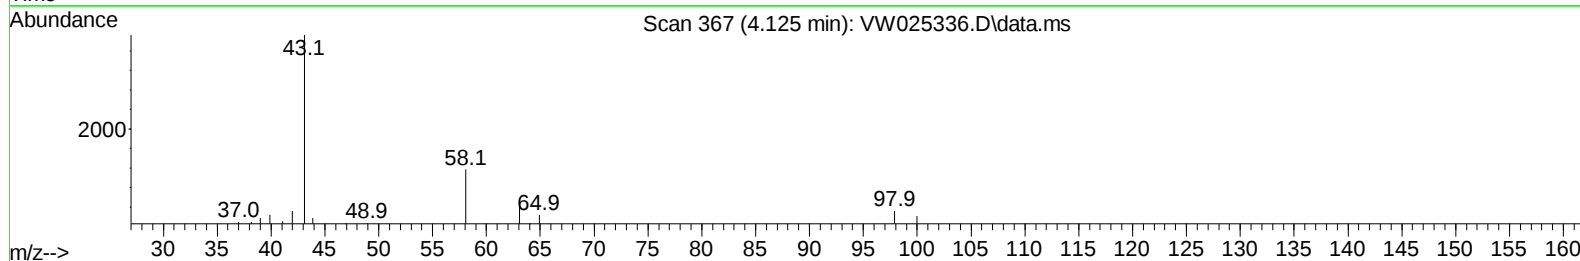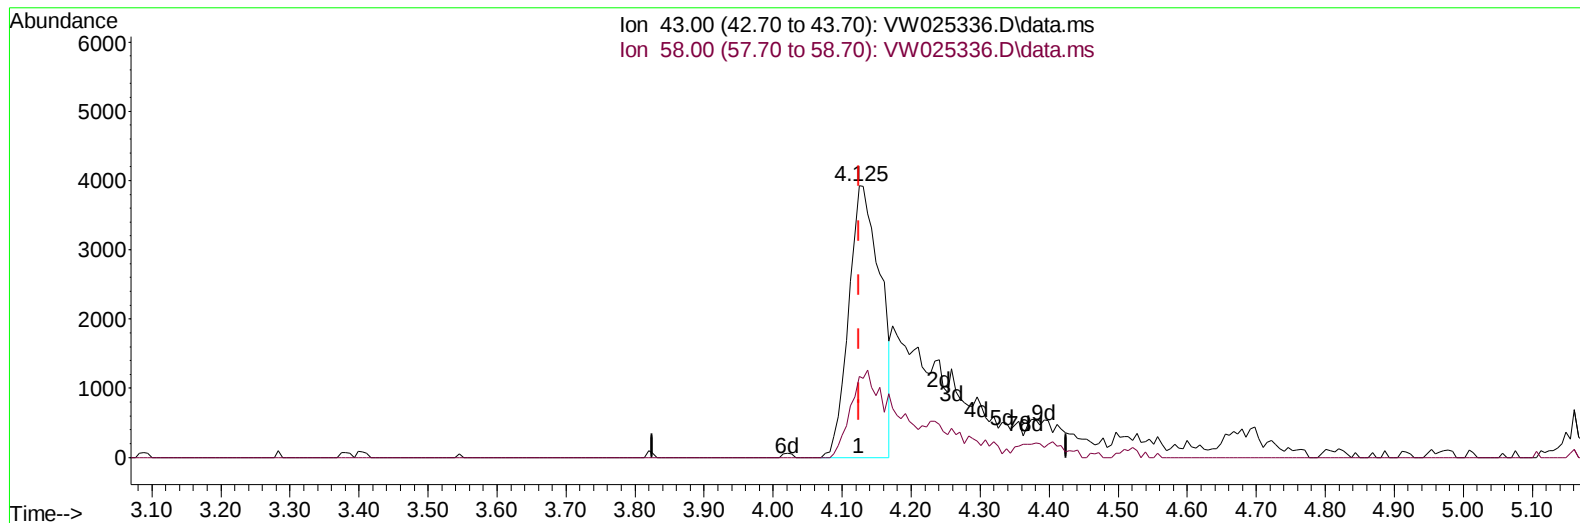

TIC: VW025336.D\data.ms

(13) Acetone (T)

4.125min (-0.000) 10.19 ug/L

response 12396

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	23.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
 Data File : VW025336.D
 Acq On : 15 Feb 2023 13:48
 Operator : SY/MD
 Sample : 01557-02
 Misc : 5.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1166

Manual IntegrationsAPPROVED

Quant Time: Feb 15 22:07:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 15 22:06:10 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/16/2023
 Supervised By :Mahesh Dadoda 02/20/2023

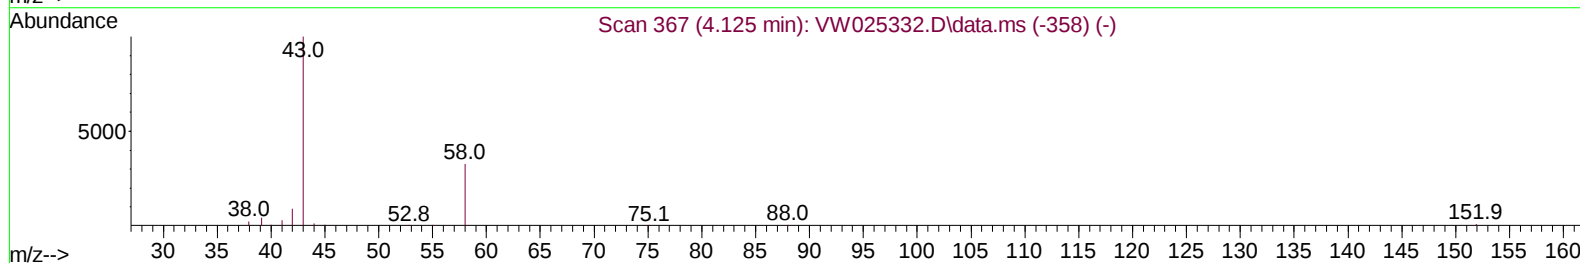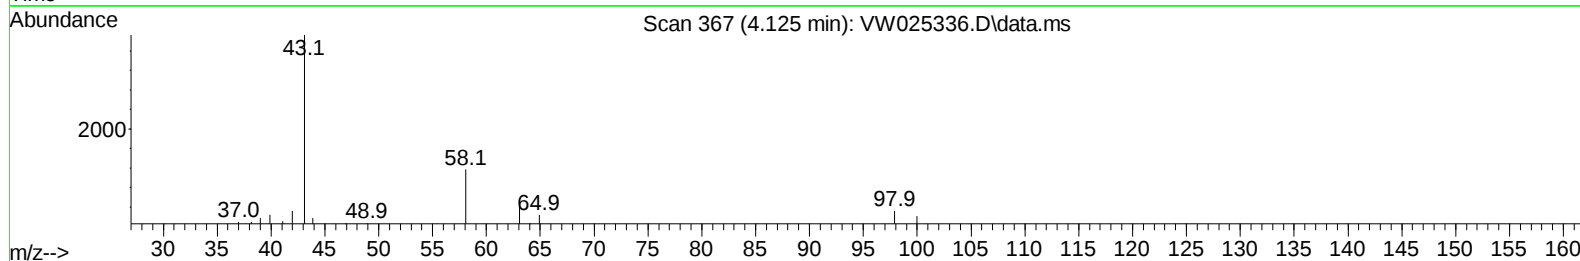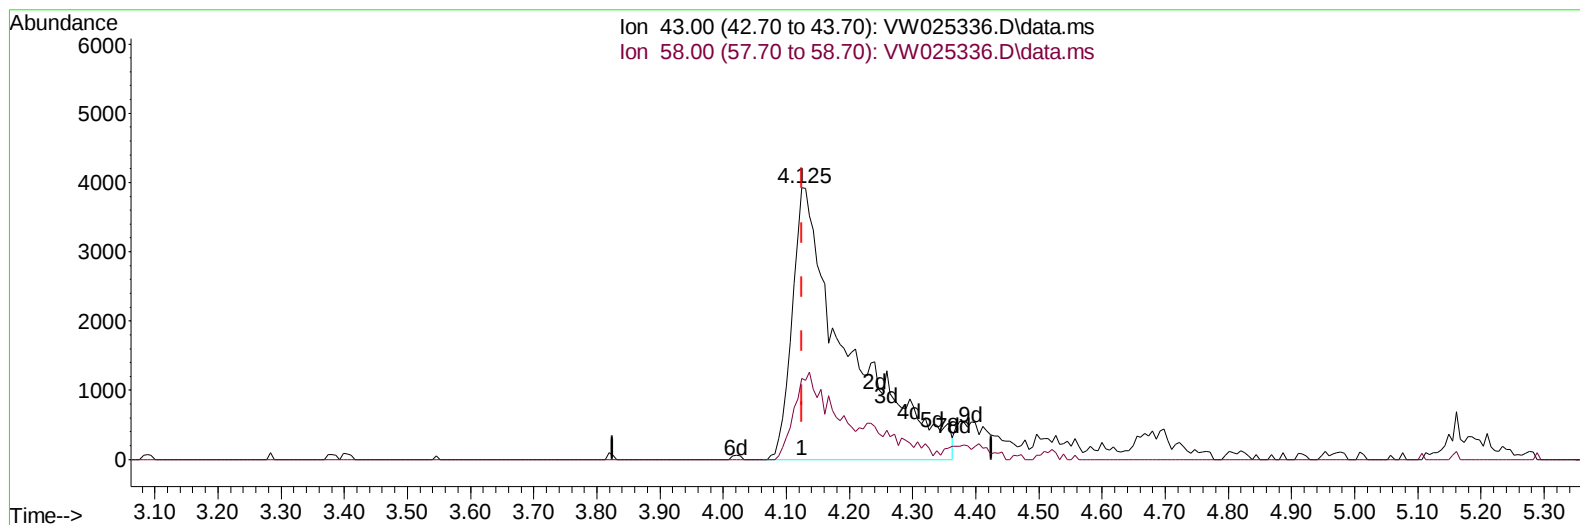

TIC: VW025336.D\data.ms

(13) Acetone (T)

4.125min (-0.000) 19.78 ug/L m

response 24060

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.50	12.33
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
 Data File : VW025336.D
 Acq On : 15 Feb 2023 13:48
 Operator : SY/MD
 Sample : 01557-02
 Misc : 5.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1166

Manual IntegrationsAPPROVED

Quant Time: Feb 15 22:07:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 15 22:06:10 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/16/2023
 Supervised By :Mahesh Dadoda 02/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		439223	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		389520	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		146660	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		60806	14.306	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	57.240%		
7) Chloroethane-d5	2.899	69		61130	16.198	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.800%		
11) 1,1-Dichloroethene-d2	4.021	63		129830	11.016	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	44.080%#		
21) 2-Butanone-d5	7.075	46		61976	56.170	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	112.340%		
24) Chloroform-d	7.648	84		213871	18.578	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	74.320%		
26) 1,2-Dichloroethane-d4	8.307	65		121567	21.679	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	86.720%		
32) Benzene-d6	8.270	84		411051	17.411	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	69.640%		
36) 1,2-Dichloropropane-d6	9.270	67		125193	18.124	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	72.480%		
41) Toluene-d8	10.319	98		370299	17.547	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	70.200%		
43) trans-1,3-Dichloroprop...	10.575	79		53215	20.617	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	82.480%		
47) 2-Hexanone-d5	10.922	63		49303	63.660	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	127.320%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		113136	24.085	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	96.320%		
66) 1,2-Dichlorobenzene-d4	13.848	152		104081	20.455	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	81.800%		
Target Compounds							
13) Acetone	4.125	43		24060m	19.776	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021523\
Data File : VW025336.D
Acq On : 15 Feb 2023 13:48
Operator : SY/MD
Sample : 01557-02
Misc : 5.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C1166

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/16/2023
Supervised By :Mahesh Dadoda 02/20/2023

Quant Time: Feb 15 22:07:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 15 22:06:10 2023
Response via : Initial Calibration

