
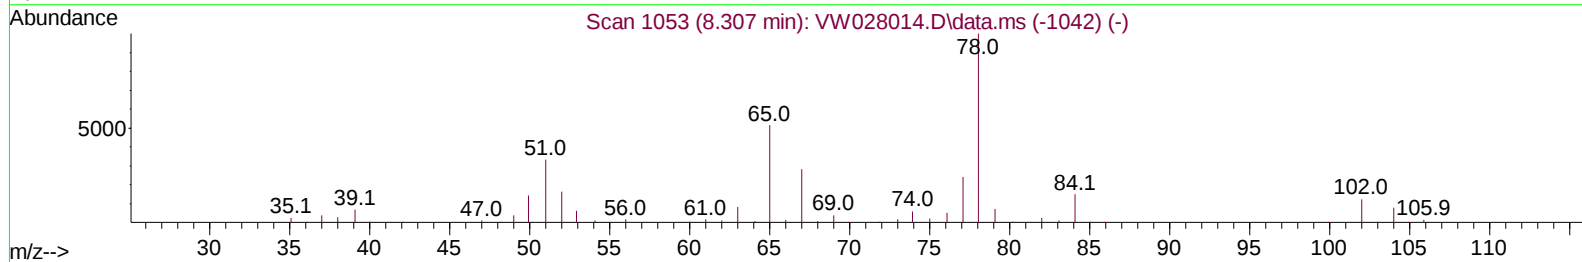
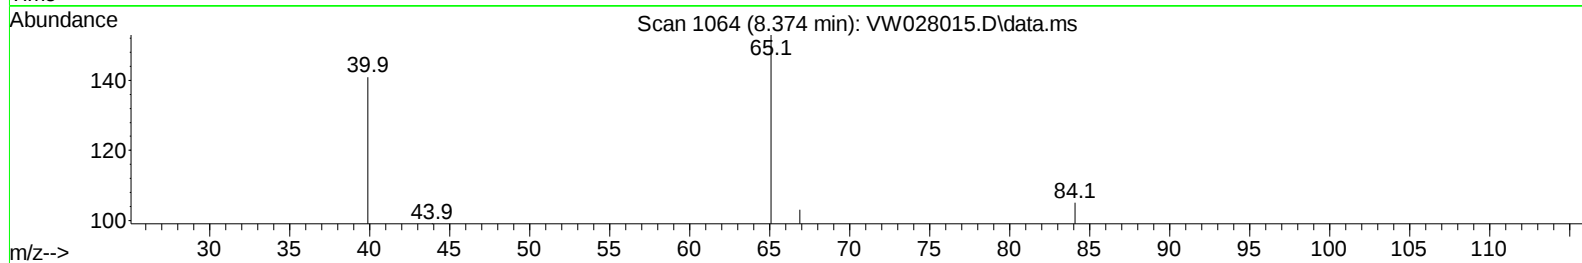


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021524\
Data File : VW028015.D
Acq On : 15 Feb 2024 10:45
Operator : SY/MD
Sample : VW0215SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 20:53:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 15 20:52:49 2024
Response via : Initial Calibration

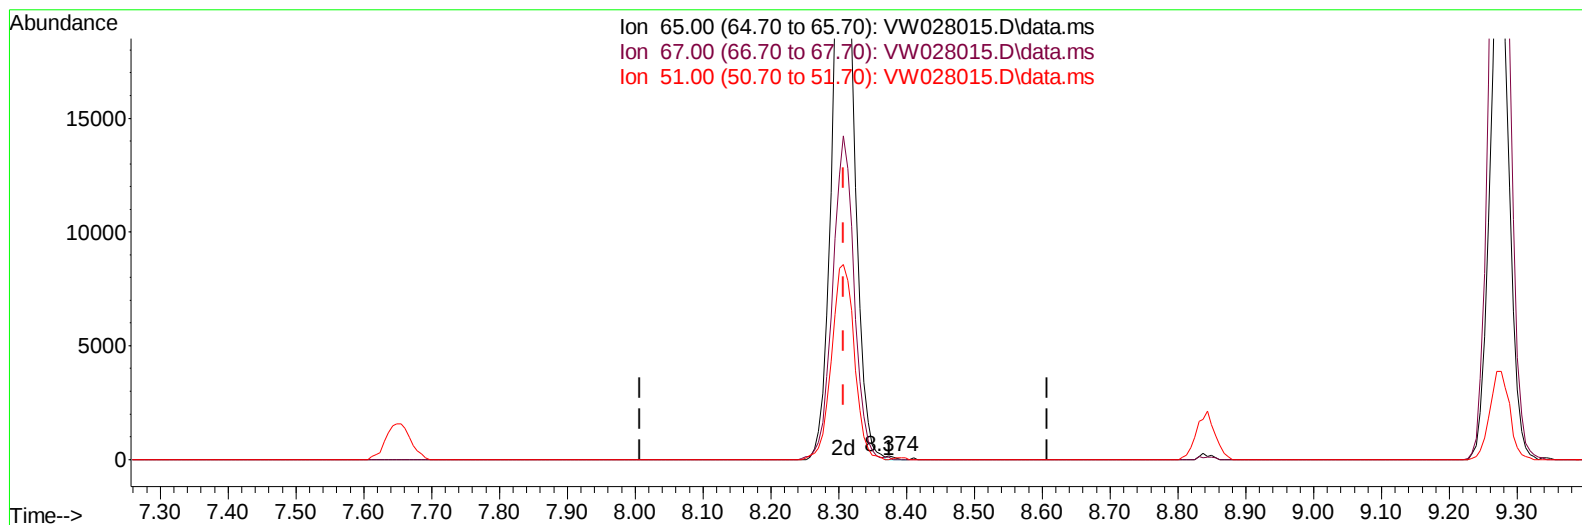

TIC: VW028015.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.374min (+ 0.067) 0.04 ug/L

response 119

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.20	66.39
51.00	88.70	88.24
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021524\
Data File : VW028015.D
Acq On : 15 Feb 2024 10:45
Operator : SY/MD
Sample : VW0215SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 20:53:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 15 20:52:49 2024
Response via : Initial Calibration

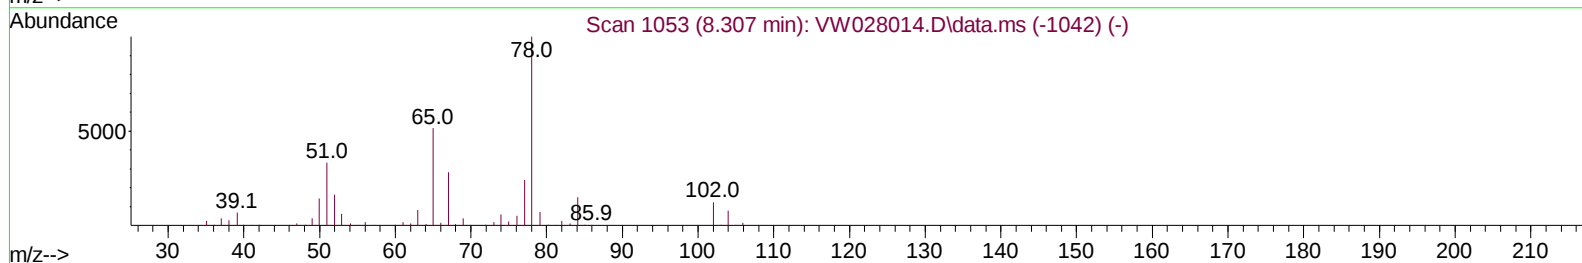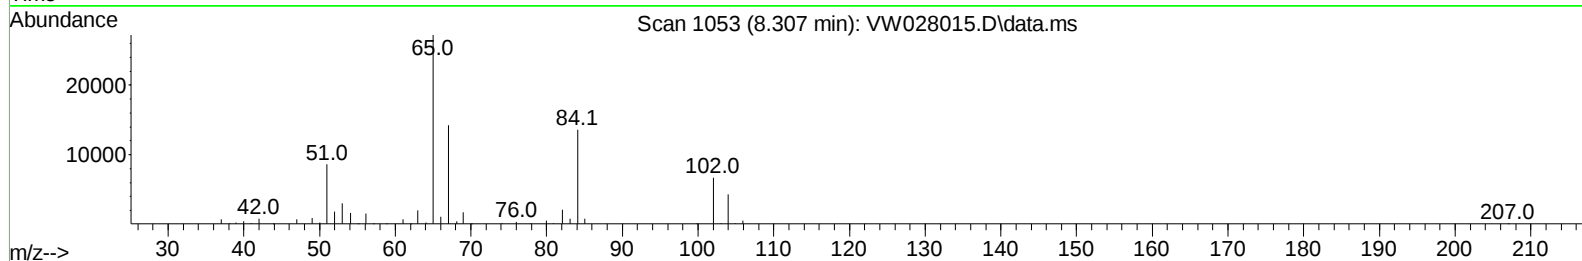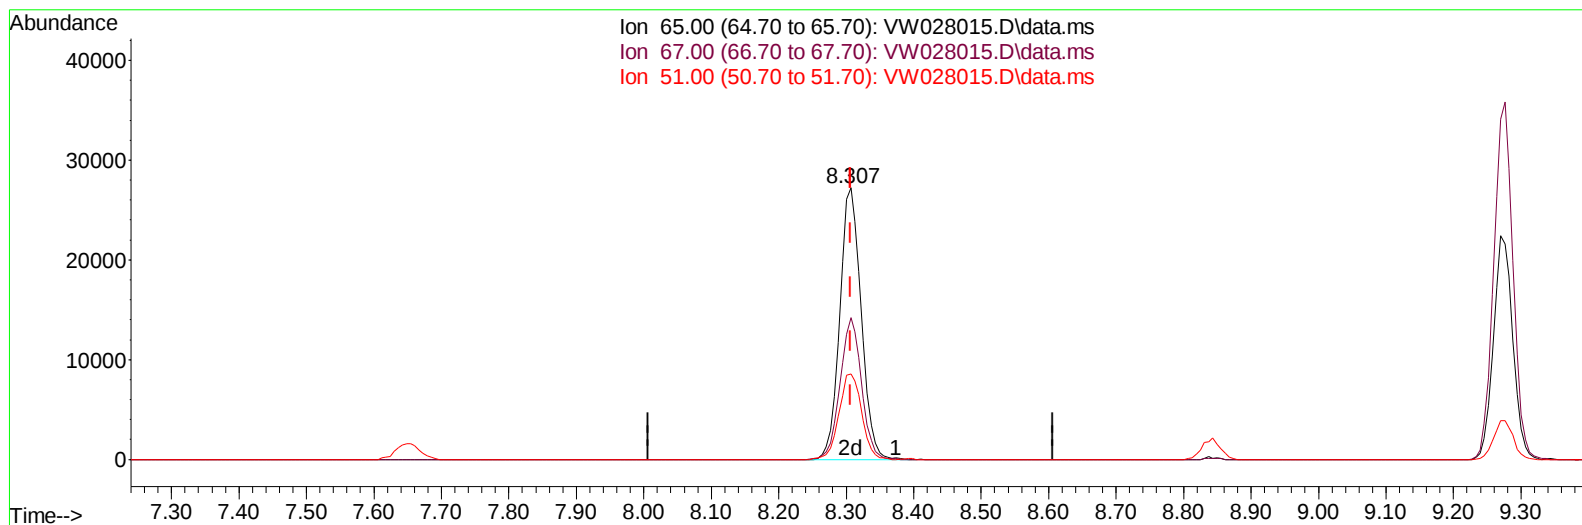

TIC: VW028015.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (+ 0.000) 21.07 ug/L m****response 59936**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.20	0.13#
51.00	88.70	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021524\
 Data File : VW028015.D
 Acq On : 15 Feb 2024 10:45
 Operator : SY/MD
 Sample : VW0215SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 20:53:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 15 20:52:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	269364	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	242115	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120502	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	58437	18.523	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.080%	
7) Chloroethane-d5	2.905	69	51056	21.336	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	85.360%	
11) 1,1-Dichloroethene-d2	4.021	65	25645	18.997	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	76.000%	
21) 2-Butanone-d5	7.075	46	21253	43.356	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	86.720%	
24) Chloroform-d	7.654	84	127658	20.268	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	81.080%	
26) 1,2-Dichloroethane-d4	8.307	65	59936m	21.070	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	84.280%	
32) Benzene-d6	8.276	84	263223	20.320	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.280%	
36) 1,2-Dichloropropane-d6	9.276	67	70721	20.136	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	80.560%	
41) Toluene-d8	10.325	98	253042	20.416	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	81.680%	
43) trans-1,3-Dichloroprop...	10.575	79	28530	19.752	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.000%	
47) 2-Hexanone-d5	10.922	63	19285	40.367	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	80.740%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	52020	19.816	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	79.280%	
66) 1,2-Dichlorobenzene-d4	13.848	152	87146	21.277	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	85.120%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021524\
Data File : VW028015.D
Acq On : 15 Feb 2024 10:45
Operator : SY/MD
Sample : VW0215SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 20:53:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 15 20:52:49 2024
Response via : Initial Calibration

