


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021524\
Data File : VW028013.D
Acq On : 15 Feb 2024 08:50
Operator : SY/MD
Sample : BFB437
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB437

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Thu Feb 15 20:52:49 2024

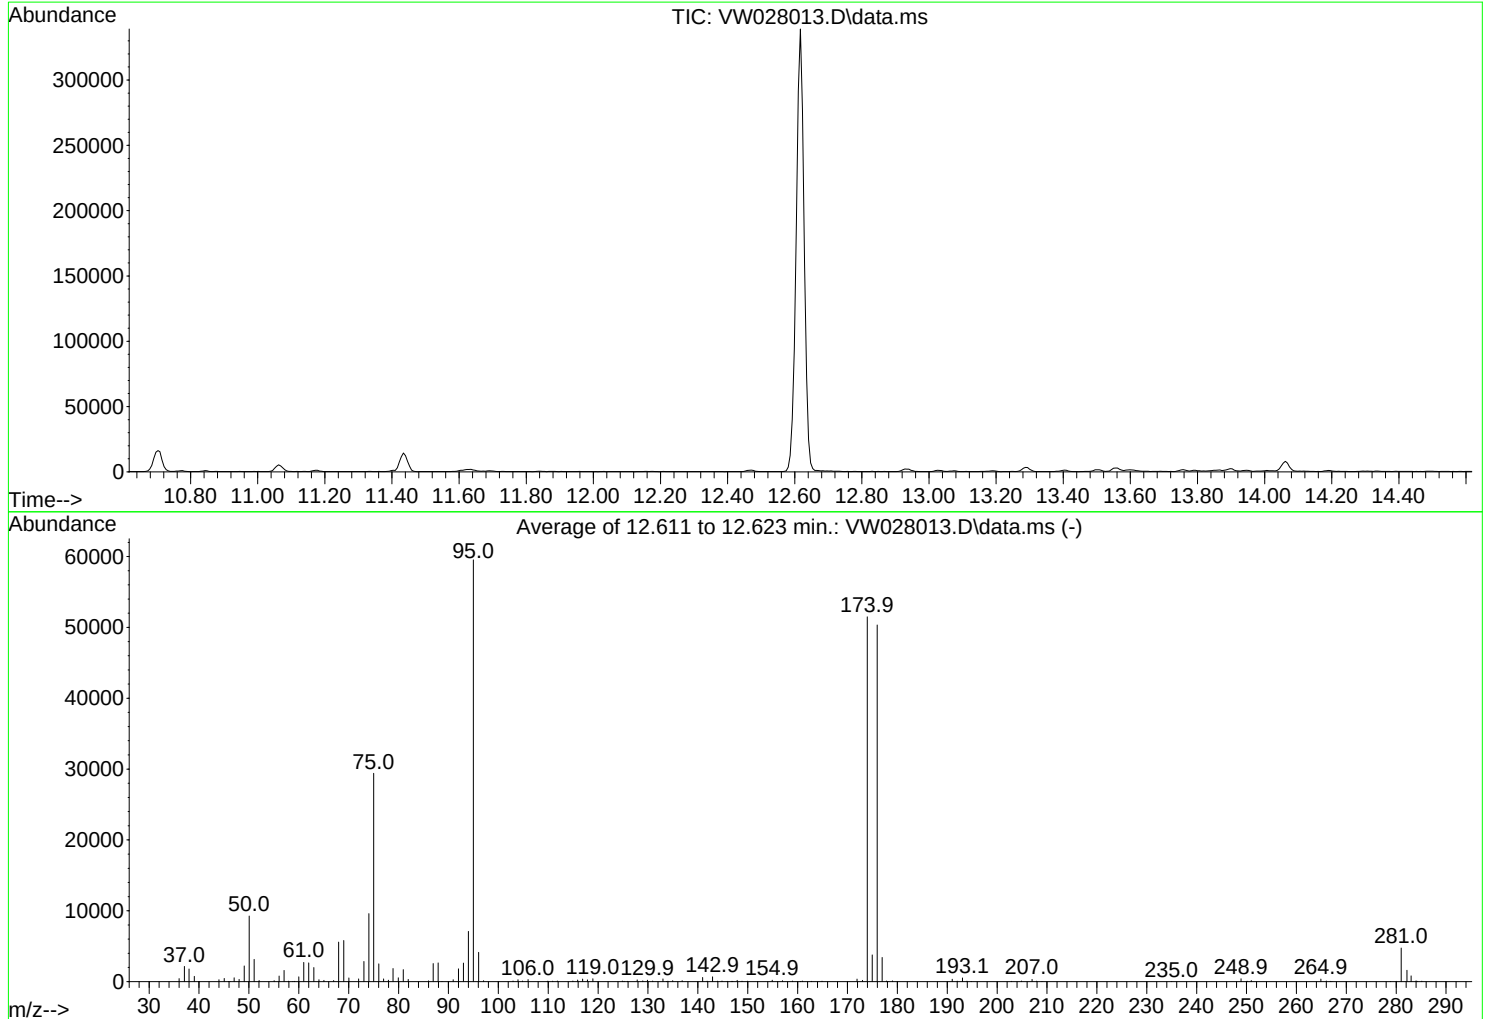

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9263	PASS
75	95	30	80	49.4	29400	PASS
95	95	100	100	100.0	59533	PASS
96	95	5	9	7.0	4145	PASS
173	174	0.00	2	0.4	187	PASS
174	95	50	120	86.5	51480	PASS
175	174	5	9	7.3	3763	PASS
176	174	95	101	97.8	50349	PASS
177	176	5	9	6.8	3401	PASS

Scan 1752 (12.568 min): VW028013.D\data.ms
BFB437

m/z	Abundance
39.90	211.0
44.00	115.0
281.00	94.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

m/z	Abundance
36.00	456.0
37.10	2128.0
38.00	1935.0
39.00	792.0
39.90	234.0
44.00	404.0
45.10	502.0
46.20	59.0
47.10	526.0
48.10	330.0
49.10	2257.0
50.10	9359.0
51.10	2909.0
52.00	163.0
55.10	139.0
56.00	705.0
57.00	1628.0
58.00	55.0
59.10	83.0
60.00	639.0
61.00	2662.0
62.00	2744.0
63.00	2115.0
64.00	234.0
65.00	253.0
67.10	166.0
68.00	5139.0
69.00	5904.0
70.00	494.0
72.00	384.0
73.10	3252.0
74.00	9397.0
75.00	28856.0
76.10	2548.0
77.00	472.0
77.90	278.0
78.90	1890.0
80.00	505.0
80.90	1608.0
81.90	328.0
85.90	125.0
86.90	2407.0
88.00	2343.0
91.00	240.0
92.00	1684.0
93.00	2550.0
94.00	6682.0
95.00	55528.0
96.10	4048.0
97.00	157.0
103.00	202.0
104.00	261.0
104.90	100.0
105.90	256.0
109.80	124.0
110.90	55.0
111.90	82.0
114.90	133.0
115.90	239.0
116.90	336.0
117.90	273.0
118.90	522.0
124.90	179.0
125.90	60.0
127.90	266.0
129.00	86.0
129.90	203.0
131.00	131.0
133.00	625.0
134.00	197.0
134.90	190.0
136.90	141.0
140.90	500.0
141.80	56.0
143.00	643.0
144.00	55.0
144.90	75.0
146.80	143.0
147.90	104.0
149.00	86.0
154.90	224.0
156.90	123.0
159.00	136.0
160.90	123.0
162.80	116.0
164.90	160.0
171.90	345.0
173.90	47896.0
175.00	3603.0
176.00	42416.0
177.00	3071.0
177.90	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

179.00	205.0
191.00	555.0
192.00	143.0
193.00	893.0
193.90	128.0
202.90	125.0
204.90	213.0
207.00	533.0
208.00	139.0
209.00	86.0
235.00	87.0
248.90	623.0
250.10	110.0
251.00	296.0
264.90	538.0
266.00	165.0
266.80	142.0
278.90	63.0
280.00	149.0
281.00	6886.0
282.10	2760.0
283.00	1467.0
284.00	332.0
285.10	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

m/z	Abundance
36.00	422.0
37.00	2519.0
38.00	1921.0
39.10	823.0
39.90	179.0
44.10	400.0
45.10	430.0
47.10	553.0
48.00	372.0
49.00	2479.0
50.00	10470.0
51.00	3681.0
52.10	192.0
55.00	137.0
56.00	971.0
57.10	1577.0
57.90	68.0
58.80	54.0
59.20	63.0
60.00	746.0
61.00	3148.0
62.00	2815.0
63.00	2335.0
64.10	331.0
65.10	210.0
67.00	152.0
68.00	6606.0
69.00	6331.0
70.10	556.0
72.00	430.0
73.10	2929.0
74.10	10642.0
75.00	32248.0
76.00	2861.0
77.00	396.0
78.00	190.0
78.90	2079.0
80.00	574.0
80.90	1925.0
82.00	354.0
86.00	116.0
86.90	2826.0
88.00	3059.0
90.90	339.0
92.00	2044.0
93.00	2736.0
94.00	8093.0
95.00	66304.0
96.00	4703.0
97.10	175.0
102.80	60.0
103.90	283.0
104.80	81.0
105.90	430.0
110.00	115.0
110.90	81.0
111.80	65.0
115.00	65.0
115.90	256.0
116.90	435.0
117.80	276.0
119.00	355.0
124.80	117.0
125.20	110.0
125.90	76.0
127.90	203.0
128.90	137.0
129.90	208.0
130.90	89.0
133.00	325.0
135.00	127.0
136.90	113.0
140.90	641.0
141.80	58.0
143.00	660.0
143.90	82.0
144.80	92.0
145.90	78.0
147.00	75.0
147.90	256.0
148.80	68.0
149.90	113.0
152.00	52.0
154.90	213.0
156.90	159.0
159.00	100.0
161.00	157.0
164.80	50.0
171.90	403.0
173.00	560.0
173.90	57768.0
174.90	4041.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

175.90	59416.0
176.90	3862.0
177.70	139.0
179.00	106.0
191.00	379.0
192.00	69.0
193.10	482.0
194.00	72.0
194.80	56.0
204.90	89.0
207.00	342.0
207.90	92.0
248.90	354.0
250.10	93.0
250.90	129.0
264.90	411.0
266.00	82.0
267.10	96.0
281.00	5450.0
282.20	1303.0
283.00	655.0
284.20	140.0
285.20	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

m/z	Abundance
36.00	395.0
37.00	1787.0
38.00	1515.0
39.00	603.0
40.00	230.0
44.10	384.0
45.00	394.0
45.90	97.0
47.00	568.0
48.00	261.0
49.00	1910.0
50.00	7960.0
51.00	2810.0
52.10	143.0
55.00	149.0
56.10	711.0
57.00	1524.0
58.00	53.0
60.00	621.0
61.00	2334.0
62.00	2344.0
63.00	1501.0
64.00	262.0
65.10	104.0
66.90	152.0
68.00	5025.0
69.00	5199.0
70.00	519.0
72.00	365.0
73.00	2353.0
74.00	8752.0
75.00	27096.0
76.00	2100.0
77.00	314.0
78.00	142.0
78.90	1577.0
79.90	523.0
81.00	1557.0
82.00	279.0
86.10	88.0
87.00	2422.0
87.90	2509.0
88.70	69.0
91.00	211.0
92.00	1686.0
93.00	2607.0
94.00	6497.0
95.00	56768.0
96.00	3685.0
97.00	62.0
104.00	246.0
104.90	77.0
106.00	229.0
109.90	78.0
110.90	59.0
111.80	92.0
114.90	103.0
115.90	202.0
116.90	337.0
117.90	231.0
118.90	345.0
127.80	285.0
128.90	151.0
129.90	201.0
130.90	86.0
132.90	225.0
133.70	52.0
134.90	124.0
136.80	134.0
141.00	620.0
141.90	80.0
142.90	713.0
143.90	55.0
144.80	93.0
145.90	57.0
147.00	80.0
147.90	174.0
148.80	65.0
150.00	119.0
154.90	158.0
156.00	60.0
157.00	160.0
158.80	57.0
160.60	50.0
171.90	339.0
174.00	48776.0
174.90	3644.0
176.00	49216.0
177.00	3270.0
178.10	96.0
179.00	61.0
191.00	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

193.00	186.0
206.90	96.0
249.00	220.0
251.10	65.0
265.00	144.0
281.10	2151.0
282.00	732.0
283.00	345.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437