

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021621\
 Data File : VW018163.D
 Acq On : 16 Feb 2021 15:27
 Operator : SY/VA
 Sample : M1414-05
 Misc : 6.94G/10ML/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBGX1

Manual Integrations
 APPROVED

MMDadoda
 2/18/2021 11:54:26 AM

Quant Time: Feb 17 01:06:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 17 01:02:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	40417	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	37583	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	17865	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	6663	13.26	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	53.04%		
7) Chloroethane-d5	2.885	69	7982	20.02	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.08%		
10) 1,1-Dichloroethene-d2	4.019	63	13424	13.37	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	53.48%		
20) 2-Butanone-d5	7.085	46	3619	27.00	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	54.00%		
24) Chloroform-d	7.652	84	22619	21.33	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.32%		
26) 1,2-Dichloroethane-d4	8.305	65	11689	20.69	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	82.76%		
29) Benzene-d6	8.274	84	42362	20.53	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.12%		
33) 1,2-Dichloropropane-d6	9.274	67	12774	22.13	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.52%		
37) Toluene-d8	10.323	98	37313	19.00	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.00%		
38) trans-1,3-Dichloroprop...	10.579	79	4668	17.84	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.36%		
39) 2-Hexanone-d5	10.920	63	3513	31.84	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	63.68%		
48) 1,1,2,2-Tetrachloroeth...	12.688	84	10430	20.57	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	82.28%		
61) 1,2-Dichlorobenzene-d4	13.853	152	15560	24.42	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.68%		
Target Compounds						Qvalue
13) Acetone	4.147	43	805m	8.12	ug/L	
16) Methylene chloride	4.921	84	2079	3.21	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021621\
Data File : VW018163.D
Acq On : 16 Feb 2021 15:27
Operator : SY/VA
Sample : M1414-05
Misc : 6.94G/10ML/MSVOA_W/SOIL
ALS Vial : 16 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampled :
DBGX1

Manual Integrations
APPROVED

MMDadoda
2/18/2021 11:54:26 AM


Quant Time: Feb 17 01:06:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 17 01:02:43 2021
Response via : Initial Calibration

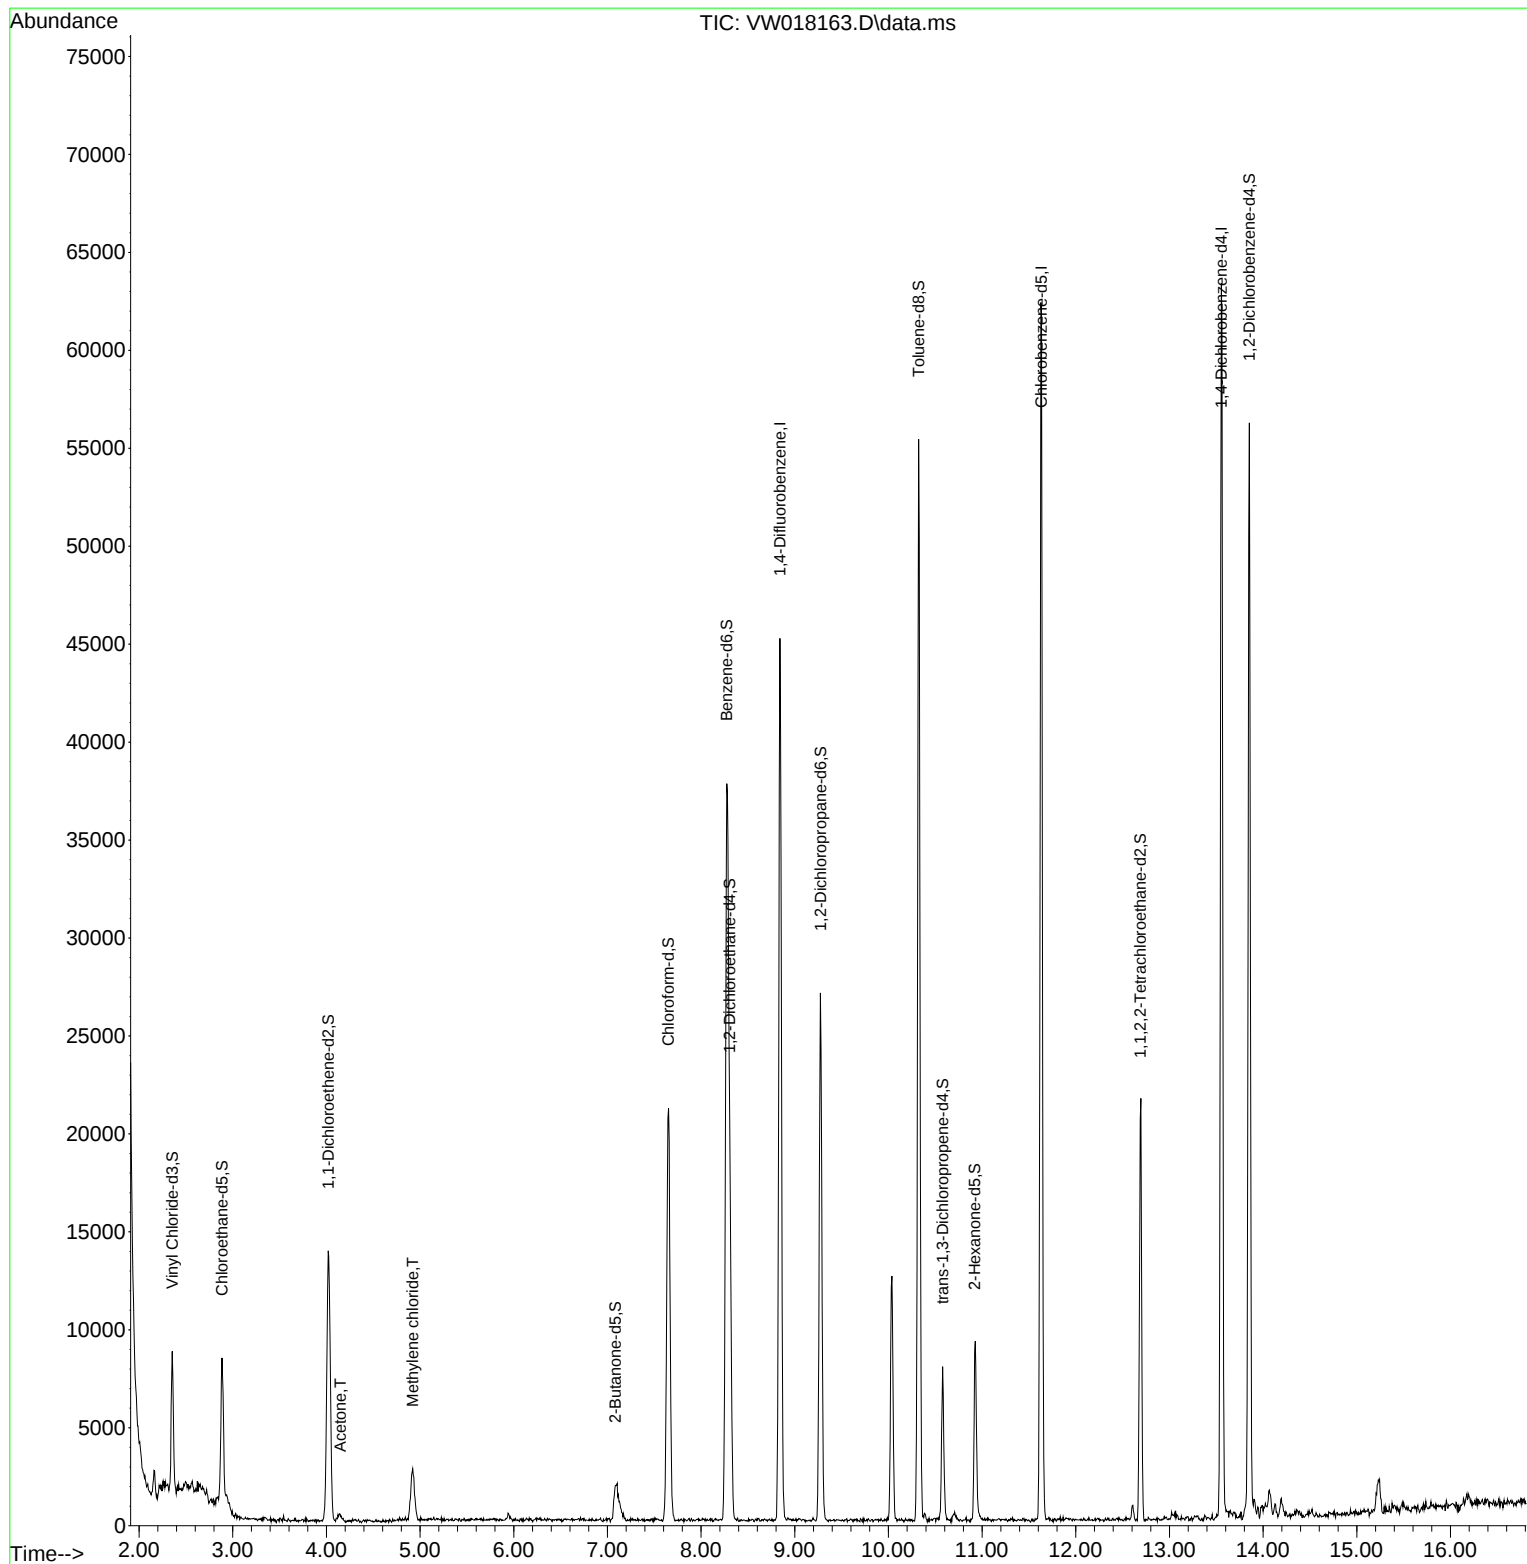



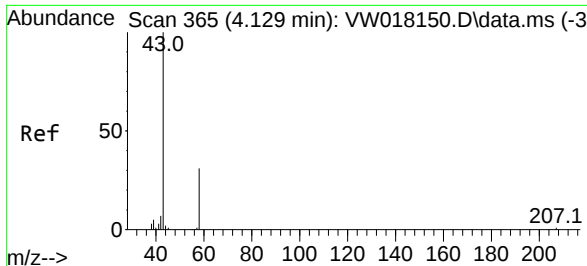


#13
Acetone
Concen: 8.12 ug/L m
RT: 4.147 min Scan# 368
Delta R.T. 0.018 min
Lab File: VW018163.D
Acq: 16 Feb 2021 15:27

Instrument :
MSVOA_W
ClientSampleId :
DBGX1

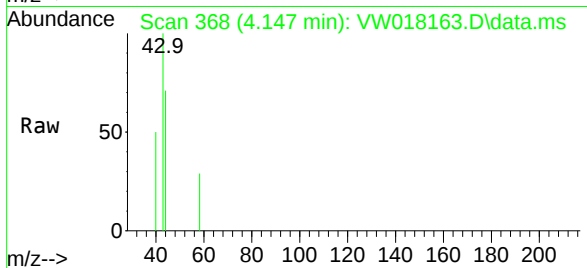

Tgt Ion: 43 Resp: 805
Ion Ratio Lower Upper
43 100
58 21.6 0.0 68.4

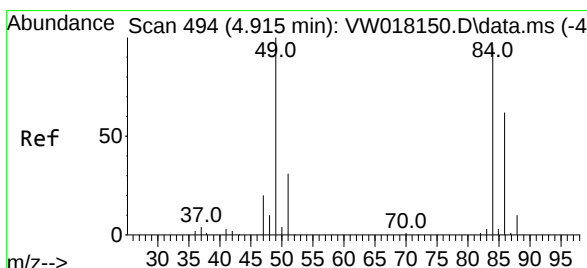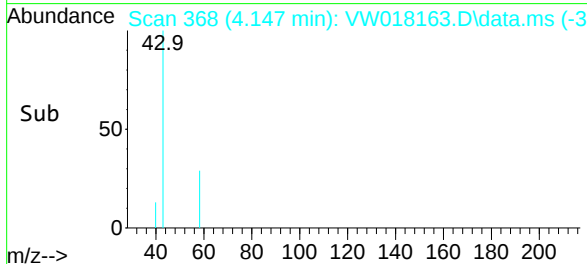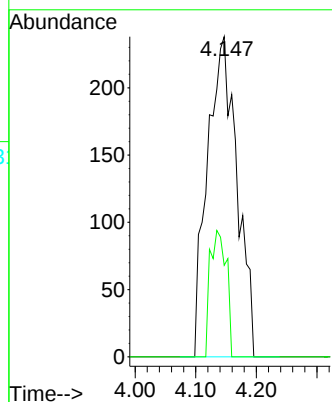

#16
Methylene chloride
Concen: 3.21 ug/L
RT: 4.921 min Scan# 495
Delta R.T. 0.006 min
Lab File: VW018163.D
Acq: 16 Feb 2021 15:27

Tgt Ion: 84 Resp: 2079
Ion Ratio Lower Upper
84 100
49 97.9 81.2 150.8
86 68.9 44.5 82.7

