
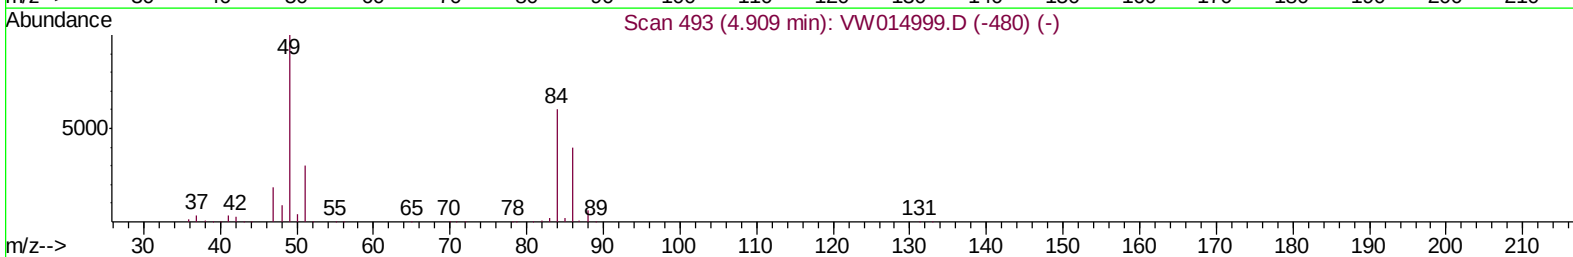
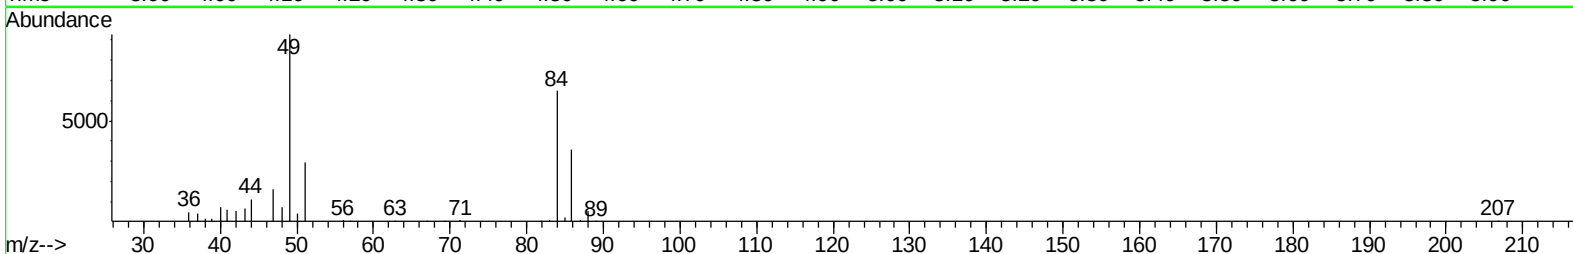


Data File : VW015000.D
Acq On : 17 Feb 2020 12:51
Operator : SY/VA
Sample : VW0217SBL07
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:22:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SFAMWLM021320SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Feb 18 04:18:26 2020
Response via : Initial Calibration

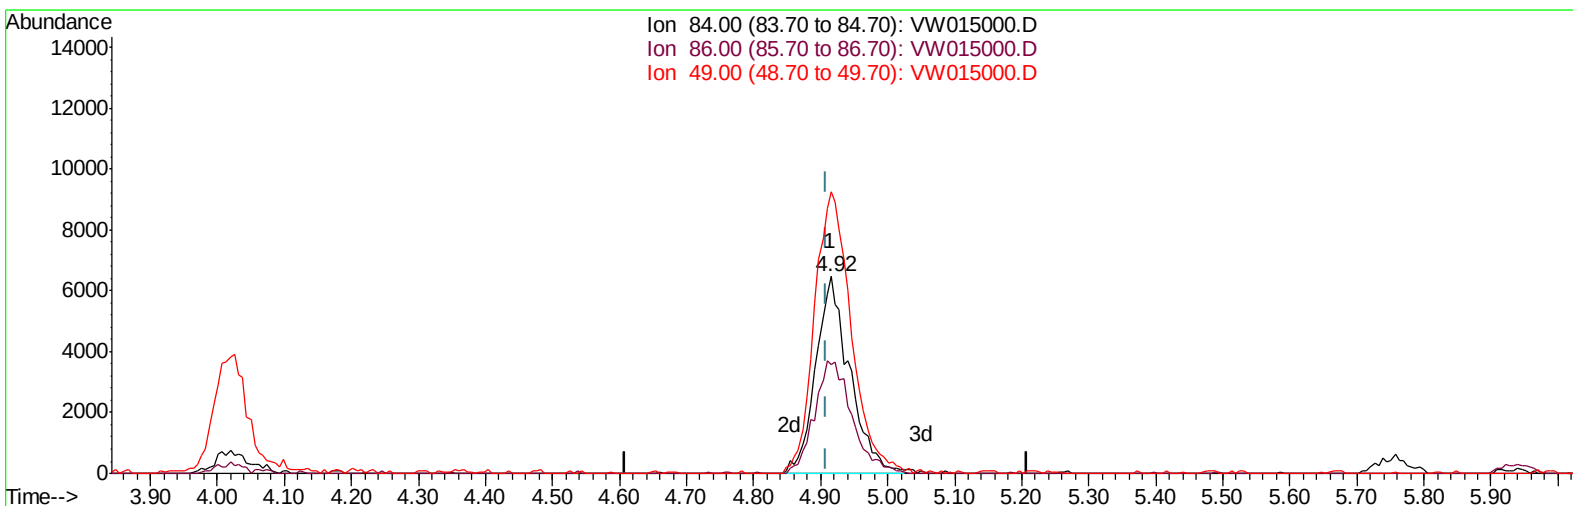

TIC: VW015000.D

(16) Methylene chloride (T)

4.916min (+0.006) 1.62ug/L m

response 22784

Ion	Exp%	Act%
84.00	100	100
86.00	63.40	55.27
49.00	155.70	143.26
0.00	0.00	0.00