

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021723\
 Data File : VW025343.D
 Acq On : 17 Feb 2023 13:40
 Operator : SY/MD
 Sample : 01557-04
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Feb 18 01:22:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Feb 15 22:06:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	362146	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	323798	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	156414	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	73059	20.848	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.400%
7) Chloroethane-d5	2.893	69	60547	19.458	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.840%
11) 1,1-Dichloroethene-d2	4.021	63	138485	14.251	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.000%
21) 2-Butanone-d5	7.075	46	45148	49.627	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.260%
24) Chloroform-d	7.648	84	189456	19.960	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.840%
26) 1,2-Dichloroethane-d4	8.380	65	66	0.014	ug/L	0.07
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.270	84	390028	19.874	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.480%
36) 1,2-Dichloropropane-d6	9.270	67	109866	19.134	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.520%
41) Toluene-d8	10.318	98	359731	20.506	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.040%
43) trans-1,3-Dichloroprop...	10.575	79	49865	23.241	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.960%
47) 2-Hexanone-d5	10.922	63	36142	56.138	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.280%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	87724	22.465	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.880%
66) 1,2-Dichlorobenzene-d4	13.854	152	108983	20.083	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.320%
Target Compounds						Qvalue
34) Trichloroethene	8.843	95	11256	1.793	ug/L	# 5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021723\
Data File : VW025343.D
Acq On : 17 Feb 2023 13:40
Operator : SY/MD
Sample : 01557-04
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001


Quant Time: Feb 18 01:22:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Feb 15 22:06:10 2023
Response via : Initial Calibration

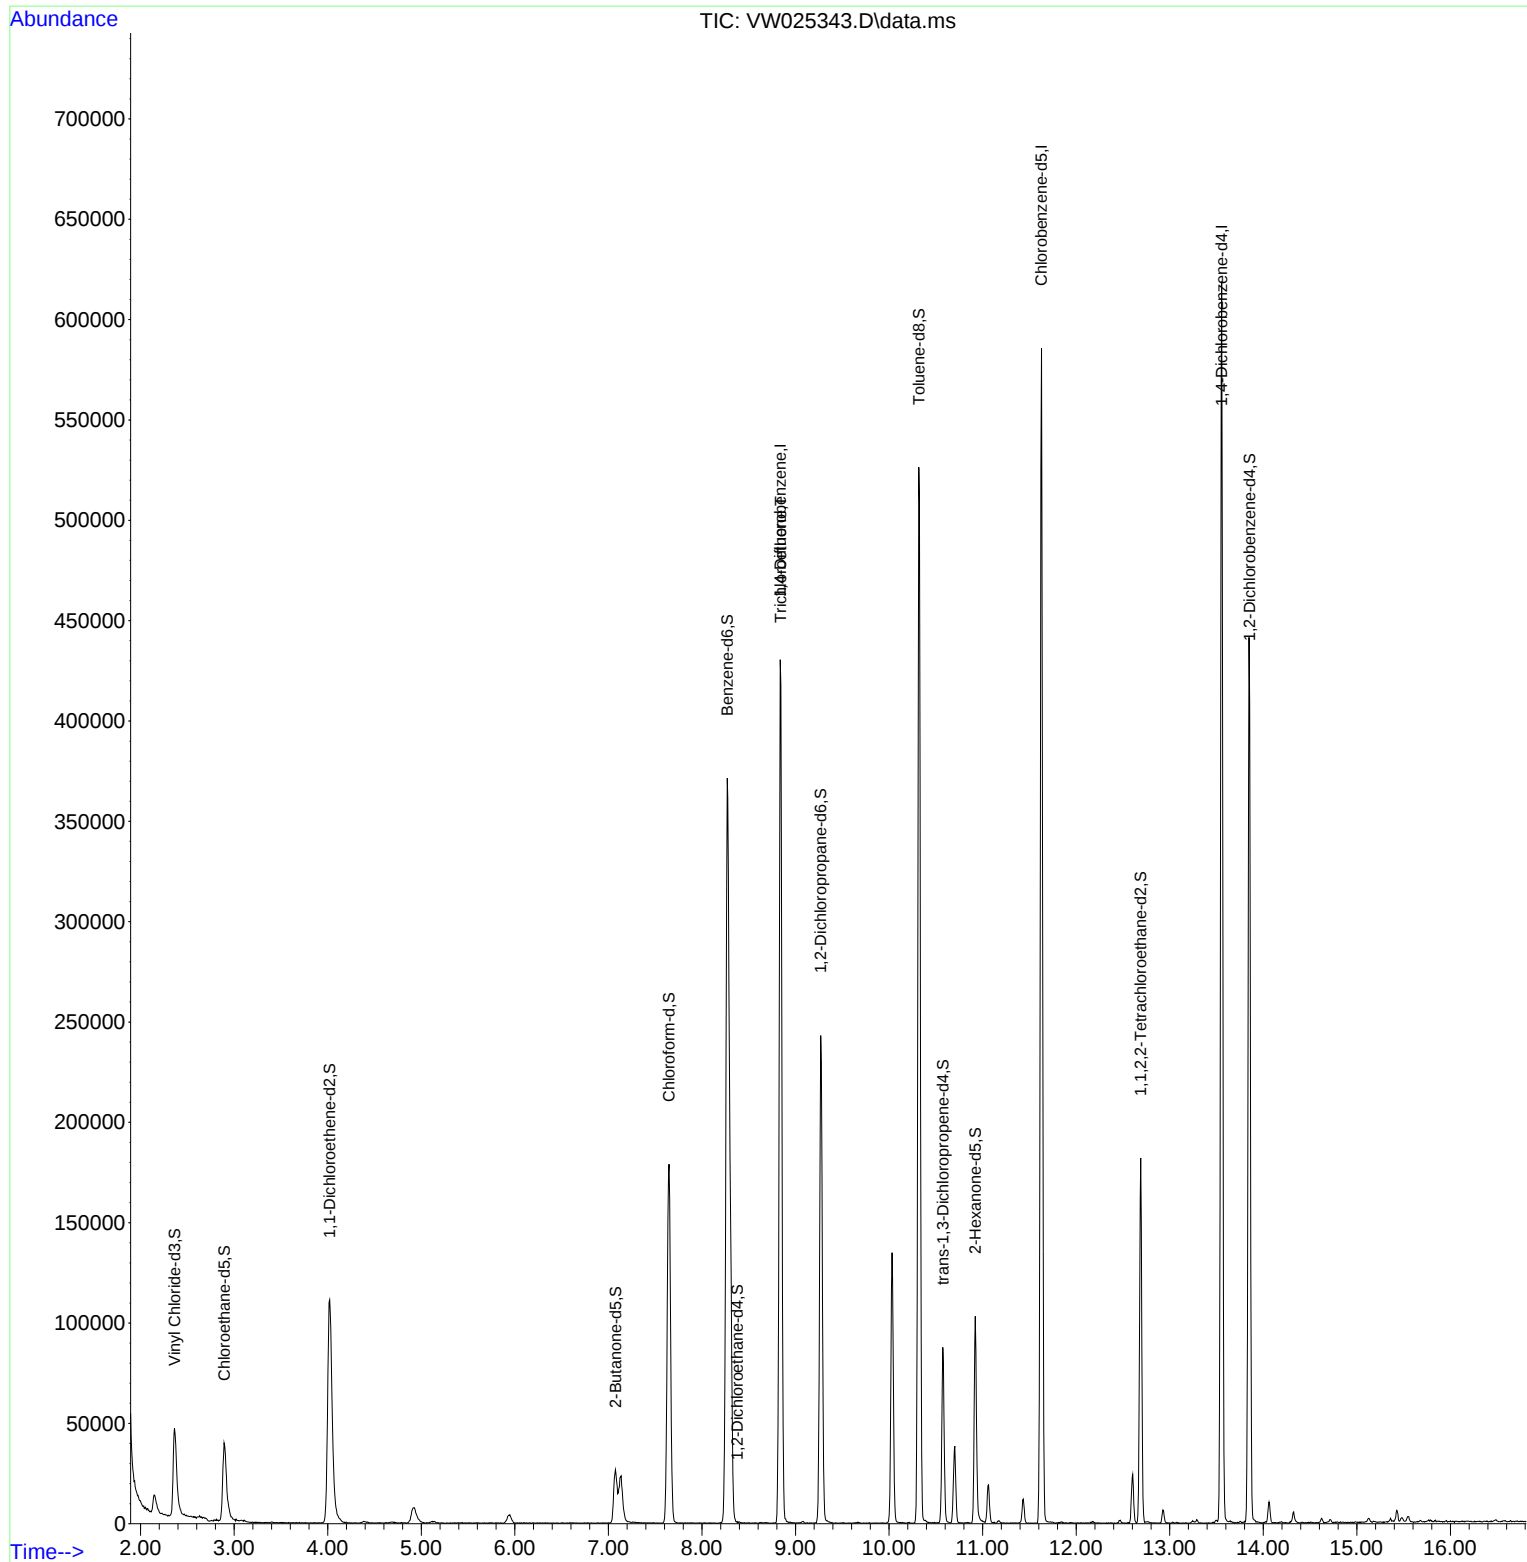

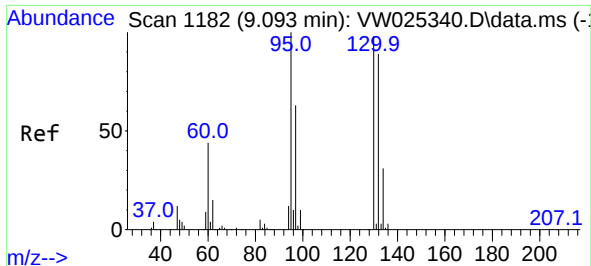

#34
 Trichloroethene
 Concen: 1.793 ug/L
 RT: 8.843 min Scan# 11
 Delta R.T. -0.250 min
 Lab File: VW025343.D
 Acq: 17 Feb 2023 13:40

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

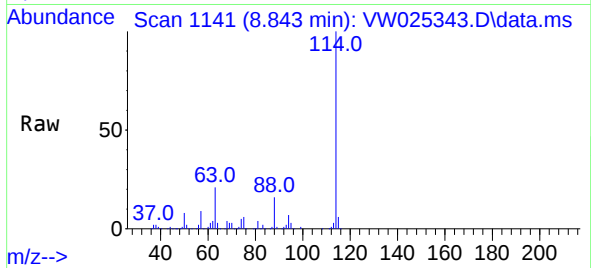

Tgt Ion: 95 Resp: 11256

Ion	Ratio	Lower	Upper
95	100		
97	0.0	45.4	84.2#
132	0.0	67.1	124.5#
130	0.0	69.2	128.6#

