
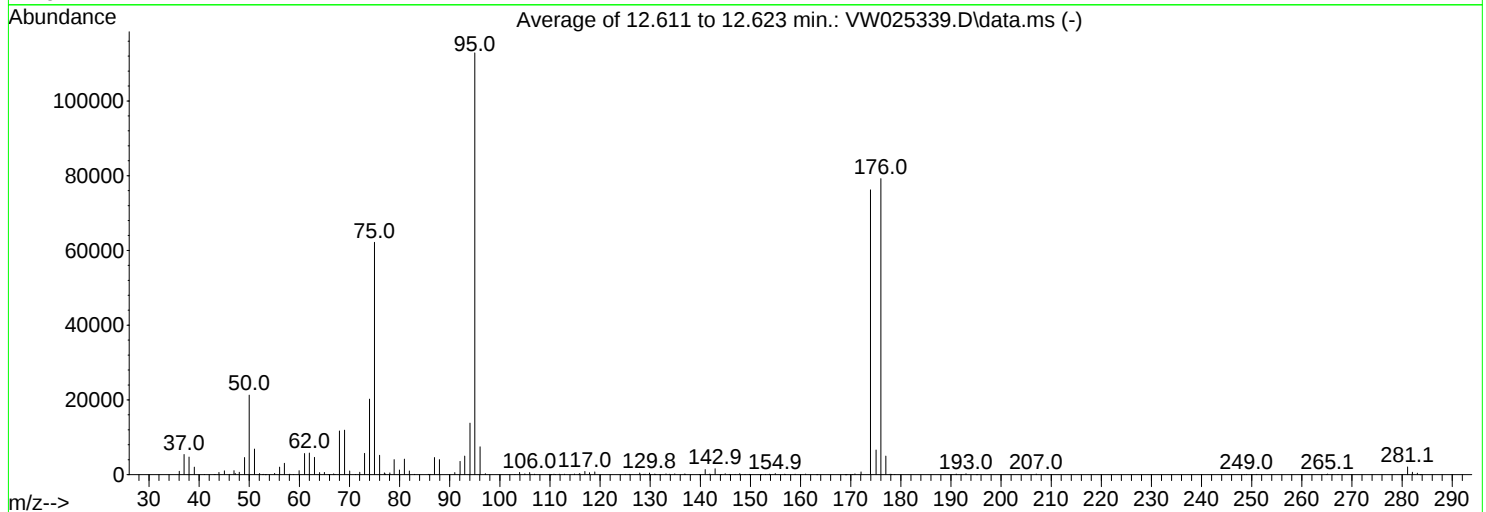


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021723\
Data File : VW025339.D
Acq On : 17 Feb 2023 08:24
Operator : SY/MD
Sample : BFB482
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB482

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020323SMA.M
Title : SFAM01.0
Last Update : Wed Feb 15 22:06:10 2023

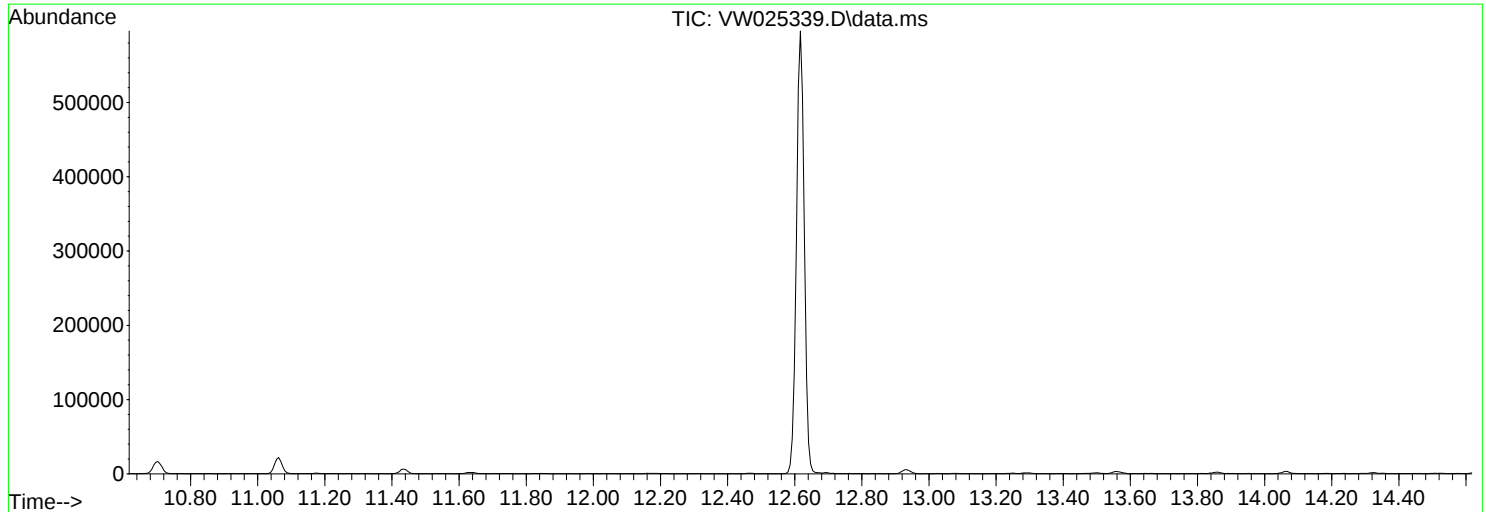

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	21264	PASS
75	95	30	80	55.1	62168	PASS
95	95	100	100	100.0	112883	PASS
96	95	5	9	6.6	7436	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.5	76216	PASS
175	174	5	9	8.6	6577	PASS
176	174	95	105	104.0	79229	PASS
177	176	5	10	6.3	4982	PASS

m/z	Abundance
39.90	175.0
44.00	159.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

m/z	Abundance
36.10	954.0
37.00	5493.0
38.00	4706.0
39.00	2123.0
39.90	131.0
41.00	110.0
43.00	75.0
44.00	891.0
45.10	889.0
46.30	64.0
46.90	869.0
47.20	869.0
48.00	597.0
49.10	5198.0
50.00	21752.0
51.10	7175.0
52.10	279.0
52.70	76.0
53.20	67.0
55.00	340.0
56.00	2012.0
57.00	2861.0
58.10	100.0
58.80	73.0
60.00	997.0
61.00	5585.0
62.00	5813.0
63.00	4684.0
64.00	522.0
65.00	617.0
65.90	58.0
67.10	263.0
68.00	12363.0
69.00	11848.0
70.10	904.0
71.30	79.0
72.00	737.0
73.00	6026.0
74.00	20264.0
75.00	60584.0
76.00	5161.0
77.00	741.0
78.00	415.0
78.90	4077.0
79.90	1419.0
80.90	4134.0
82.00	889.0
83.00	141.0
85.70	72.0
87.00	4364.0
88.00	4121.0
90.90	549.0
92.00	3409.0
93.00	4681.0
94.00	13788.0
95.00	110568.0
96.10	7471.0
97.10	302.0
103.00	196.0
103.90	551.0
105.00	217.0
106.00	532.0
106.90	175.0
109.90	162.0
110.80	105.0
112.00	149.0
112.90	139.0
114.90	213.0
115.80	392.0
116.90	687.0
117.90	474.0
119.00	697.0
125.00	124.0
125.80	85.0
127.90	452.0
128.70	223.0
129.80	367.0
130.90	215.0
131.90	60.0
133.20	361.0
133.80	149.0
134.80	195.0
136.80	268.0
140.90	1284.0
141.90	191.0
143.00	1596.0
143.90	69.0
145.00	316.0
145.80	207.0
147.00	109.0
148.00	176.0
148.90	134.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

150.00	75.0
153.10	95.0
153.80	162.0
154.90	258.0
156.80	174.0
159.00	137.0
161.00	149.0
163.20	52.0
170.80	228.0
172.00	800.0
173.90	63824.0
175.10	5675.0
176.00	70760.0
177.00	4071.0
177.90	236.0
178.80	71.0
191.00	323.0
192.10	105.0
193.00	368.0
195.10	55.0
207.00	227.0
249.00	185.0
251.00	116.0
264.90	184.0
265.10	181.0
266.10	142.0
267.20	141.0
281.10	2931.0
282.00	940.0
283.00	748.0
283.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

m/z	Abundance
36.10	954.0
37.00	5630.0
38.00	5334.0
39.10	2160.0
40.00	200.0
41.10	68.0
43.20	115.0
43.90	701.0
45.10	1085.0
46.10	158.0
47.00	1444.0
48.10	680.0
49.00	4961.0
50.00	23576.0
51.00	7395.0
52.00	316.0
52.90	154.0
55.00	394.0
56.00	2066.0
57.00	3661.0
58.10	235.0
58.90	128.0
60.00	1196.0
61.00	6502.0
62.00	6508.0
63.00	4985.0
64.10	664.0
65.00	822.0
66.80	334.0
68.00	12528.0
69.00	12889.0
70.10	1152.0
71.10	107.0
72.10	644.0
73.00	6295.0
74.00	22208.0
75.00	68800.0
76.00	6023.0
76.90	689.0
78.10	582.0
78.90	4569.0
80.00	1259.0
80.90	4692.0
81.90	1036.0
83.00	93.0
86.00	170.0
86.90	4877.0
87.90	4602.0
91.00	668.0
92.00	3786.0
93.00	5655.0
94.00	15326.0
95.00	125376.0
96.00	8135.0
97.10	238.0
104.00	642.0
105.00	223.0
105.90	584.0
107.00	143.0
109.80	89.0
110.80	220.0
111.80	110.0
112.80	94.0
114.80	157.0
116.00	417.0
117.00	1040.0
117.90	549.0
118.80	868.0
125.90	53.0
127.90	475.0
129.00	262.0
129.80	443.0
130.90	253.0
133.10	213.0
133.80	141.0
134.90	213.0
137.00	405.0
139.80	84.0
140.90	1465.0
141.80	233.0
143.00	1937.0
144.00	72.0
144.90	366.0
146.90	177.0
147.80	246.0
148.90	166.0
149.80	166.0
152.00	66.0
153.80	142.0
155.00	373.0
157.00	218.0
158.90	141.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

161.00	234.0
168.90	60.0
170.40	88.0
170.90	219.0
172.00	743.0
174.00	85224.0
175.00	7451.0
176.00	83840.0
177.00	5734.0
178.10	141.0
191.10	172.0
193.00	284.0
207.00	182.0
248.50	82.0
249.00	137.0
251.00	99.0
265.20	220.0
281.10	2117.0
282.10	623.0
283.10	323.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

m/z	Abundance
36.00	802.0
37.00	5004.0
38.00	4039.0
39.10	1718.0
40.00	176.0
44.00	632.0
45.00	1086.0
46.00	94.0
47.00	891.0
47.90	667.0
49.00	3631.0
50.00	18464.0
51.00	5933.0
52.10	294.0
52.90	95.0
55.10	314.0
56.10	1909.0
57.00	2607.0
58.20	87.0
59.90	989.0
61.10	4825.0
62.00	5023.0
63.00	4271.0
64.00	522.0
65.00	352.0
66.90	281.0
68.00	10198.0
69.00	10955.0
70.00	872.0
72.00	537.0
73.00	4822.0
74.00	18136.0
75.00	57120.0
76.00	4309.0
77.20	536.0
78.00	366.0
78.90	3409.0
80.00	1011.0
81.00	3586.0
82.00	991.0
85.80	131.0
86.10	133.0
87.00	4451.0
88.00	3368.0
91.10	422.0
92.10	3491.0
93.00	4578.0
94.10	12254.0
95.00	102704.0
96.00	6701.0
97.10	246.0
103.90	552.0
105.00	234.0
105.90	539.0
106.90	97.0
110.10	67.0
110.70	100.0
111.10	84.0
111.80	179.0
113.00	129.0
115.00	141.0
115.90	518.0
116.90	823.0
117.90	520.0
119.00	687.0
125.00	93.0
125.90	75.0
127.90	373.0
128.90	189.0
129.90	503.0
131.10	254.0
133.10	69.0
133.80	128.0
135.00	188.0
136.80	199.0
139.80	88.0
141.00	1402.0
142.00	144.0
142.90	1227.0
144.20	120.0
144.90	152.0
146.00	135.0
147.80	308.0
149.70	93.0
152.90	130.0
153.80	65.0
155.00	223.0
156.80	212.0
158.80	112.0
161.00	102.0
169.10	61.0
170.80	145.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482

172.10	592.0
174.00	79600.0
175.10	6606.0
176.00	83088.0
177.00	5140.0
177.80	171.0
178.20	135.0
190.90	75.0
192.90	148.0
207.10	91.0
265.10	117.0
281.10	1104.0
282.10	382.0
283.00	119.0
283.60	50.0

Instrument :
MSVOA_W
ClientSampleId :
BFB482