

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW021920\
Quantitation Report (Qedit)




Data File : VW015011.D
Acq On : 19 Feb 2020 17:04
Operator : SY/VA
Sample : L1584-04
Misc : 3.61G/10ML/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AM1

Manual Integrations
APPROVED

MMDadoda
2/24/2020 12:33:13 PM

Quant Time: Feb 20 03:34:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 20 03:31:47 2020
Response via : Initial Calibration

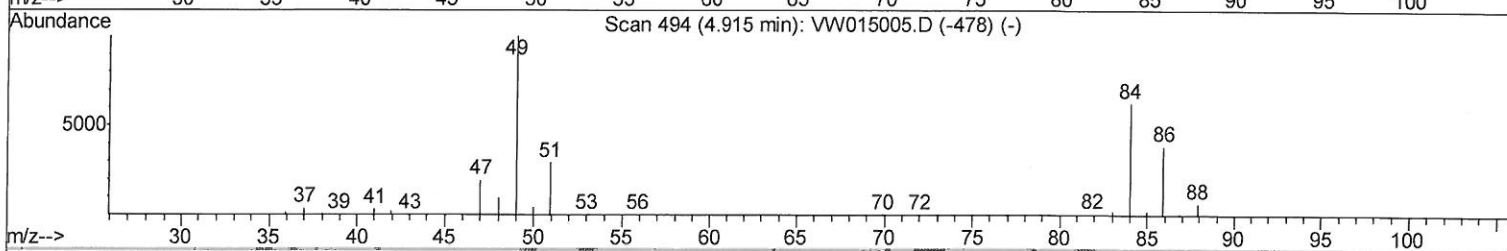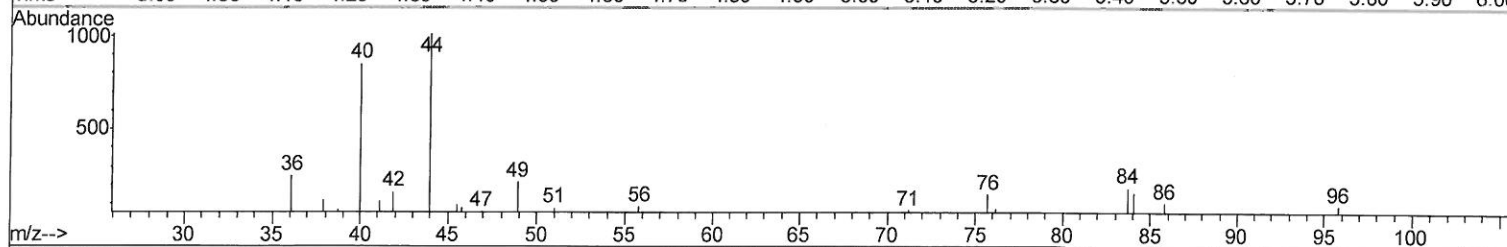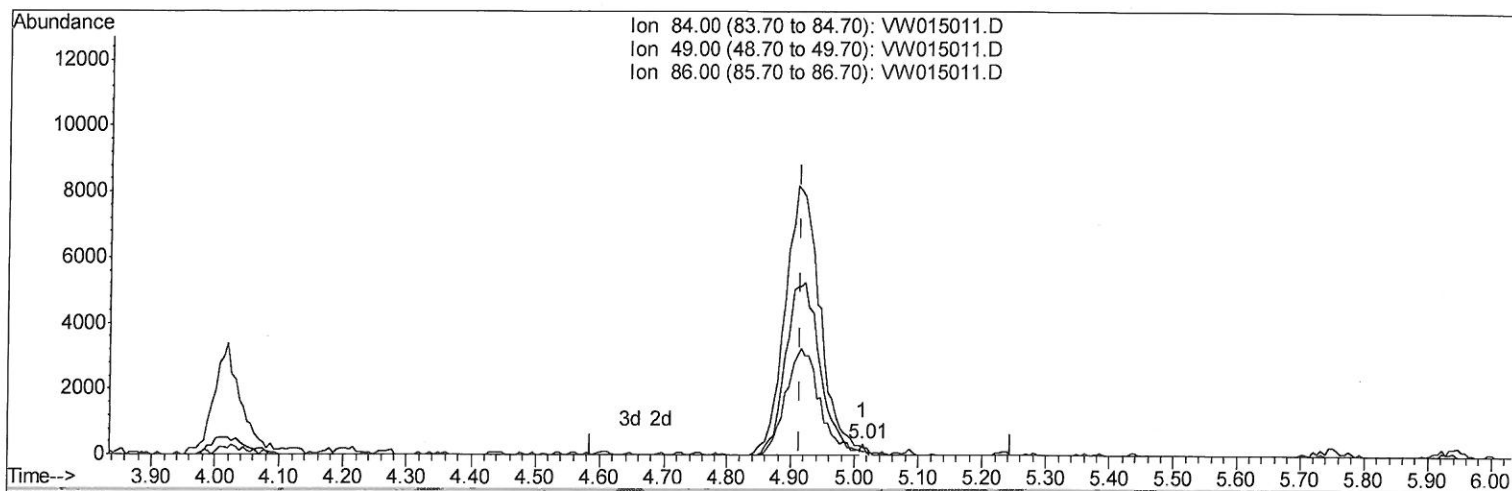

TIC: VW015011.D

(16) Methylene chloride (T)

5.013min (+0.097) 0.01ug/L

response 161

Ion	Exp%	Act%
84.00	100	100
49.00	136.80	62.36#
86.00	63.20	30.75#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW021920\
Quantitation Report (Qedit)




Data File : VW015011.D
Acq On : 19 Feb 2020 17:04
Operator : SY/VA
Sample : L1584-04
Misc : 3.61G/10ML/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AM1

Manual Integrations
APPROVED

MMDadoda
2/24/2020 12:33:13 PM

Quant Time: Feb 20 03:34:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 20 03:31:47 2020
Response via : Initial Calibration

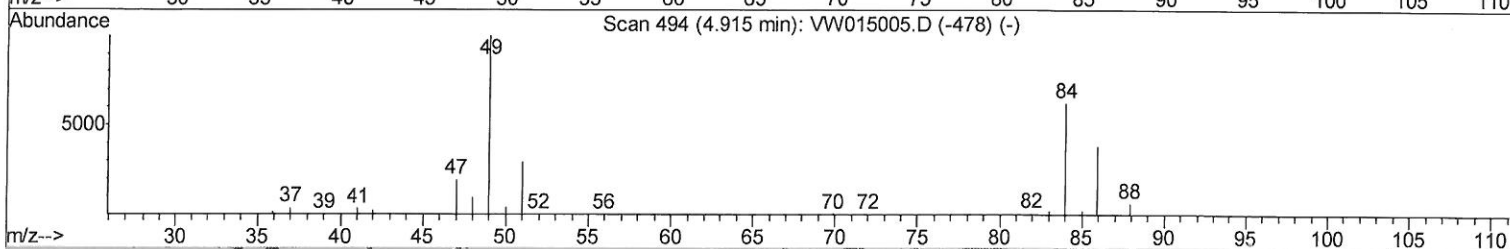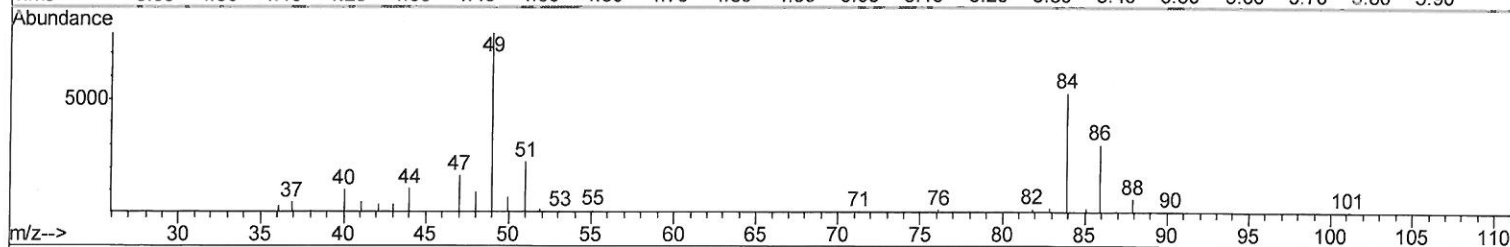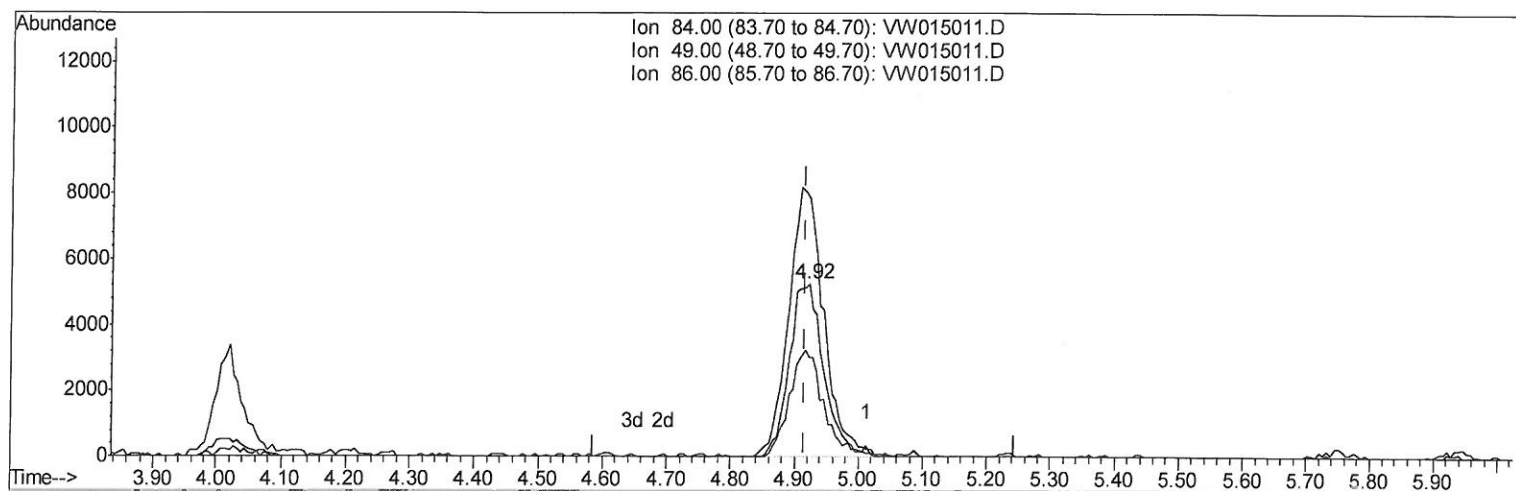

TIC: VW015011.D

(16) Methylene chloride (T)

4.921min (+0.006) 1.59ug/L m

response 19727

Ion	Exp%	Act%
84.00	100	100
49.00	136.80	149.40
86.00	63.20	57.36
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW021920\
Quantitation Report (QT Reviewed)

Data File : VW015011.D
Acq On : 19 Feb 2020 17:04
Operator : SY/VA
Sample : L1584-04
Misc : 3.61G/10ML/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AM1

Manual Integrations
APPROVED

MMDadoda
2/24/2020 12:33:13 PM

Quant Time: Feb 20 03:57:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 20 03:31:47 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	679189	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	612780	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	189204	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	150612	13.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.56%
7) Chloroethane-d5	2.89	69	214167	23.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.16%
10) 1,1-Dichloroethene-d2	4.01	63	314833	15.33	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.32%
20) 2-Butanone-d5	7.07	46	154980	49.11	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.22%
24) Chloroform-d	7.65	84	497246	25.79	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.16%
26) 1,2-Dichloroethane-d4	8.30	65	301285	28.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	112.92%
29) Benzene-d6	8.27	84	930979	23.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.48%
33) 1,2-Dichloropropane-d6	9.27	67	348100	27.11	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.44%
37) Toluene-d8	10.32	98	742472	21.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.64%
38) trans-1,3-Dichloropropene-	10.58	79	95280	18.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.16%
39) 2-Hexanone-d5	10.92	63	95342	40.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.46%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	242770	25.11	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	171281	23.34	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.36%

Target Compounds

				Qvalue	
13) Acetone	4.12	43	25161	7.725	ug/L 94
14) Carbon disulfide	4.38	76	12996	0.449	ug/L 100
16) Methylene chloride	4.92	84	19727m	1.594	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW021920\
Quantitation Report (QT Reviewed)

Data File : VW015011.D
Acq On : 19 Feb 2020 17:04
Operator : SY/VA
Sample : L1584-04
Misc : 3.61G/10ML/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0AM1

Manual Integrations
APPROVED

MMDadoda
2/24/2020 12:33:13 PM

Quant Time: Feb 20 03:57:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Thu Feb 20 03:31:47 2020
Response via : Initial Calibration

