

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022020\
Quantitation Report (Qedit)




Data File : VW015016.D
Acq On : 20 Feb 2020 14:18
Operator : SY/VA
Sample : VW0220SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK07

Manual Integrations
APPROVED

MMDadoda
2/21/2020 3:21:46 PM

Quant Time: Feb 21 02:00:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 21 01:58:19 2020
Response via : Initial Calibration

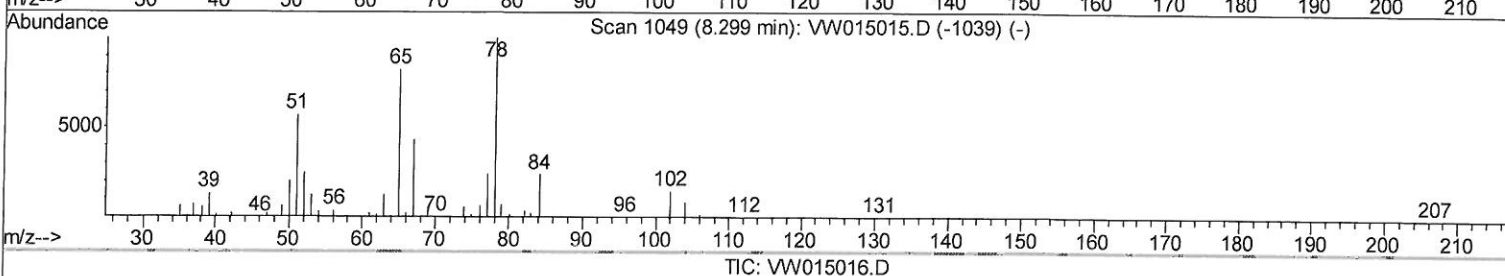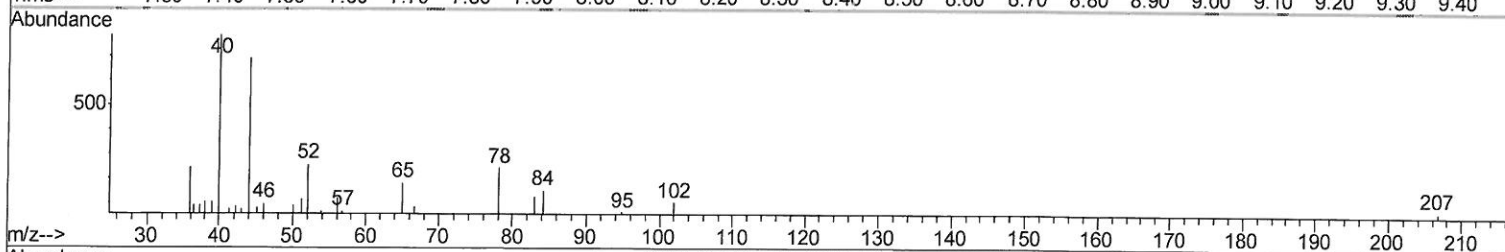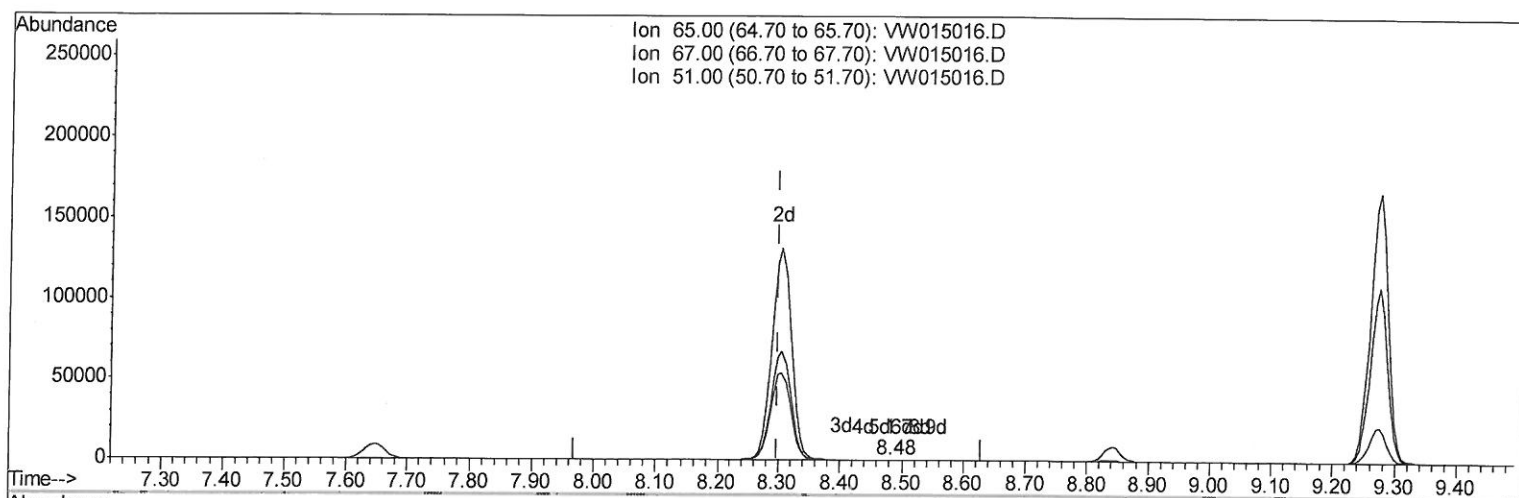

TIC: VW015016.D

(26) 1,2-Dichloroethane-d4 (S)

8.482min (+0.183) 0.01ug/L

response 102

Ion	Exp%	Act%
65.00	100	100
67.00	53.80	50.98
51.00	115.00	128.43
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022020\
Quantitation Report (Qedit)




Data File : VW015016.D
Acq On : 20 Feb 2020 14:18
Operator : SY/VA
Sample : VW0220SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK07

Manual Integrations
APPROVED

MMDadoda
2/21/2020 3:21:46 PM

Quant Time: Feb 21 02:00:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 21 01:58:19 2020
Response via : Initial Calibration

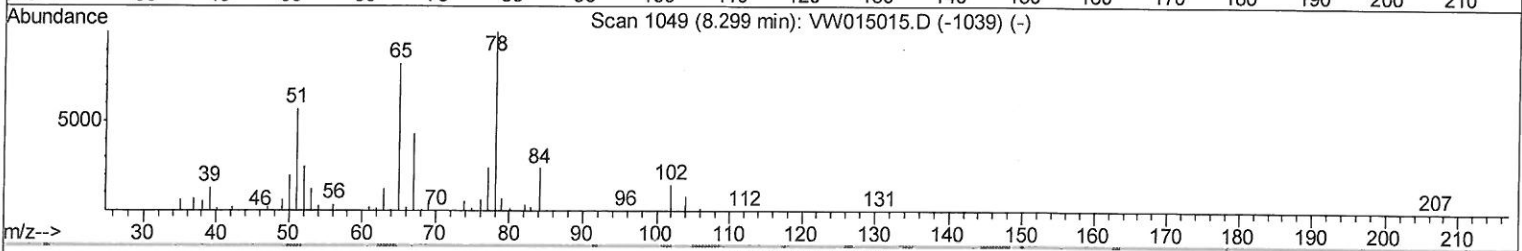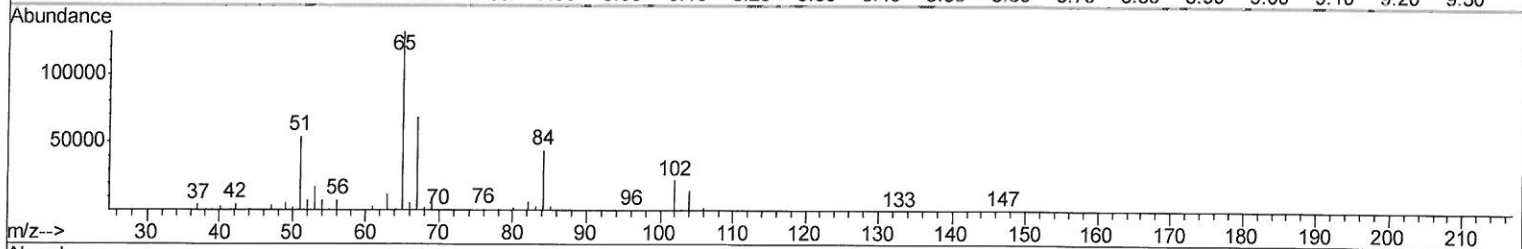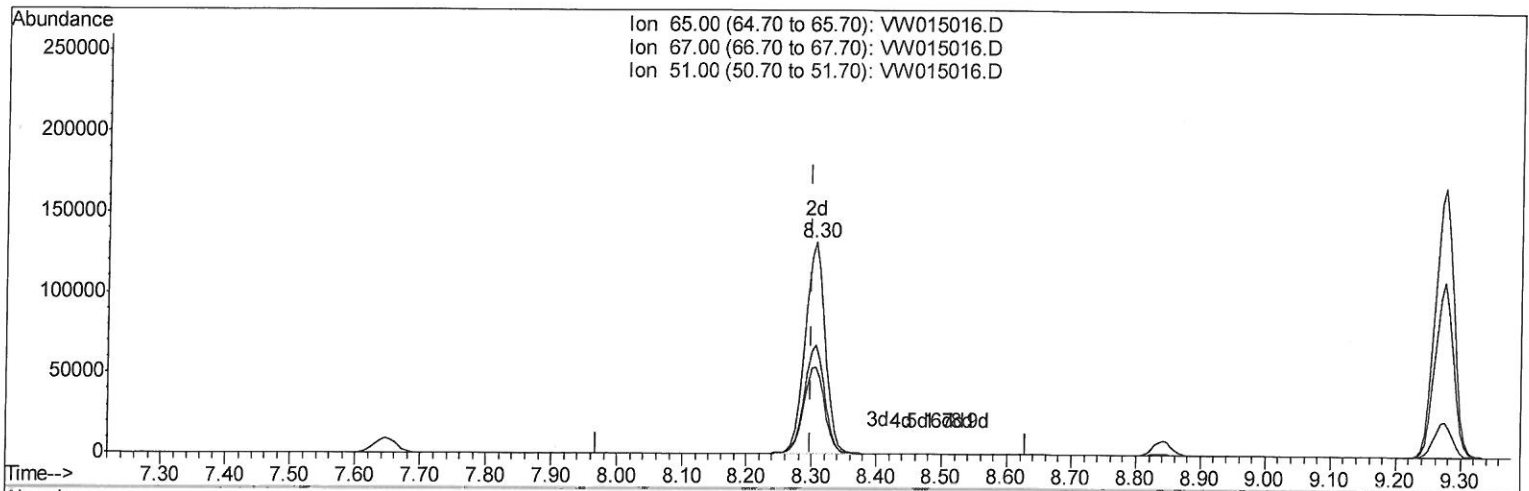

TIC: VW015016.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.006) 24.72ug/L m

response 283482

Ion	Exp%	Act%
65.00	100	100
67.00	53.80	0.02#
51.00	115.00	0.05#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022020\
Quantitation Report (QT Reviewed)

Data File : VW015016.D
Acq On : 20 Feb 2020 14:18
Operator : SY/VA
Sample : VW0220SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK07

Manual Integrations
APPROVED

MMDadoda
2/21/2020 3:21:46 PM

Quant Time: Feb 21 02:06:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 21 01:58:19 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	729764	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	680046	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	265497	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	255257	21.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.52%
7) Chloroethane-d5	2.89	69	216362	22.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.48%
10) 1,1-Dichloroethene-d2	4.02	63	368885	16.71	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.84%
20) 2-Butanone-d5	7.07	46	147644	43.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.10%
24) Chloroform-d	7.65	84	483812	23.35	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	8.30	65	283482m	24.72	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.88%
29) Benzene-d6	8.27	84	939837	21.49	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.96%
33) 1,2-Dichloropropane-d6	9.27	67	334100	23.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.76%
37) Toluene-d8	10.32	98	766099	19.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.64%
38) trans-1,3-Dichloropropene-	10.58	79	113389	20.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.60%
39) 2-Hexanone-d5	10.93	63	96059	36.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	218533	20.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	214629	20.85	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.40%

02/21/2024

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Methylene chloride	4.92	84	28760	2.163	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022020\
Quantitation Report (QT Reviewed)

Data File : VW015016.D
Acq On : 20 Feb 2020 14:18
Operator : SY/VA
Sample : VW0220SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK07

Manual Integrations
APPROVED

MMDadoda
2/21/2020 3:21:46 PM

Quant Time: Feb 21 02:06:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 21 01:58:19 2020
Response via : Initial Calibration

