

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW022020\
 Data File : VW015020.D
 Acq On : 20 Feb 2020 16:32
 Operator : SY/VA
 Sample : L1584-07
 Misc : 5.01G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 2/21/2020 3:21:56 PM

Quant Time: Feb 21 03:05:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 21 01:58:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	703398	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	653930	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	238916	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	266832	22.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.64%
7) Chloroethane-d5	2.89	69	225375	24.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.68%
10) 1,1-Dichloroethene-d2	4.01	63	381508m	17.93	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.72%
20) 2-Butanone-d5	7.07	46	140759	43.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.14%
24) Chloroform-d	7.65	84	515200	25.80	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.20%
26) 1,2-Dichloroethane-d4	8.31	65	294125	26.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.44%
29) Benzene-d6	8.27	84	976966	23.23	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.92%
33) 1,2-Dichloropropane-d6	9.27	67	349650	25.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.08%
37) Toluene-d8	10.32	98	807865	21.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.32%
38) trans-1,3-Dichloropropene-	10.58	79	115808	21.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.60%
39) 2-Hexanone-d5	10.92	63	93574	37.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	223705	21.68	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.72%
61) 1,2-Dichlorobenzene-d4	13.85	152	223706	24.15	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.60%

Target Compounds					Ovalue
13) Acetone	4.12	43	13601	4.032 ug/L	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW022020\
Data File : VW015020.D
Acq On : 20 Feb 2020 16:32
Operator : SY/VA
Sample : L1584-07
Misc : 5.01G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
2/21/2020 3:21:56 PM

Quant Time: Feb 21 03:05:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM020520S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 21 01:58:19 2020
Response via : Initial Calibration

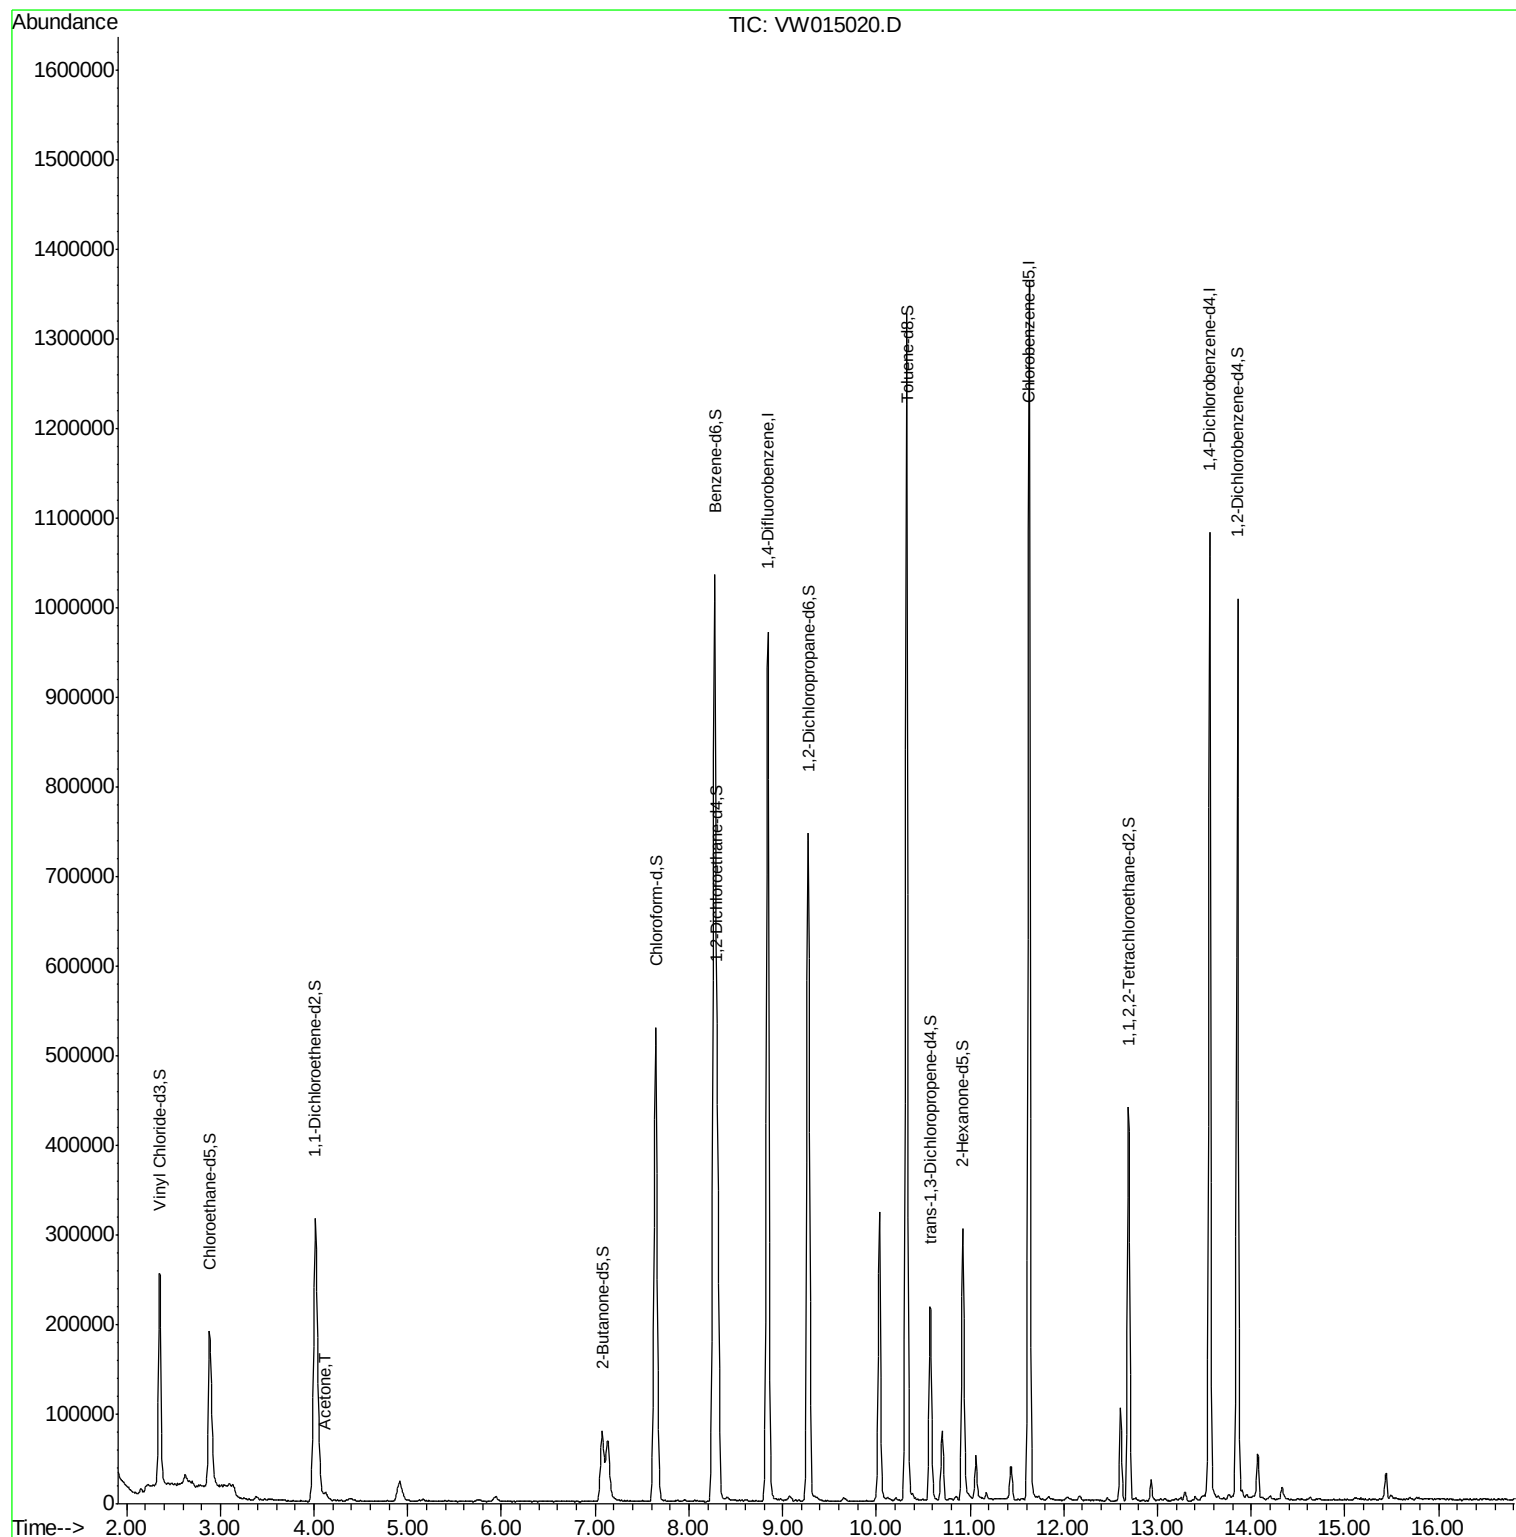

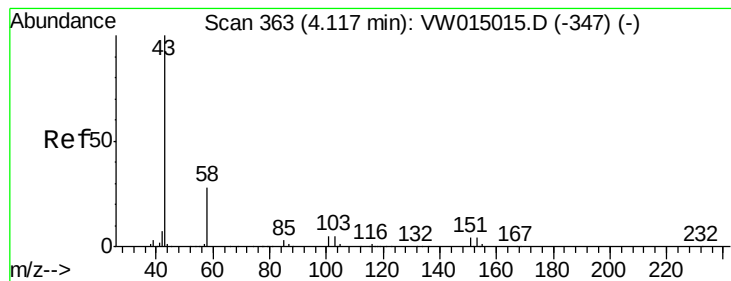

#13

Acetone

Concen: 4.032 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW015020.D

Acq: 20 Feb 2020 16:32

Instrument :

MSVOA_W

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 13601

Ion Ratio Lower Upper

43 100

58 13.7 0.0 60.4

Manual Integrations

APPROVED

MMDadoda

2/21/2020 3:21:56 PM

