
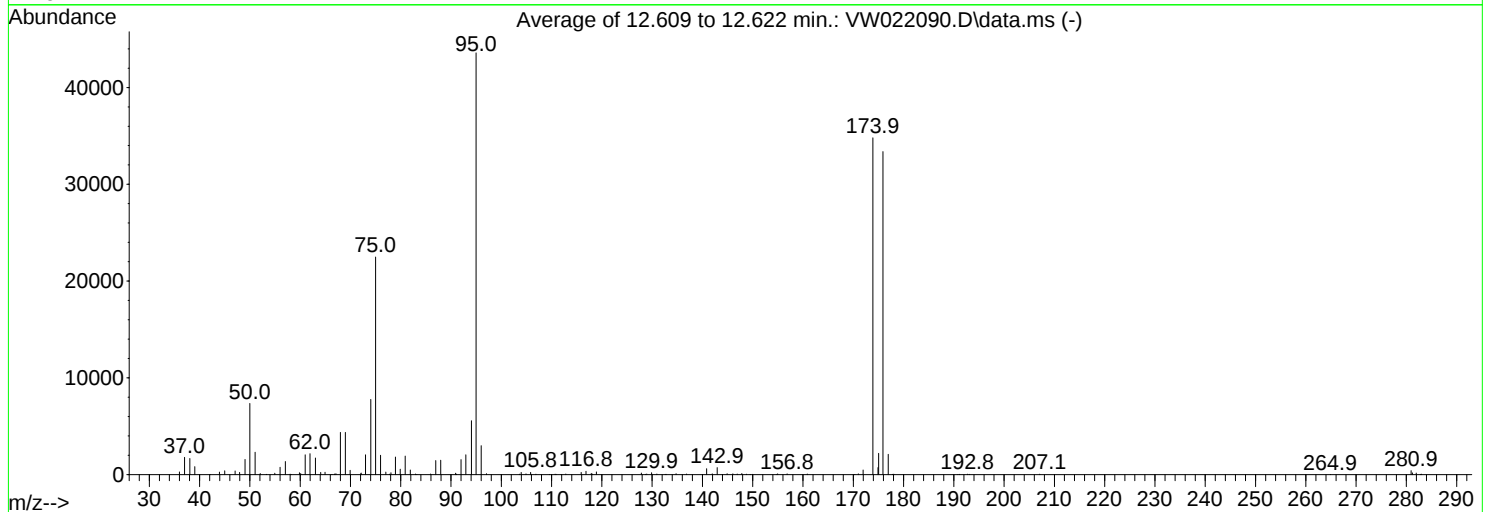


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022222\
 Data File : VW022090.D
 Acq On : 22 Feb 2022 08:49
 Operator : SY/VA
 Sample : BFB511
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB511

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020122SMA.M
 Title : SFAM01.0
 Last Update : Tue Feb 22 00:39:16 2022

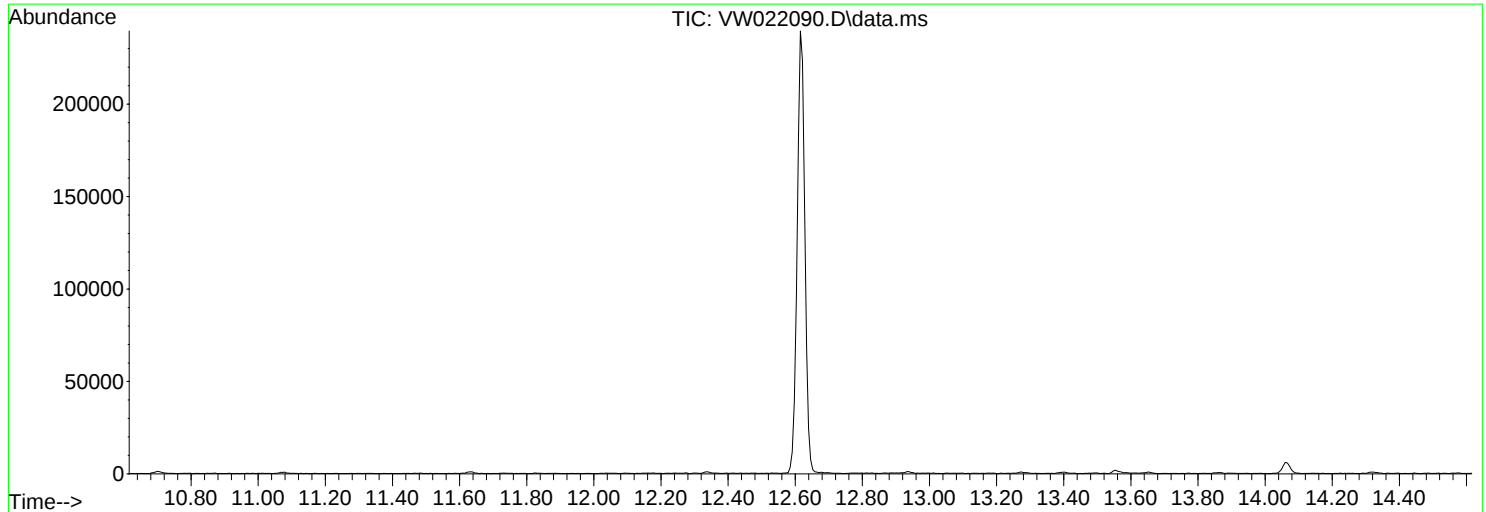

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	7357	PASS
75	95	30	80	51.6	22480	PASS
95	95	100	100	100.0	43584	PASS
96	95	5	9	6.9	2996	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.8	34797	PASS
175	174	5	9	6.3	2196	PASS
176	174	95	105	95.9	33384	PASS
177	176	5	10	6.3	2104	PASS

m/z	Abundance
36.10	367.0
37.00	1547.0
38.00	1449.0
39.10	728.0
40.10	104.0
42.10	71.0
43.90	309.0
45.00	340.0
46.00	84.0
47.00	472.0
48.00	137.0
49.00	1392.0
50.00	6901.0
51.10	2065.0
52.10	95.0
53.30	54.0
55.00	140.0
56.00	740.0
57.00	1291.0
58.00	83.0
59.80	345.0
61.00	1711.0
61.90	1808.0
63.10	1465.0
64.10	189.0
65.00	228.0
66.80	85.0
67.10	84.0
68.00	3698.0
69.00	3499.0
69.90	359.0
72.00	238.0
73.00	1787.0
74.00	6913.0
75.00	20000.0
76.00	1555.0
77.00	234.0
77.80	151.0
78.10	150.0
79.00	1583.0
80.00	566.0
80.90	1752.0
81.90	536.0
83.00	60.0
85.90	61.0
87.00	1276.0
88.00	1224.0
90.90	207.0
92.00	1499.0
93.00	1941.0
94.10	4948.0
95.00	36416.0
96.00	2809.0
97.00	135.0
103.60	135.0
104.00	192.0
104.90	108.0
105.90	181.0
110.70	81.0
111.90	66.0
115.90	172.0
116.90	303.0
117.90	211.0
118.90	266.0
127.90	140.0
128.70	107.0
129.90	142.0
131.00	80.0
132.60	83.0
134.80	94.0
140.80	419.0
142.00	109.0
142.90	634.0
144.80	88.0
146.10	99.0
146.90	66.0
147.80	90.0
149.50	61.0
154.80	104.0
156.80	77.0
160.90	53.0
171.00	98.0
171.90	333.0
173.90	27336.0
174.90	2169.0
175.90	26624.0
177.00	1690.0
178.10	57.0
191.10	97.0
193.10	109.0
207.10	111.0
281.00	875.0

Instrument :
MSVOA_W
ClientSampleId :
BFB511

282.00193.0

282.80124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB511

m/z	Abundance
36.00	338.0
37.00	1933.0
38.00	2048.0
39.10	908.0
40.00	168.0
44.00	416.0
45.00	421.0
47.10	312.0
48.00	350.0
49.10	1807.0
50.00	8156.0
51.10	2474.0
52.00	99.0
53.30	52.0
55.00	168.0
56.00	766.0
57.10	1440.0
58.00	81.0
60.10	362.0
61.00	2384.0
62.00	2649.0
63.10	1921.0
64.10	261.0
65.00	296.0
66.30	63.0
67.10	191.0
68.00	5048.0
69.00	4892.0
70.00	563.0
72.20	318.0
73.00	2411.0
74.00	8506.0
75.00	25064.0
76.00	2396.0
77.00	295.0
78.00	221.0
78.90	2180.0
79.90	600.0
80.90	2052.0
81.90	502.0
82.90	81.0
83.20	72.0
86.90	1522.0
87.90	1708.0
90.90	237.0
92.00	1505.0
92.90	2226.0
94.00	6067.0
95.00	49520.0
96.00	3353.0
97.10	90.0
104.00	294.0
105.00	87.0
105.80	267.0
106.90	66.0
110.70	78.0
112.80	108.0
116.00	219.0
116.90	391.0
118.10	200.0
118.90	278.0
127.90	168.0
129.00	118.0
129.90	245.0
131.00	54.0
132.80	72.0
134.70	94.0
136.90	111.0
140.90	700.0
141.90	135.0
143.00	801.0
144.00	57.0
144.90	134.0
146.10	65.0
146.80	93.0
147.90	144.0
148.80	82.0
150.00	65.0
155.00	125.0
156.90	98.0
171.00	144.0
172.00	679.0
173.90	40360.0
175.10	3107.0
175.90	35120.0
176.90	2190.0
177.80	119.0
190.80	52.0
192.80	100.0
264.90	60.0
281.20	538.0
281.90	141.0

Instrument :
MSVOA_W
ClientSampleId :
BFB511

283.00

103.0

Instrument :
MSVOA_W
ClientSampleId :
BFB511

m/z	Abundance
36.00	403.0
37.00	1858.0
38.10	1525.0
39.00	851.0
39.90	120.0
44.00	382.0
45.00	414.0
46.10	73.0
47.00	354.0
47.90	218.0
49.00	1494.0
50.00	7014.0
51.00	2387.0
52.00	148.0
54.90	152.0
56.00	782.0
57.00	1346.0
58.20	74.0
59.90	276.0
61.00	2052.0
62.00	2022.0
63.00	1801.0
64.10	236.0
64.90	232.0
66.90	120.0
68.00	4347.0
69.00	4705.0
70.00	418.0
72.10	194.0
73.00	1941.0
74.10	7882.0
75.00	22376.0
76.00	2053.0
77.10	253.0
78.10	211.0
78.90	1719.0
79.80	546.0
80.90	1978.0
81.90	382.0
82.90	57.0
86.00	145.0
86.90	1567.0
88.00	1518.0
91.10	177.0
92.00	1659.0
93.00	2006.0
94.00	5712.0
95.00	44816.0
96.00	2827.0
97.00	78.0
103.80	236.0
104.80	74.0
105.90	268.0
106.90	92.0
109.60	62.0
110.90	83.0
112.90	93.0
115.80	293.0
116.80	335.0
117.90	181.0
118.90	304.0
127.80	184.0
128.90	96.0
129.90	200.0
130.90	65.0
132.80	50.0
134.80	102.0
136.80	108.0
140.90	729.0
143.00	734.0
145.00	99.0
145.90	92.0
147.00	63.0
147.80	135.0
148.70	53.0
150.00	54.0
154.90	114.0
156.90	98.0
160.80	130.0
170.30	63.0
172.00	449.0
173.90	36696.0
175.00	3482.0
175.90	38408.0
176.90	2432.0
178.00	74.0
192.70	57.0
207.10	52.0
280.90	372.0
282.00	143.0
283.00	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB511

m/z	Abundance
35.90	80.0
37.30	59.0
39.80	174.0
44.00	97.0
46.20	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB511