

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
 Data File : VW022114.D
 Acq On : 23 Feb 2022 17:24
 Operator : SY/VA
 Sample : VW0223SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Feb 24 03:35:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 24 03:35:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	169521	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	155061	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	71716	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	53919	24.386	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	97.560%	
7) Chloroethane-d5	2.885	69	36867	21.192	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.760%	
11) 1,1-Dichloroethene-d2	4.019	63	60981	18.010	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	72.040%	
21) 2-Butanone-d5	7.086	46	16561	44.548	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.100%	
24) Chloroform-d	7.653	84	87297	23.081	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	92.320%	
26) 1,2-Dichloroethane-d4	8.305	65	46705	23.756	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	95.040%	
32) Benzene-d6	8.274	84	174704	24.209	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	96.840%	
36) 1,2-Dichloropropane-d6	9.274	67	47460	23.681	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	94.720%	
41) Toluene-d8	10.323	98	169911	23.683	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	94.720%	
43) trans-1,3-Dichloroprop...	10.579	79	19975	22.479	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.920%	
47) 2-Hexanone-d5	10.926	63	15175	46.038	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.080%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	39286	22.336	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	89.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	59622	25.884	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.520%	
Target Compounds						
39) cis-1,3-Dichloropropene	10.042	75	1792	0.674	ug/L #	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
Data File : VW022114.D
Acq On : 23 Feb 2022 17:24
Operator : SY/VA
Sample : VW0223SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Feb 24 03:35:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 24 03:35:08 2022
Response via : Initial Calibration

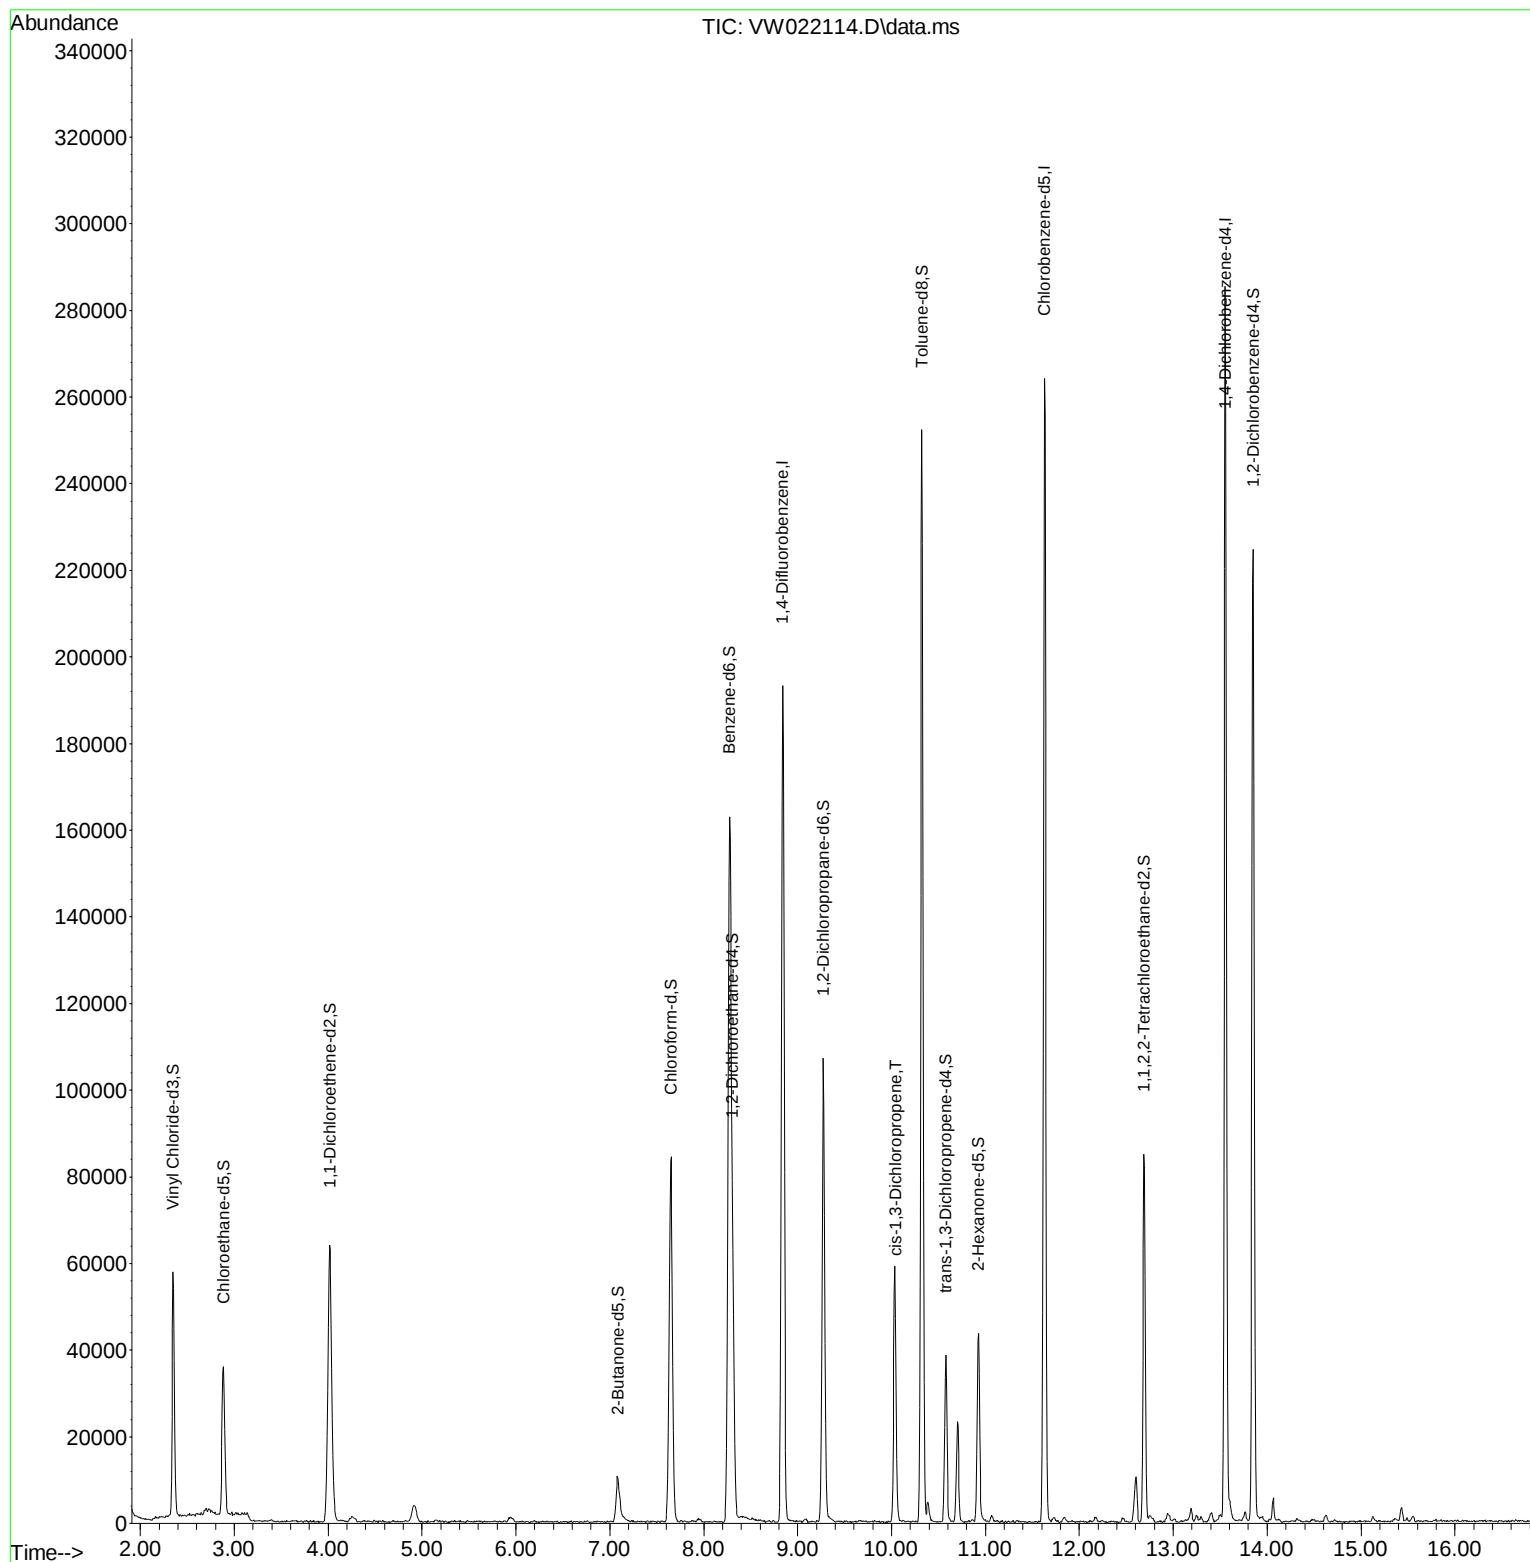

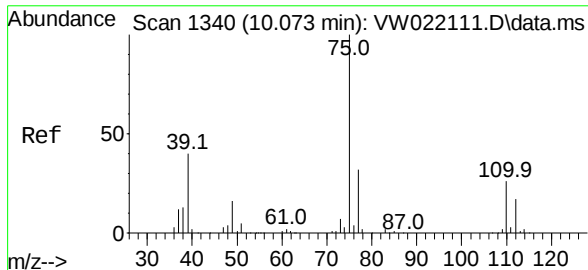

cis-1,3-Dichloropropene
 Concen: 0.674 ug/L
 RT: 10.042 min Scan# 1335
 Delta R.T. -0.031 min
 Lab File: VW022114.D
 Acq: 23 Feb 2022 17:24

Instrument : MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 1792
 Ion Ratio Lower Upper
 75 100
 77 51.2 20.6 38.2#

