

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
 Data File : VW022120.D
 Acq On : 23 Feb 2022 20:14
 Operator : SY/VA
 Sample : N1631-10
 Misc : 4.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Feb 24 03:36:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 24 03:35:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	170559	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	160706	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77393	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	37986	17.075	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.320%	
7) Chloroethane-d5	2.879	69	33797	19.309	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.240%	
11) 1,1-Dichloroethene-d2	4.007	63	46538	13.661	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	54.640%	
21) 2-Butanone-d5	7.074	46	22949	61.355	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	122.700%	
24) Chloroform-d	7.647	84	81603	21.444	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	85.760%	
26) 1,2-Dichloroethane-d4	8.305	65	44898	22.698	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.800%	
32) Benzene-d6	8.275	84	154781	20.695	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.760%	
36) 1,2-Dichloropropane-d6	9.274	67	45073	21.700	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	86.800%	
41) Toluene-d8	10.323	98	147745	19.870	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.480%	
43) trans-1,3-Dichloroprop...	10.579	79	18071	19.622	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	78.480%	
47) 2-Hexanone-d5	10.920	63	19222	56.267	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	112.540%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	44637	24.487	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	97.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152	57864	23.278	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.120%	
Target Compounds					Qvalue	
39) cis-1,3-Dichloropropene	10.030	75	1791	0.650	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
Data File : VW022120.D
Acq On : 23 Feb 2022 20:14
Operator : SY/VA
Sample : N1631-10
Misc : 4.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Feb 24 03:36:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 24 03:35:08 2022
Response via : Initial Calibration

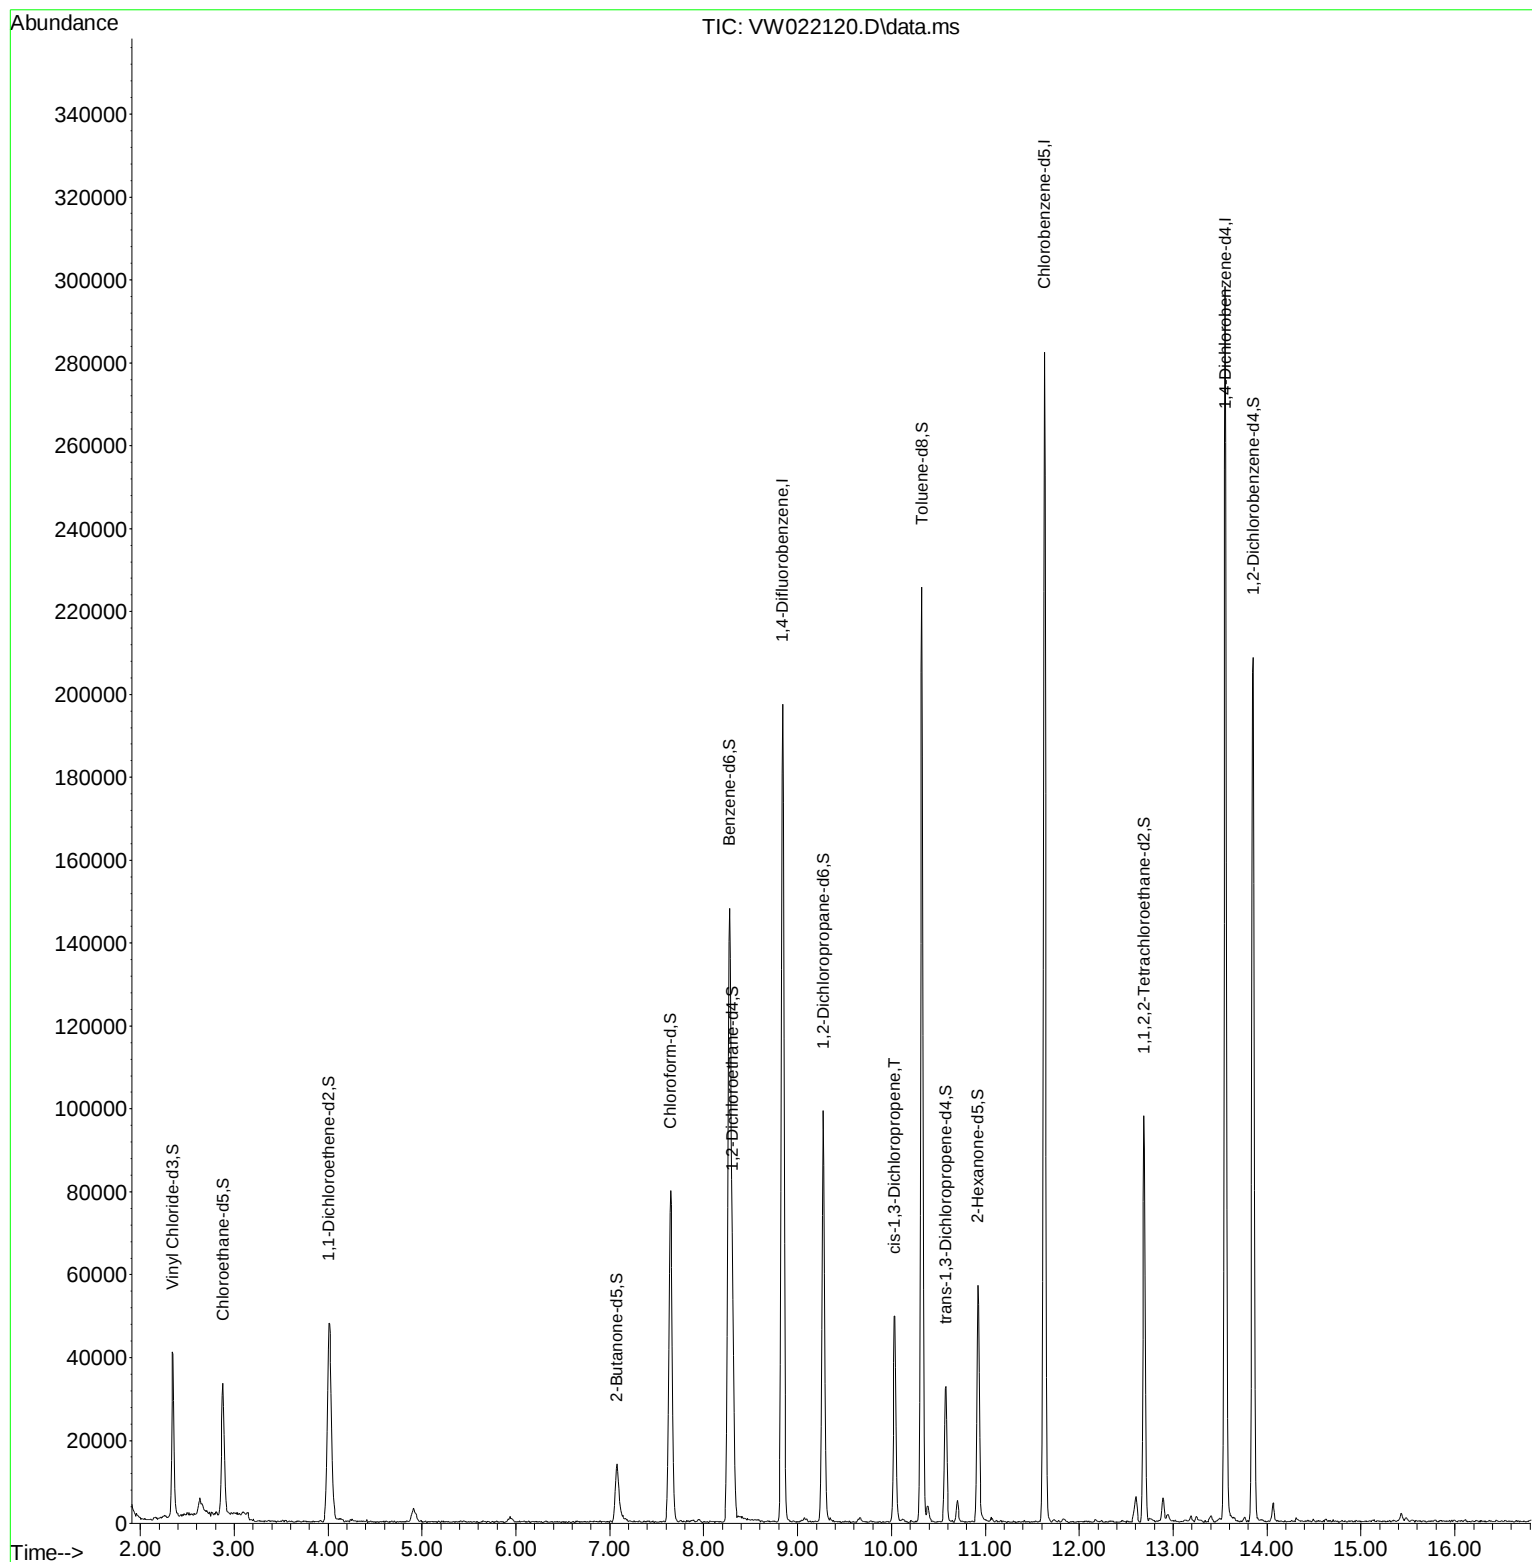

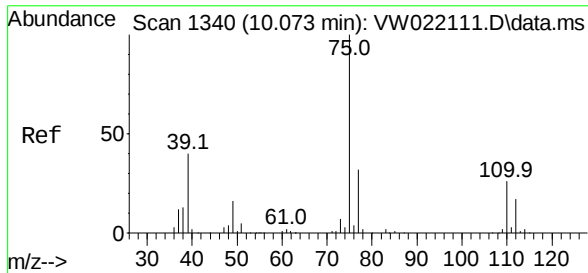

cis-1,3-Dichloropropene
 Concen: 0.650 ug/L
 RT: 10.030 min Scan# 1333
 Delta R.T. -0.043 min
 Lab File: VW022120.D
 Acq: 23 Feb 2022 20:14

Instrument : MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 1791
 Ion Ratio Lower Upper
 75 100
 77 37.4 20.6 38.2

