




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
 Data File : VW022124.D
 Acq On : 23 Feb 2022 21:50
 Operator : SY/VA
 Sample : N1631-14
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRJ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/24/2022
 Supervised By :Mahesh Dadoda 02/28/2022

Quant Time: Feb 24 03:37:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 24 03:35:08 2022
 Response via : Initial Calibration

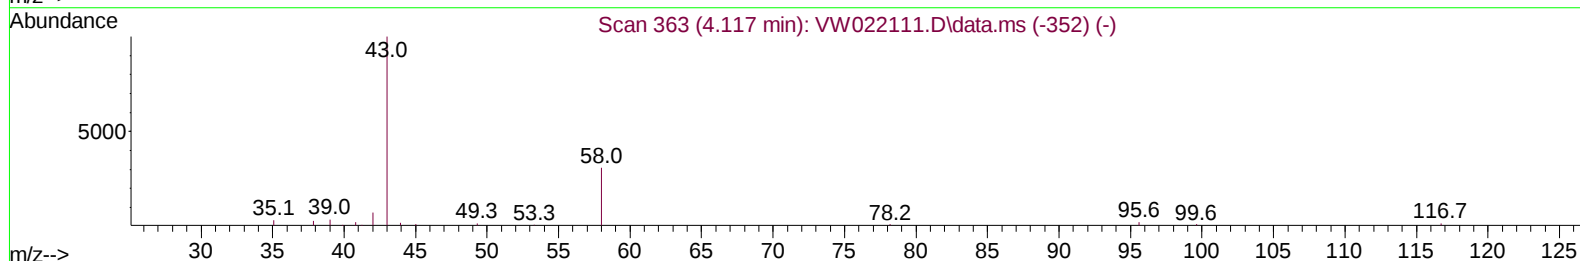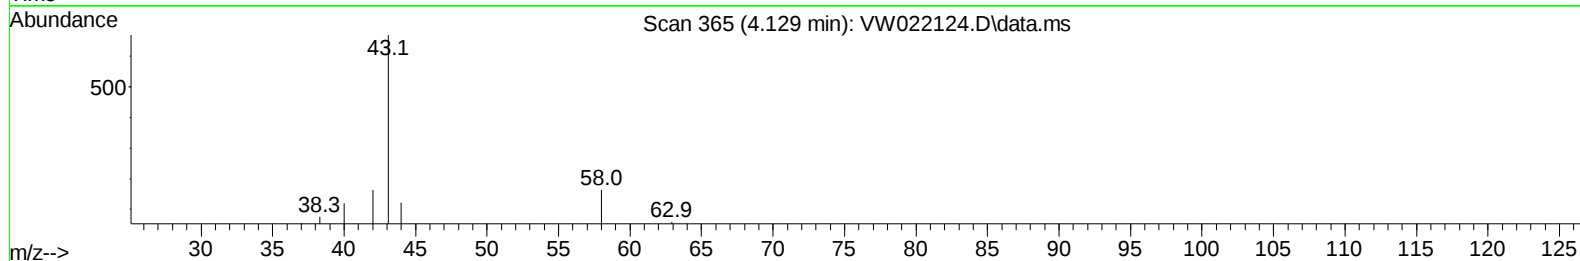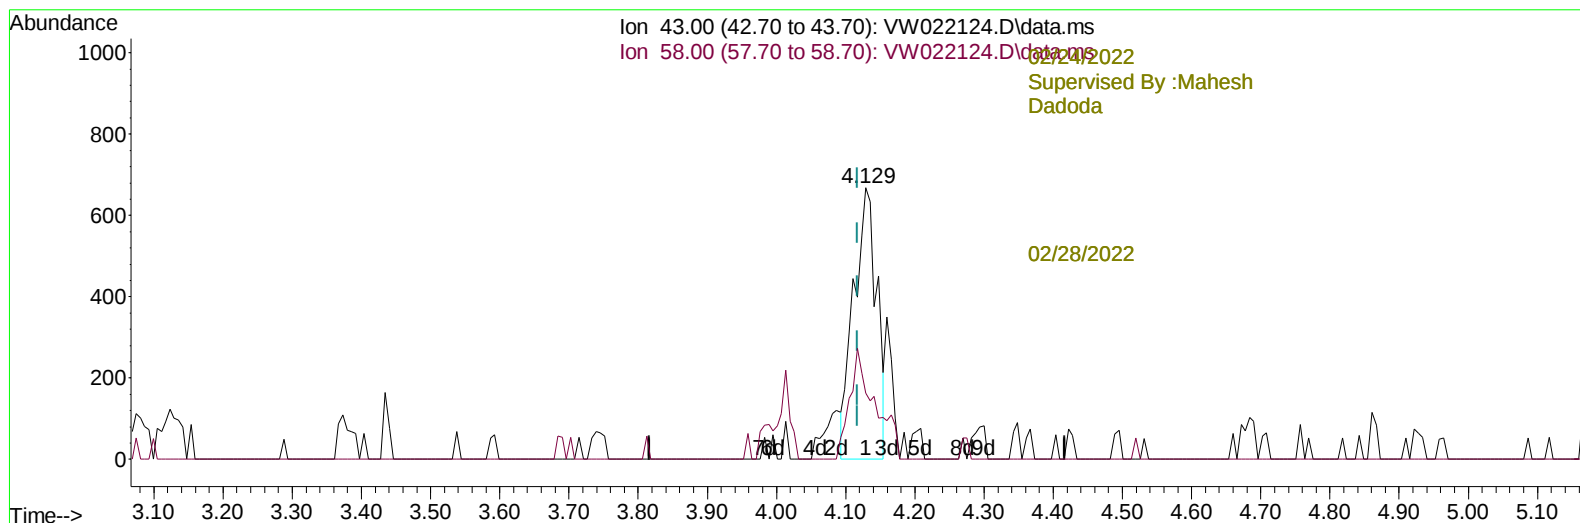

TIC: VW022124.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 5.26 ug/L

response 1543

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	29.55
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
 Data File : VW022124.D
 Acq On : 23 Feb 2022 21:50
 Operator : SY/VA
 Sample : N1631-14
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRJ0

Manual IntegrationsAPPROVED

Quant Time: Feb 24 03:37:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 24 03:35:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/24/2022
 Supervised By :Mahesh Dadoda 02/28/2022

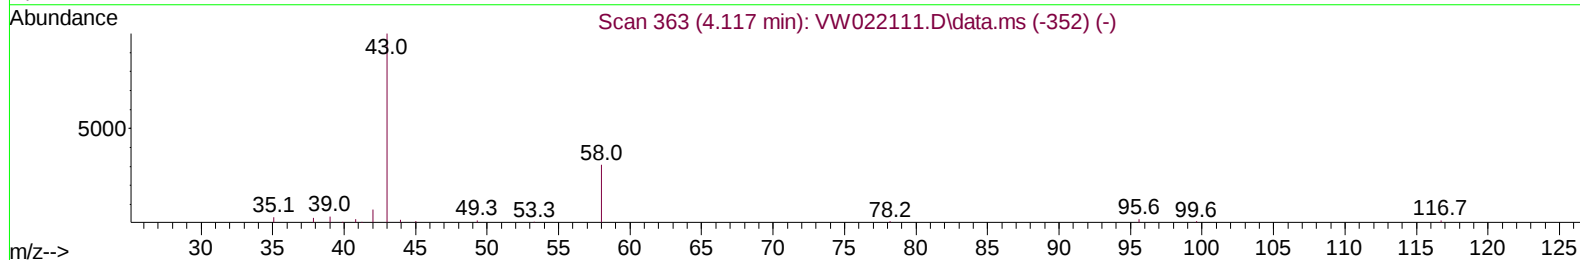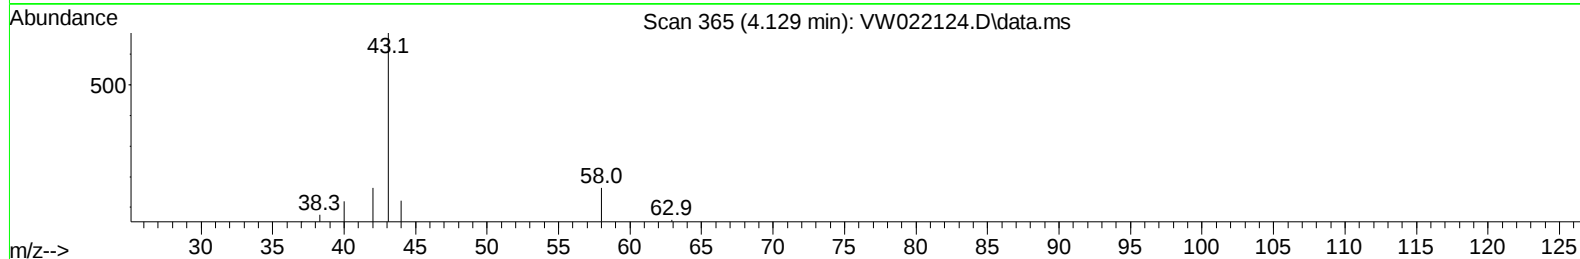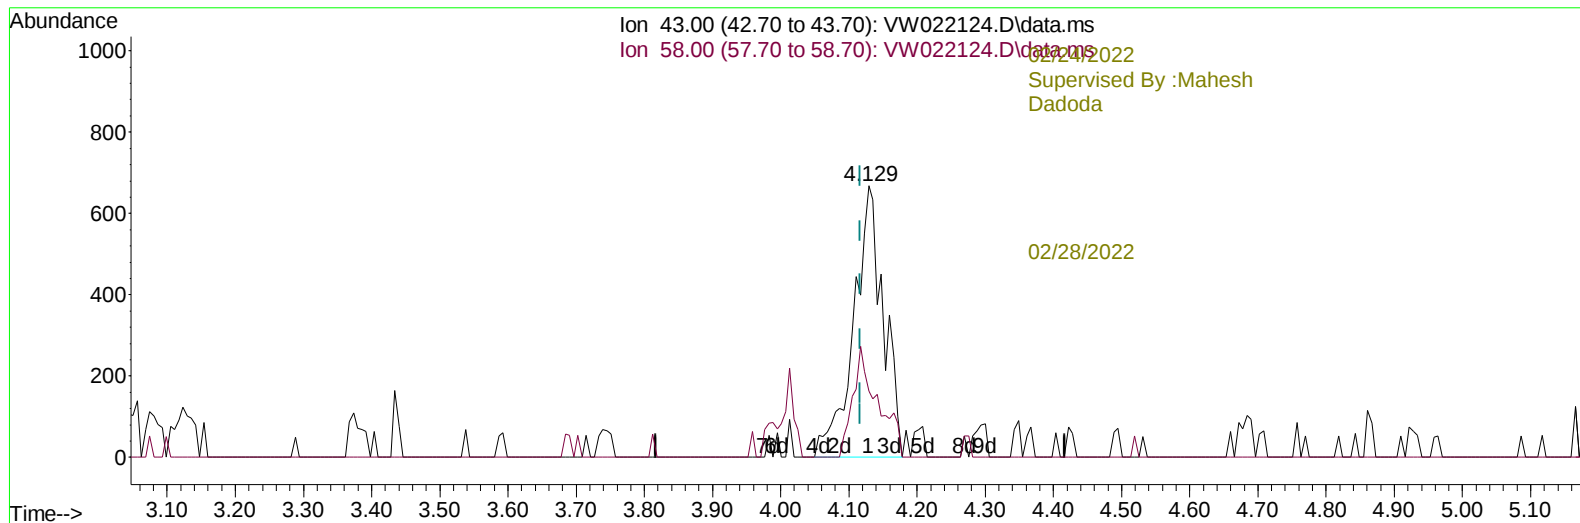

TIC: VW022124.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 6.88 ug/L m

response 2019

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	22.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
 Data File : VW022124.D
 Acq On : 23 Feb 2022 21:50
 Operator : SY/VA
 Sample : N1631-14
 Misc : 6.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRJ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/24/2022
 Supervised By :Mahesh Dadoda 02/28/2022

Quant Time: Feb 24 03:37:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Feb 24 03:35:08 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----02/24/2022							
Supervised By :Mahesh Dadoda							
Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		163826	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		135417	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		41773	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		40631	19.015	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	76.040%		
7) Chloroethane-d5	2.879	69		34456	20.494	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.960%		
11) 1,1-Dichloroethene-d2	4.013	63		46660	14.259	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.040%		
21) 2-Butanone-d5	7.074	46		22218	61.842	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	123.680%		
24) Chloroform-d	7.647	84		86737	23.730	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	94.920%		
26) 1,2-Dichloroethane-d4	8.305	65		47314	24.902	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	99.600%		
32) Benzene-d6	8.275	84		156479	24.829	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	99.320%		
36) 1,2-Dichloropropane-d6	9.275	67		47104	26.913	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	107.640%		
41) Toluene-d8	10.323	98		135676	21.654	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	86.600%		
43) trans-1,3-Dichloroprop...	10.579	79		18227	23.488	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	93.960%		
47) 2-Hexanone-d5	10.921	63		18827	65.403	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	130.800%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		41571	27.064	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	108.240%		
66) 1,2-Dichlorobenzene-d4	13.853	152		32933	24.546	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	98.200%		
Target Compounds							
13) Acetone	4.129	43		2019m	6.881	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022322\
Data File : VW022124.D
Acq On : 23 Feb 2022 21:50
Operator : SY/VA
Sample : N1631-14
Misc : 6.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRJ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/24/2022
Supervised By :Mahesh Dadoda 02/28/2022

Quant Time: Feb 24 03:37:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Feb 24 03:35:08 2022
Response via : Initial Calibration

