


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022421\
Data File : VW018230.D
Acq On : 24 Feb 2021 09:28
Operator : SY/VA
Sample : BFB11
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB111

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022321SMA.M
Title : SFAM01.0
Last Update : Thu Feb 25 02:45:29 2021

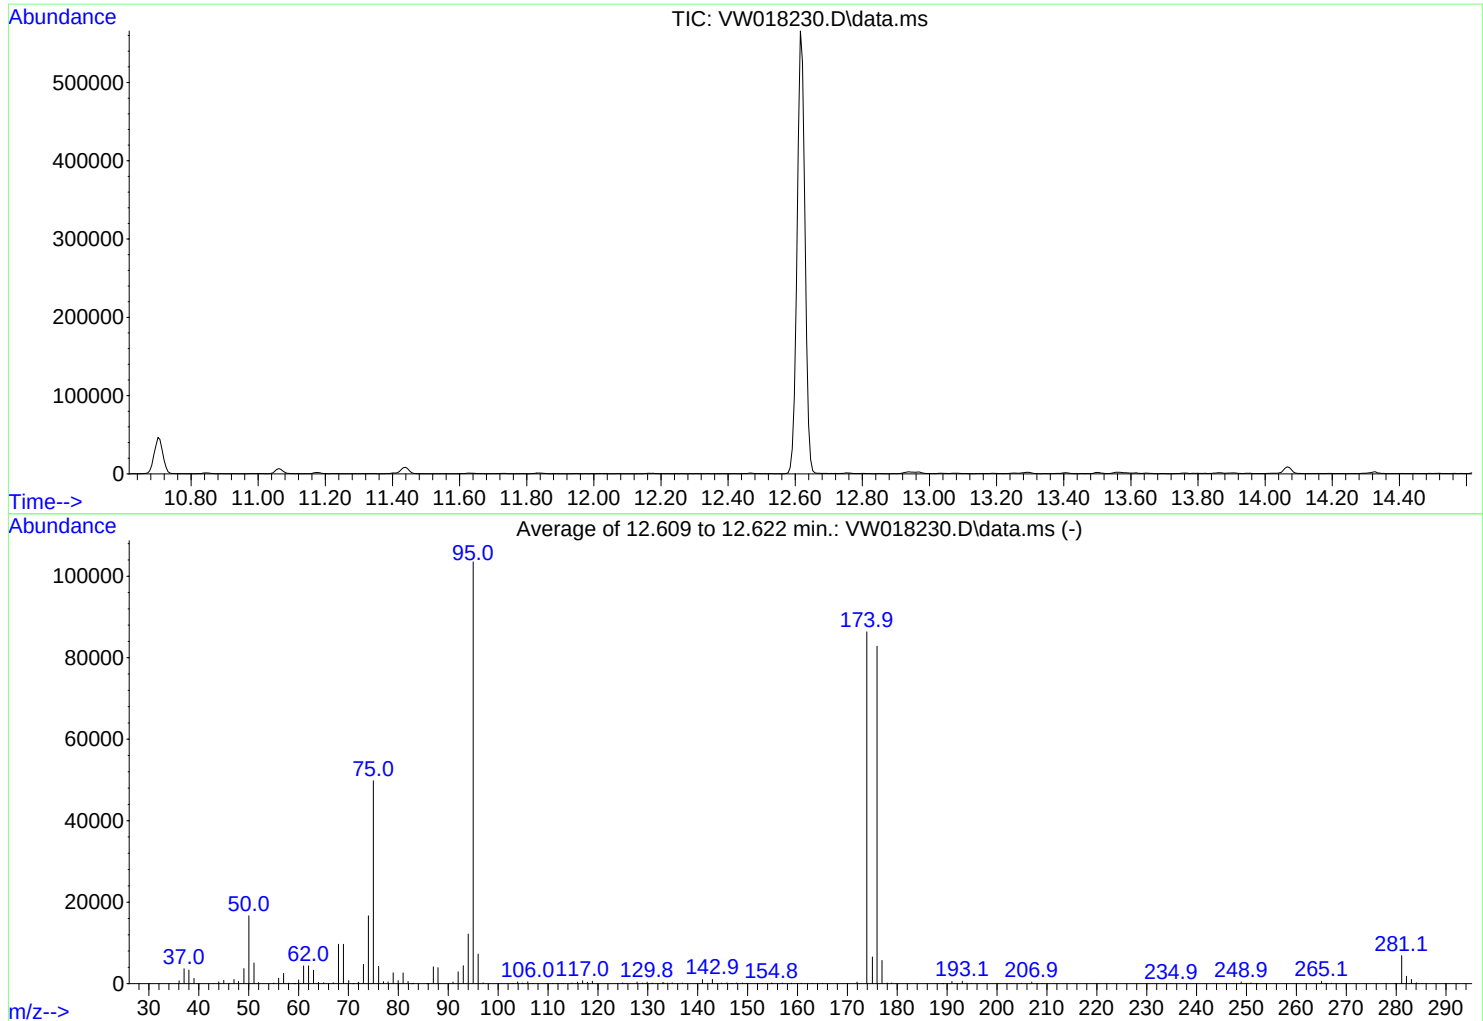

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	16652	PASS
75	95	30	80	48.1	49811	PASS
95	95	100	100	100.0	103541	PASS
96	95	5	9	7.0	7284	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.4	86360	PASS
175	174	5	9	7.6	6554	PASS
176	174	95	105	95.9	82840	PASS
177	176	5	10	6.9	5704	PASS

m/z	Abundance
36.00	630.0
37.10	3469.0
38.00	3063.0
39.10	1232.0
40.00	206.0
42.90	64.0
44.00	608.0
45.00	729.0
46.20	144.0
47.10	1163.0
48.00	469.0
49.00	3144.0
50.10	14395.0
51.00	4650.0
51.90	219.0
54.90	298.0
56.00	1208.0
57.00	2254.0
58.00	136.0
58.90	62.0
59.20	65.0
60.00	849.0
61.00	3712.0
62.00	3987.0
63.00	2858.0
64.00	254.0
65.00	272.0
66.00	73.0
67.00	181.0
68.00	8299.0
69.00	8733.0
70.00	566.0
70.90	61.0
71.90	460.0
73.00	4370.0
74.00	14550.0
75.00	44608.0
76.10	3412.0
77.10	499.0
78.10	444.0
79.00	2102.0
80.00	677.0
80.90	2252.0
81.90	548.0
83.00	97.0
85.70	59.0
87.00	3622.0
87.90	3353.0
91.00	315.0
92.00	2564.0
93.00	3822.0
94.00	9948.0
95.00	87288.0
96.00	6805.0
97.10	161.0
102.80	240.0
103.90	422.0
104.90	150.0
105.90	449.0
106.90	57.0
109.80	79.0
111.00	113.0
111.80	72.0
113.10	99.0
114.70	156.0
115.90	252.0
117.00	646.0
117.80	263.0
118.90	518.0
124.90	214.0
125.60	111.0
127.90	268.0
129.00	201.0
129.80	309.0
130.80	124.0
133.00	751.0
133.90	290.0
134.90	175.0
136.90	194.0
141.00	875.0
141.90	92.0
143.00	920.0
143.90	99.0
144.80	152.0
145.90	191.0
146.80	173.0
147.80	198.0
149.00	154.0
149.90	122.0
153.00	51.0
154.80	223.0
156.90	160.0

Instrument :
MSVOA_W
ClientSampleId :
BFB111

158.70	69.0
160.70	90.0
162.90	121.0
165.00	119.0
172.00	417.0
173.90	63816.0
175.00	5216.0
175.90	61032.0
177.00	4363.0
177.90	211.0
179.00	246.0
189.10	62.0
191.00	754.0
192.00	167.0
193.10	793.0
194.00	200.0
194.90	80.0
202.90	104.0
204.90	163.0
206.90	505.0
208.00	146.0
234.90	98.0
249.00	456.0
250.10	181.0
250.90	252.0
265.00	713.0
265.80	136.0
266.20	148.0
267.00	211.0
279.80	60.0
281.10	8994.0
282.10	2760.0
283.00	1367.0
284.20	233.0
285.20	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB111

m/z	Abundance
36.10	754.0
37.00	3921.0
38.00	3731.0
39.00	1428.0
40.00	136.0
43.00	81.0
44.00	731.0
45.00	844.0
46.20	76.0
47.10	1011.0
48.00	656.0
49.00	4343.0
50.00	19384.0
51.00	5756.0
52.00	302.0
55.10	260.0
56.00	1474.0
57.00	2824.0
58.10	92.0
60.00	1058.0
61.00	4785.0
62.00	4776.0
63.00	3558.0
64.00	404.0
65.10	280.0
66.90	296.0
68.00	11023.0
69.00	10823.0
70.00	866.0
72.10	600.0
73.00	5172.0
74.00	18440.0
75.00	55560.0
76.00	4950.0
77.00	497.0
77.90	456.0
79.00	2909.0
79.90	928.0
80.90	2806.0
81.90	626.0
83.10	115.0
85.90	185.0
87.00	4769.0
88.00	4538.0
90.90	446.0
92.00	3103.0
93.00	4958.0
94.00	13963.0
95.00	117120.0
96.00	7973.0
97.00	274.0
103.10	119.0
103.90	441.0
104.90	161.0
106.00	436.0
107.00	116.0
109.80	81.0
111.00	117.0
111.90	72.0
112.70	67.0
114.80	153.0
115.90	419.0
116.90	781.0
117.90	409.0
118.90	599.0
123.90	72.0
125.00	260.0
125.70	87.0
127.80	405.0
128.90	154.0
129.90	455.0
130.90	215.0
133.20	440.0
134.00	114.0
134.90	323.0
136.80	146.0
141.00	1134.0
142.00	161.0
142.90	1075.0
143.90	85.0
144.80	154.0
145.80	184.0
147.00	134.0
147.80	285.0
149.00	170.0
149.70	167.0
152.00	71.0
152.90	128.0
153.90	65.0
154.80	285.0
157.00	168.0
158.80	120.0

Instrument :
MSVOA_W
ClientSampleId :
BFB111

160.80	149.0
163.00	78.0
165.10	110.0
171.90	441.0
173.90	96496.0
175.00	7265.0
175.90	93224.0
177.00	6186.0
178.00	166.0
178.80	119.0
190.90	583.0
192.00	108.0
193.00	654.0
193.90	126.0
194.80	78.0
205.00	140.0
207.00	451.0
208.20	70.0
209.10	110.0
234.90	76.0
248.90	575.0
250.00	94.0
250.90	243.0
252.00	60.0
265.10	579.0
265.90	153.0
267.10	127.0
281.10	7157.0
282.00	1757.0
283.10	1077.0
284.00	204.0
285.10	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB111

m/z	Abundance
36.00	707.0
37.10	3601.0
38.00	3215.0
39.10	1262.0
40.00	186.0
44.10	590.0
45.00	796.0
47.00	933.0
47.90	493.0
49.10	3596.0
50.00	16178.0
51.10	4767.0
52.00	234.0
55.00	240.0
56.00	1303.0
57.00	2497.0
57.90	87.0
58.90	77.0
60.00	846.0
61.00	4559.0
62.00	4364.0
63.00	3492.0
64.00	291.0
65.00	225.0
67.00	298.0
68.00	9641.0
69.00	9489.0
70.10	781.0
72.00	454.0
73.00	4656.0
74.00	16984.0
75.00	49264.0
76.00	4348.0
76.90	596.0
77.90	414.0
78.90	3004.0
80.00	680.0
81.00	2828.0
82.00	518.0
82.70	57.0
86.10	165.0
87.00	3951.0
88.00	3920.0
90.90	436.0
92.00	3074.0
93.00	4371.0
94.00	12623.0
95.00	106216.0
96.00	7074.0
96.90	222.0
103.10	68.0
103.90	468.0
104.90	132.0
106.00	441.0
106.90	123.0
110.80	63.0
112.00	115.0
112.70	69.0
114.90	130.0
115.90	367.0
117.00	701.0
118.00	396.0
118.90	665.0
123.90	55.0
124.90	100.0
125.20	98.0
125.80	88.0
127.90	493.0
128.90	174.0
129.90	444.0
130.80	154.0
133.20	238.0
134.80	149.0
137.00	162.0
140.90	931.0
142.10	105.0
142.90	1251.0
144.80	133.0
145.80	204.0
146.90	137.0
148.00	239.0
148.90	101.0
150.00	118.0
152.00	70.0
153.90	65.0
155.00	263.0
156.90	178.0
158.90	132.0
160.80	161.0
165.10	57.0
171.90	351.0
173.90	98768.0

Instrument :
MSVOA_W
ClientSampleId :
BFB111

175.00	7181.0
176.00	94264.0
176.90	6564.0
177.90	127.0
178.80	112.0
190.90	301.0
193.00	314.0
194.80	60.0
204.80	112.0
206.90	218.0
208.10	63.0
209.00	67.0
249.00	227.0
250.10	56.0
250.80	92.0
265.00	415.0
266.00	129.0
281.10	4444.0
282.10	859.0
283.00	657.0
284.10	159.0

Instrument :
MSVOA_W
ClientSampleId :
BFB111

m/z	Abundance
40.00	97.0
43.90	217.0

Instrument :
MSVOA_W
ClientSampleId :
BFB111