




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022422\
 Data File : VW022133.D
 Acq On : 24 Feb 2022 12:08
 Operator : SY/VA
 Sample : N1631-14
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRJ0

Manual IntegrationsAPPROVED

Quant Time: Feb 25 04:50:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 25 04:49:00 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/25/2022
 Supervised By :Mahesh Dadoda 02/28/2022

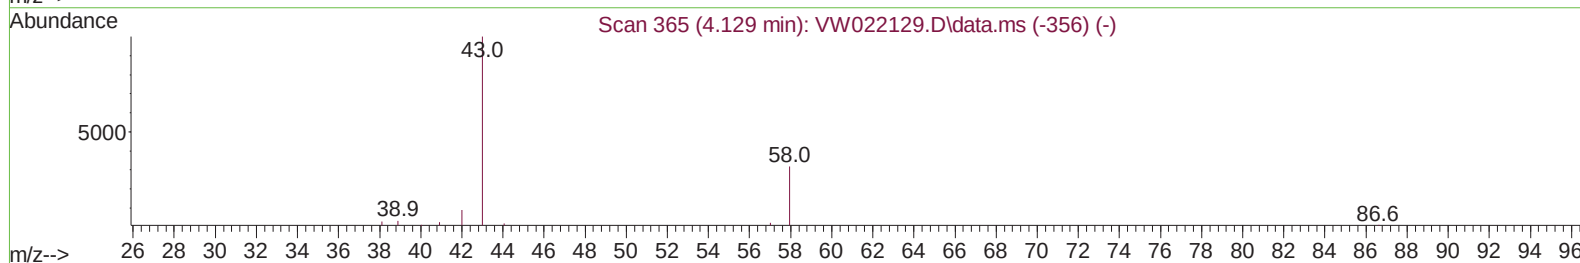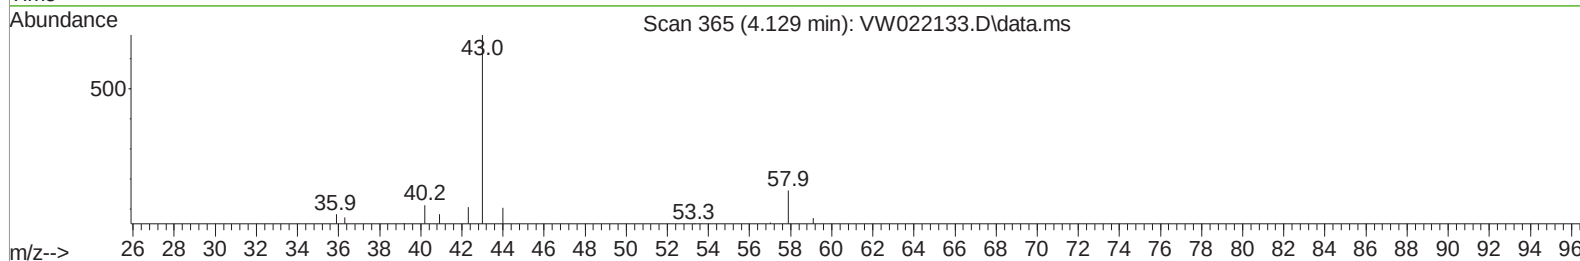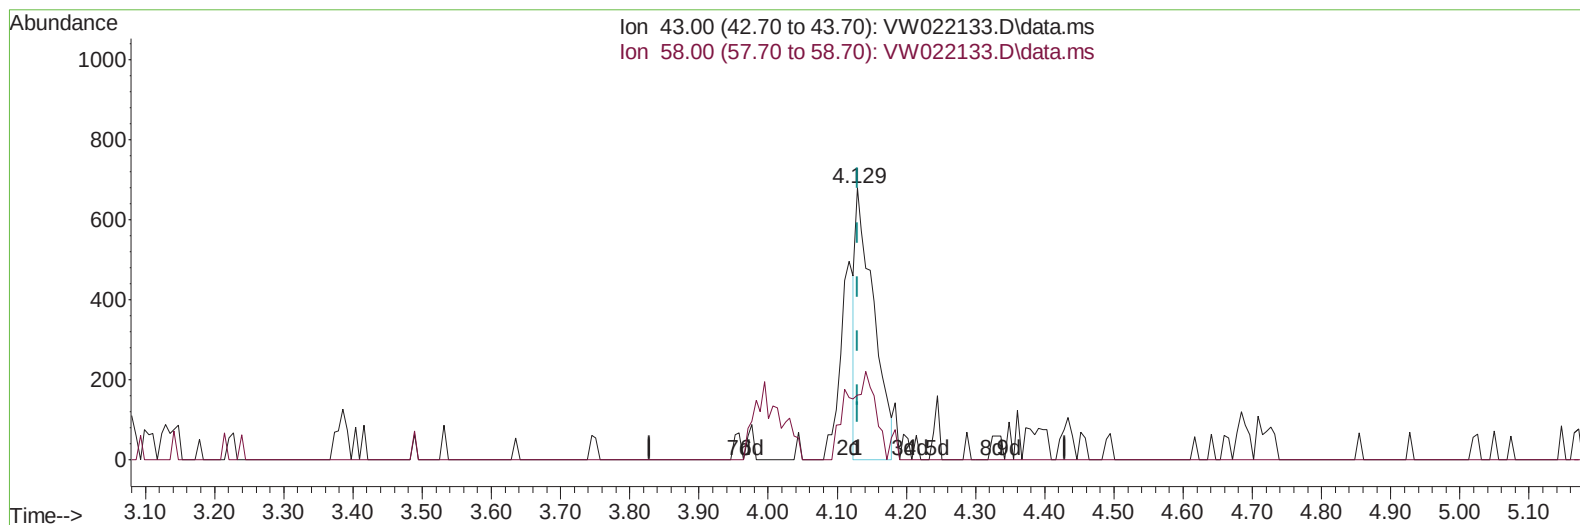

TIC: VW022133.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 3.82 ug/L

response 1215

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	26.34
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022422\
Data File : VW022133.D
Acq On : 24 Feb 2022 12:08
Operator : SY/VA
Sample : N1631-14
Misc : 5.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRJ0

Manual IntegrationsAPPROVED

Quant Time: Feb 25 04:50:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 25 04:49:00 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 02/25/2022
Supervised By :Mahesh Dadoda 02/28/2022

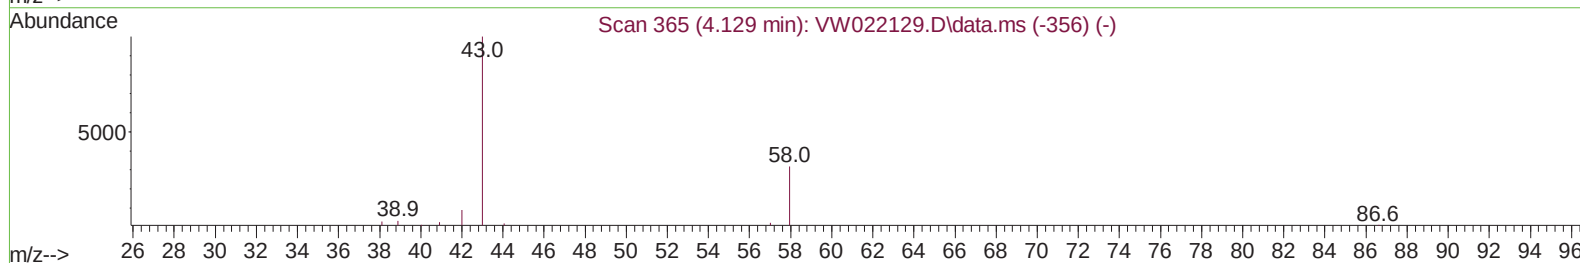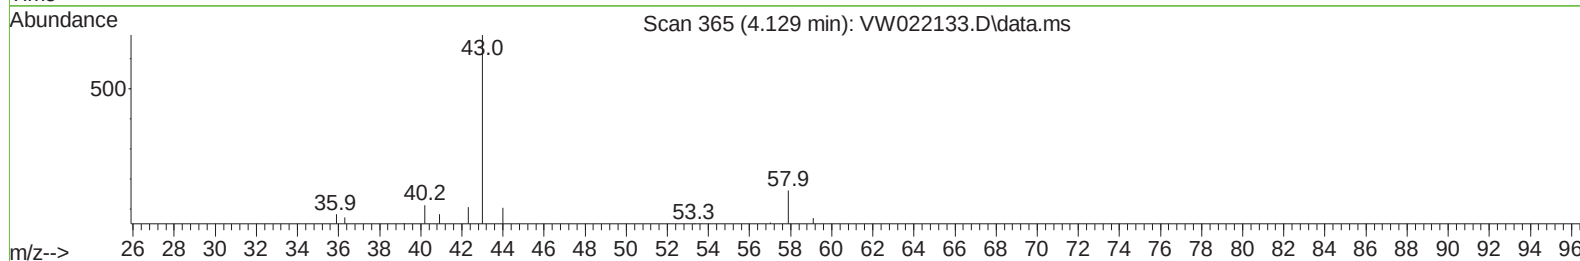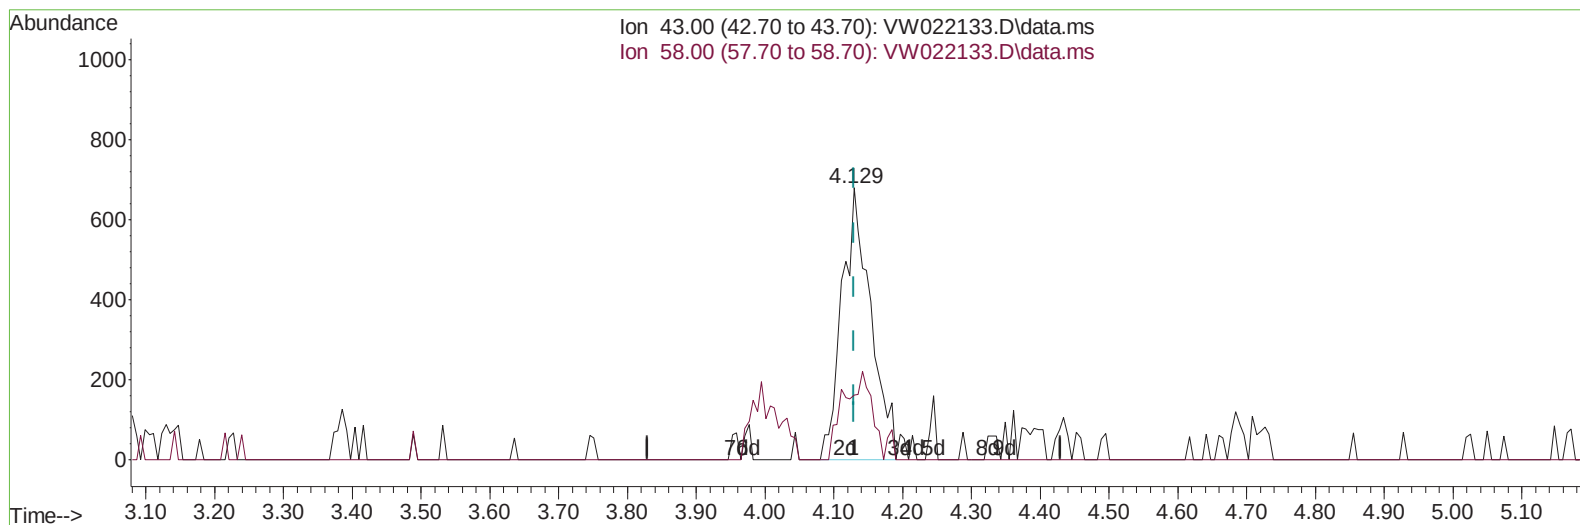

TIC: VW022133.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 6.17 ug/L m

response 1966

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	16.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022422\
 Data File : VW022133.D
 Acq On : 24 Feb 2022 12:08
 Operator : SY/VA
 Sample : N1631-14
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRJ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/25/2022
 Supervised By :Mahesh Dadoda 02/28/2022

Quant Time: Feb 25 04:50:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 25 04:49:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	177759	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	157448	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	63135	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	37023	15.968	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.880%	
7) Chloroethane-d5	2.879	69	29136	15.972	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.880%	
11) 1,1-Dichloroethene-d2	4.013	63	45455	12.802	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.200%	
21) 2-Butanone-d5	7.080	46	18935	48.573	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	97.140%	
24) Chloroform-d	7.647	84	81538	20.559	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.240%	
26) 1,2-Dichloroethane-d4	8.305	65	43006	20.861	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	83.440%	
32) Benzene-d6	8.275	84	150376	20.522	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.080%	
36) 1,2-Dichloropropane-d6	9.274	67	43621	21.436	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	85.760%	
41) Toluene-d8	10.323	98	136823	18.782	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.120%	
43) trans-1,3-Dichloroprop...	10.579	79	16259	18.020	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	72.080%	
47) 2-Hexanone-d5	10.927	63	15515	46.356	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.720%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	38157	21.366	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.480%	
66) 1,2-Dichlorobenzene-d4	13.853	152	41546	20.488	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	81.960%	
Target Compounds						
13) Acetone	4.129	43	1966m	6.175	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022422\
Data File : VW022133.D
Acq On : 24 Feb 2022 12:08
Operator : SY/VA
Sample : N1631-14
Misc : 5.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRJ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 02/25/2022
Supervised By :Mahesh Dadoda 02/28/2022

Quant Time: Feb 25 04:50:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 25 04:49:00 2022
Response via : Initial Calibration

