

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022422\
 Data File : VW022133.D
 Acq On : 24 Feb 2022 12:08
 Operator : SY/VA
 Sample : N1631-14
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRJ0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 02/25/2022
 Supervised By :Mahesh Dadoda 02/28/2022

Quant Time: Feb 25 04:50:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Feb 25 04:49:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	177759	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	157448	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	63135	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	37023	15.968	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.880%		
7) Chloroethane-d5	2.879	69	29136	15.972	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.880%		
11) 1,1-Dichloroethene-d2	4.013	63	45455	12.802	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	51.200%		
21) 2-Butanone-d5	7.080	46	18935	48.573	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.140%		
24) Chloroform-d	7.647	84	81538	20.559	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.240%		
26) 1,2-Dichloroethane-d4	8.305	65	43006	20.861	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.440%		
32) Benzene-d6	8.275	84	150376	20.522	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.080%		
36) 1,2-Dichloropropane-d6	9.274	67	43621	21.436	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.760%		
41) Toluene-d8	10.323	98	136823	18.782	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	75.120%		
43) trans-1,3-Dichloroprop...	10.579	79	16259	18.020	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	72.080%		
47) 2-Hexanone-d5	10.927	63	15515	46.356	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.720%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	38157	21.366	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.480%		
66) 1,2-Dichlorobenzene-d4	13.853	152	41546	20.488	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	81.960%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	1966m	6.175	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022422\
Data File : VW022133.D
Acq On : 24 Feb 2022 12:08
Operator : SY/VA
Sample : N1631-14
Misc : 5.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBRJ0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 02/25/2022
Supervised By :Mahesh Dadoda 02/28/2022


Quant Time: Feb 25 04:50:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Feb 25 04:49:00 2022
Response via : Initial Calibration

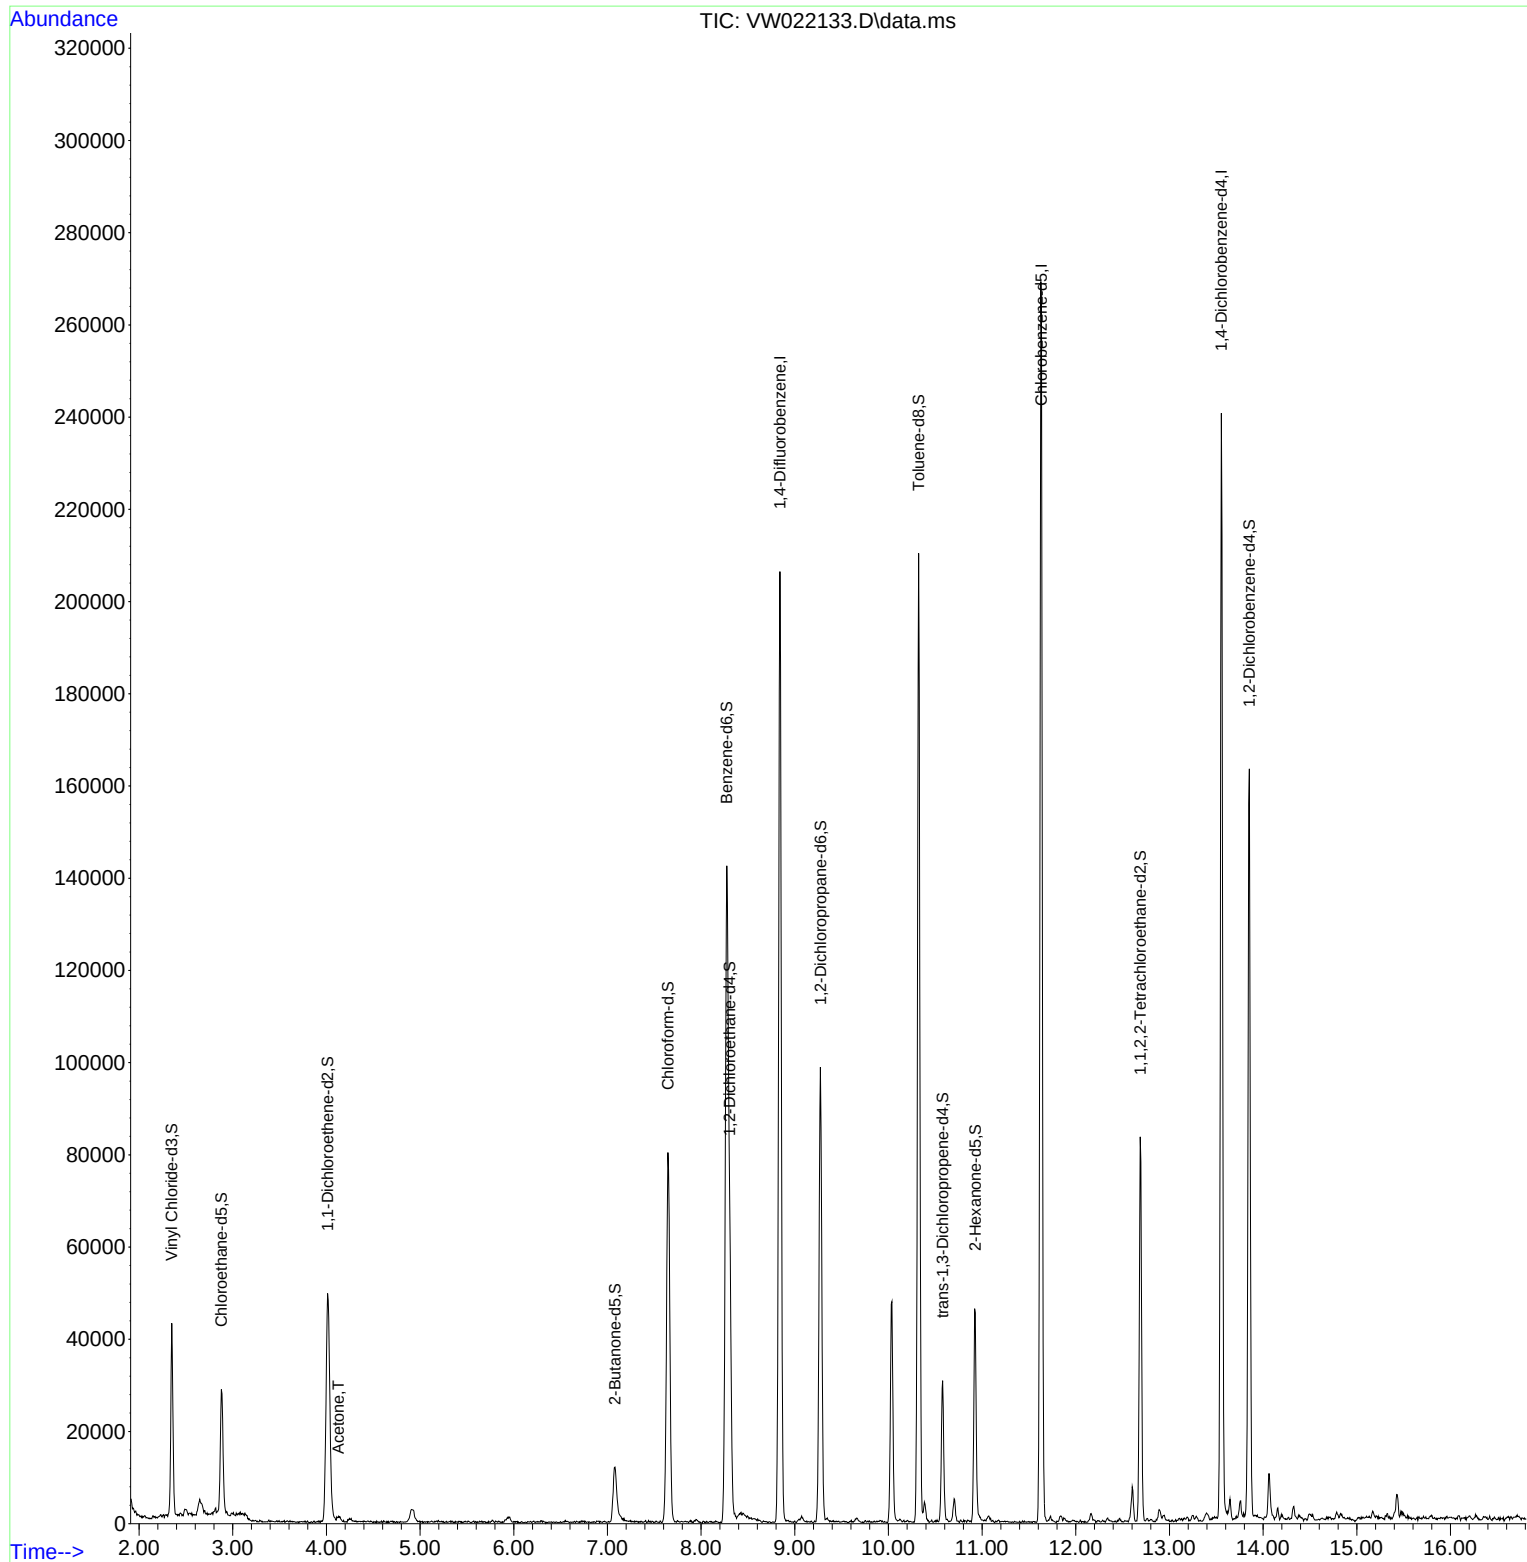

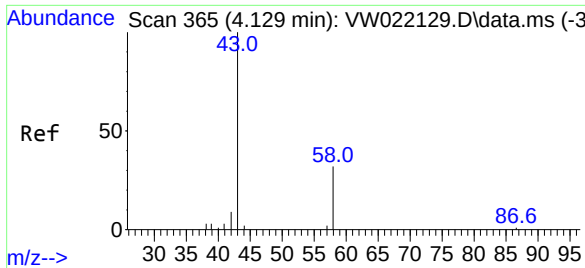

#13
 Acetone
 Concen: 6.175 ug/L m
 RT: 4.129 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW022133.D
 Acq: 24 Feb 2022 12:08

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRJ0

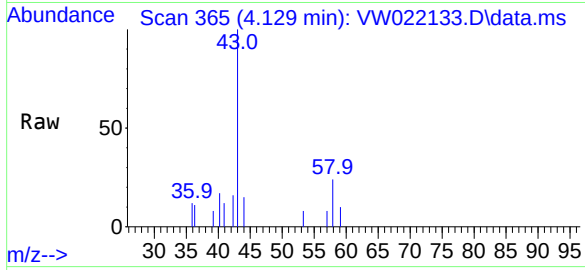

Tgt Ion: 43 Resp: 1960
 Ion Ratio Lower Upper
 43 100
 58 16.3 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 02/25/2022
 Supervised By :Mahesh Dadoda 02/28/2022

