


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW022719\
 Data File : VW008871.D
 Acq On : 27 Feb 2019 23:02
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W022119S.M
 Title : SW846 8260
 Last Update : Fri Feb 22 00:38:32 2019

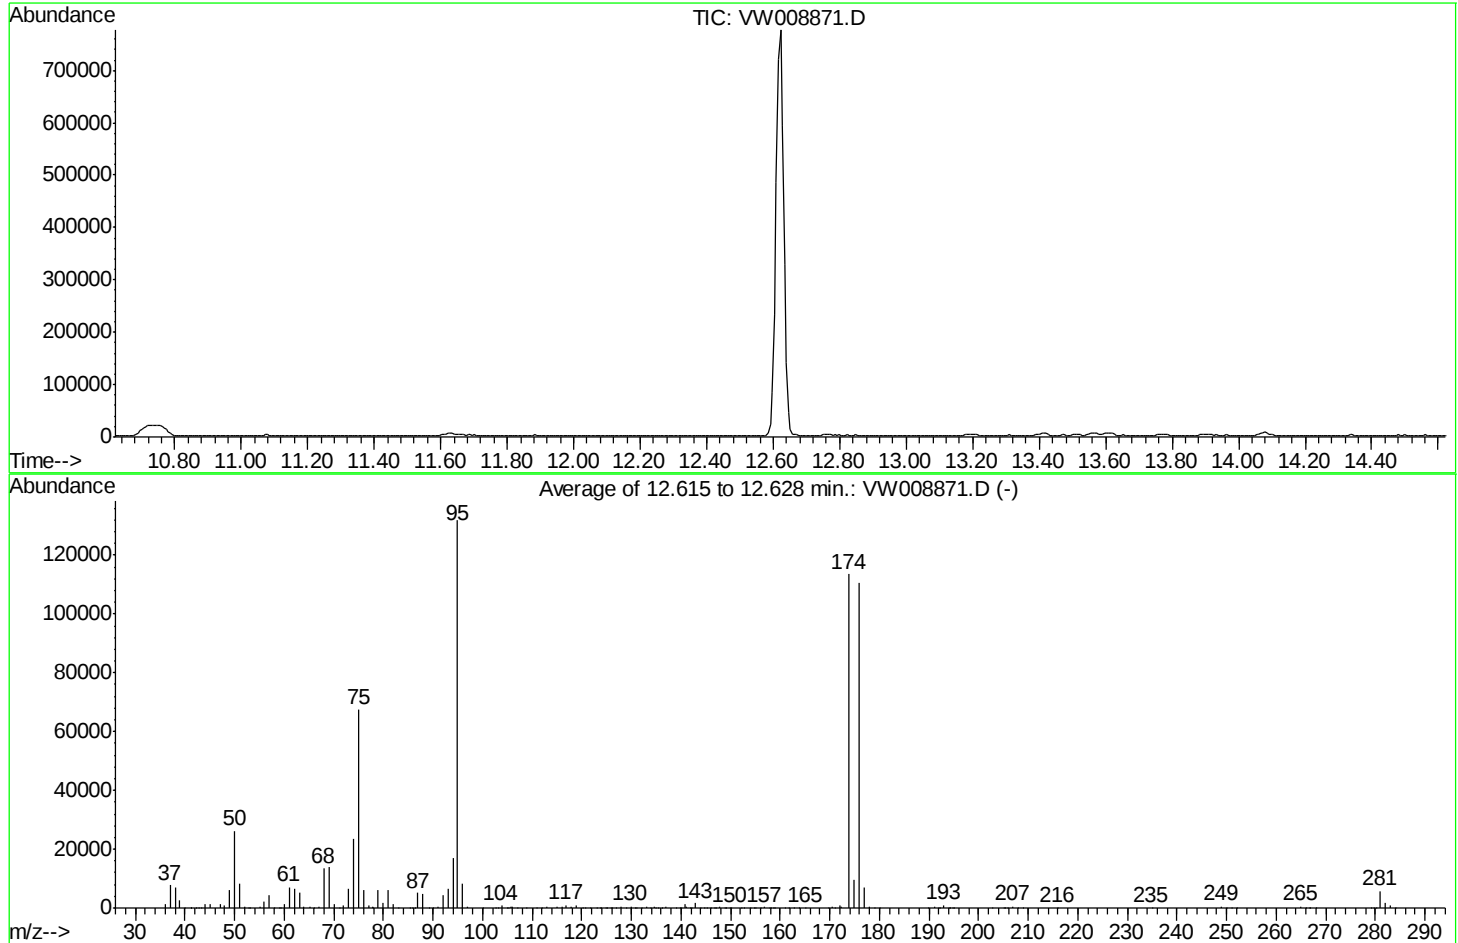

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	26309	PASS
75	95	30	60	51.0	67296	PASS
95	95	100	100	100.0	131840	PASS
96	95	5	9	6.4	8451	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.1	113565	PASS
175	174	5	9	8.3	9459	PASS
176	174	95	101	97.5	110688	PASS
177	176	5	9	6.2	6823	PASS