

Data File : VW015062.D
Acq On : 27 Feb 2020 14:12
Operator : SY/VA
Sample : L1677-15
Misc : 4.03G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CD3

Quant Time: Feb 28 04:02:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	548177	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	475956	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	131316	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	328744	23.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.88%
7) Chloroethane-d5	2.89	69	247457	25.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.16%
10) 1,1-Dichloroethene-d2	4.02	63	401398	18.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.24%
20) 2-Butanone-d5	7.07	46	99813	43.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.10%
24) Chloroform-d	7.65	84	482351	26.78	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.12%
26) 1,2-Dichloroethane-d4	8.31	65	263674	26.17	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.68%
29) Benzene-d6	8.27	84	930695	28.46	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.84%
33) 1,2-Dichloropropane-d6	9.27	67	325534	29.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	118.92%
37) Toluene-d8	10.32	98	741080	27.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.64%
38) trans-1,3-Dichloropropene-	10.57	79	92974	22.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.88%
39) 2-Hexanone-d5	10.92	63	59979	41.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	170803	24.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.56%
61) 1,2-Dichlorobenzene-d4	13.85	152	144729	30.08	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	120.32%#


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.55	75	21994	4.099 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW015062.D
Acq On : 27 Feb 2020 14:12
Operator : SY/VA
Sample : L1677-15
Misc : 4.03G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CD3

Quant Time: Feb 28 04:02:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

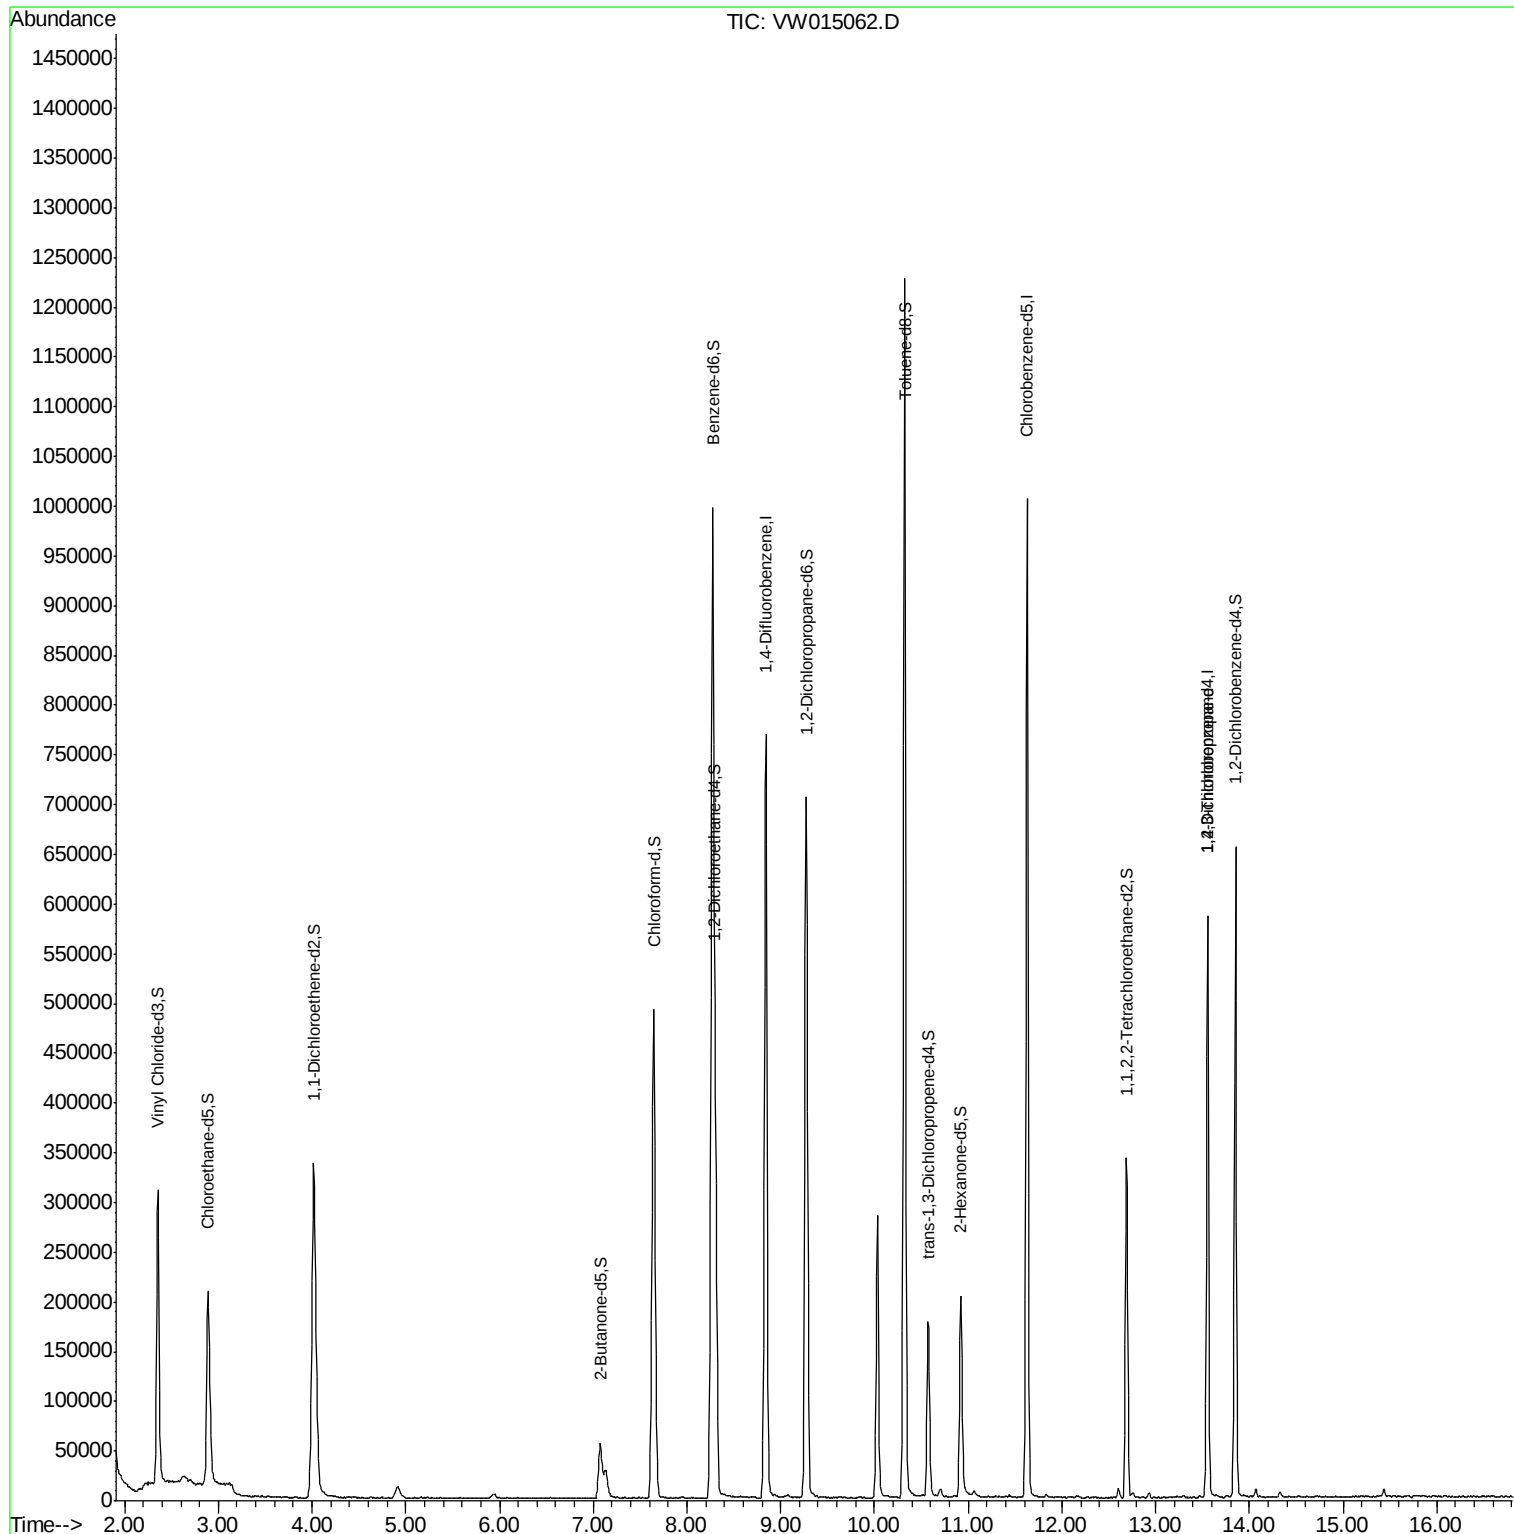

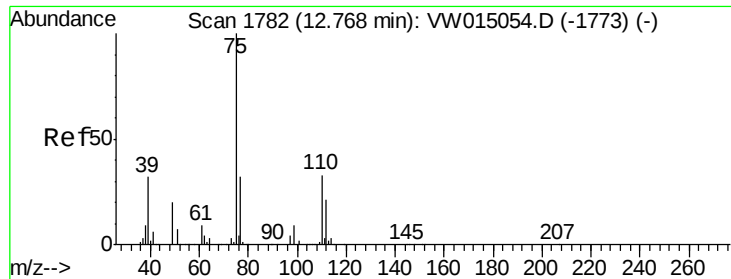

#59

1,2,3-Trichloropropane

Concen: 4.099 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW015062.D

Acq: 27 Feb 2020 14:12

Instrument :

MSVOA_W

ClientSampleId :

C0CD3

Tgt Ion: 75 Resp: 21994

Ion Ratio Lower Upper

75 100

77 35.2 25.4 38.0

