

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (Qedit)




Data File : VW015066.D
Acq On : 27 Feb 2020 15:56
Operator : SY/VA
Sample : L1677-21
Misc : 5.27G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CB8

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:29:57 PM

Quant Time: Feb 28 04:02:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

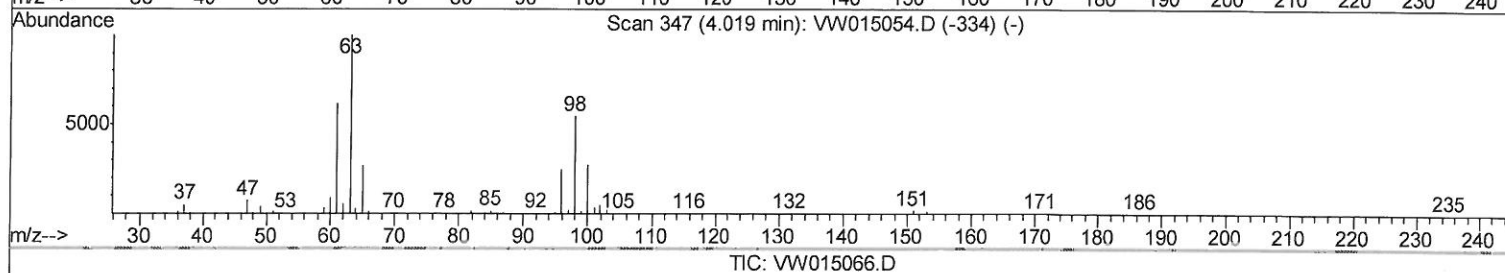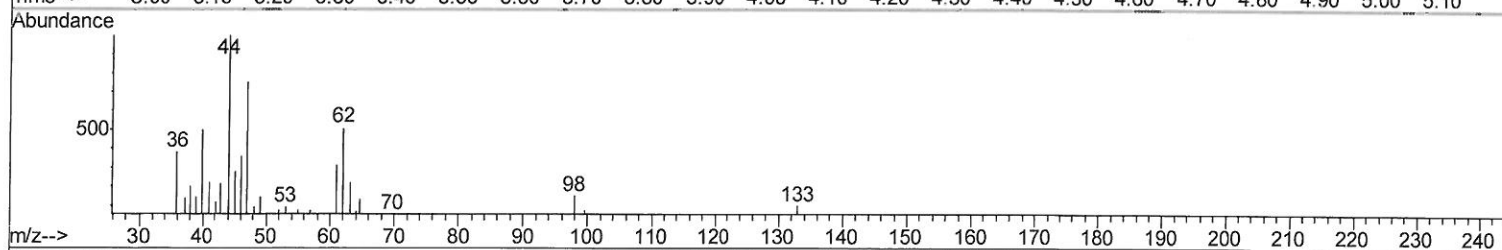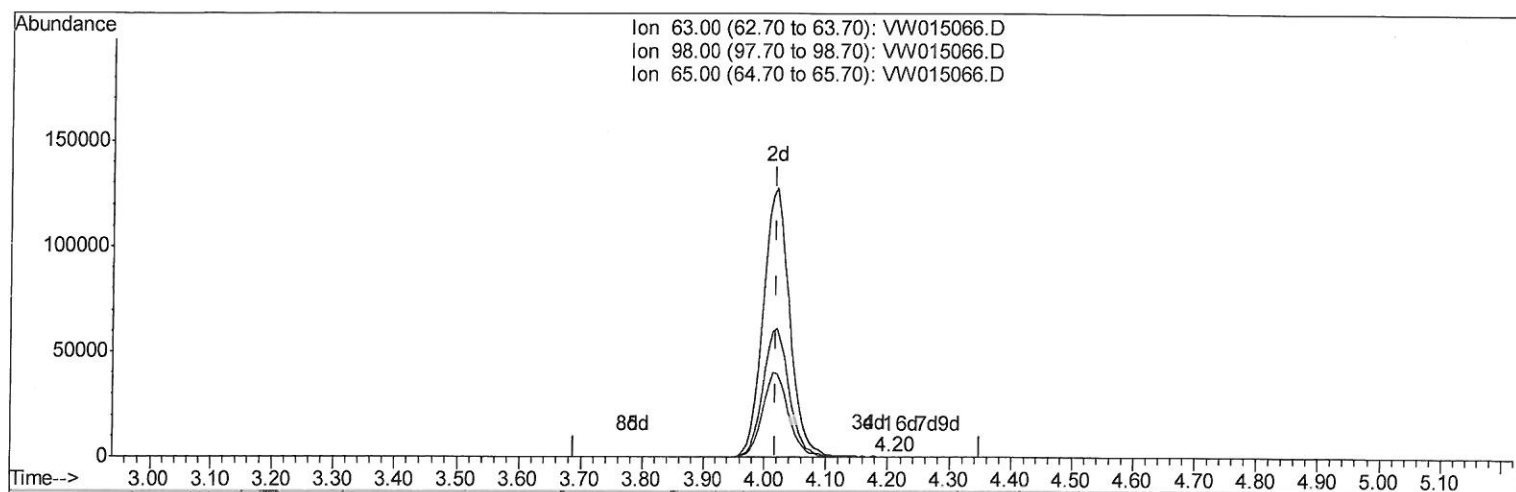

(10) 1,1-Dichloroethene-d2 (S)

4.202min (+0.183) 0.01ug/L

response 285

Ion	Exp%	Act%
63.00	100	100
98.00	61.10	72.98
65.00	23.30	29.12
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (Qedit)




Data File : VW015066.D
Acq On : 27 Feb 2020 15:56
Operator : SY/VA
Sample : L1677-21
Misc : 5.27G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CB8

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:29:57 PM

Quant Time: Feb 28 04:02:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

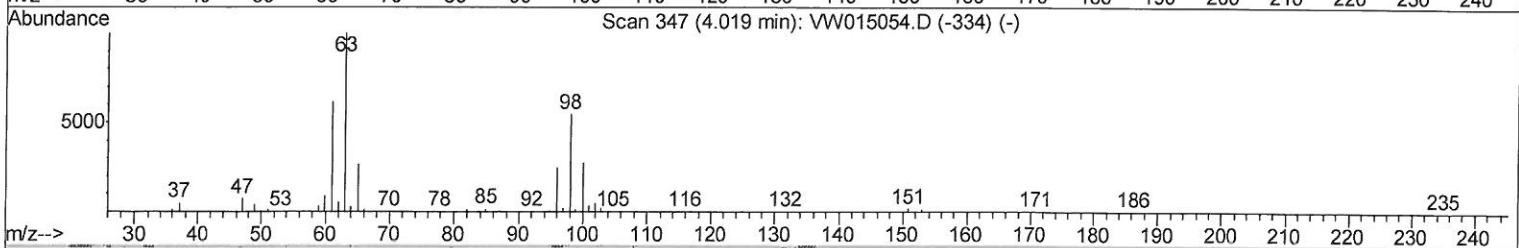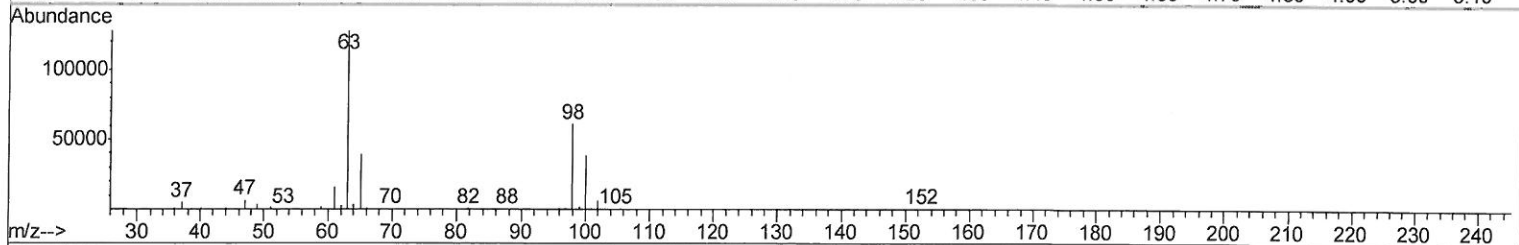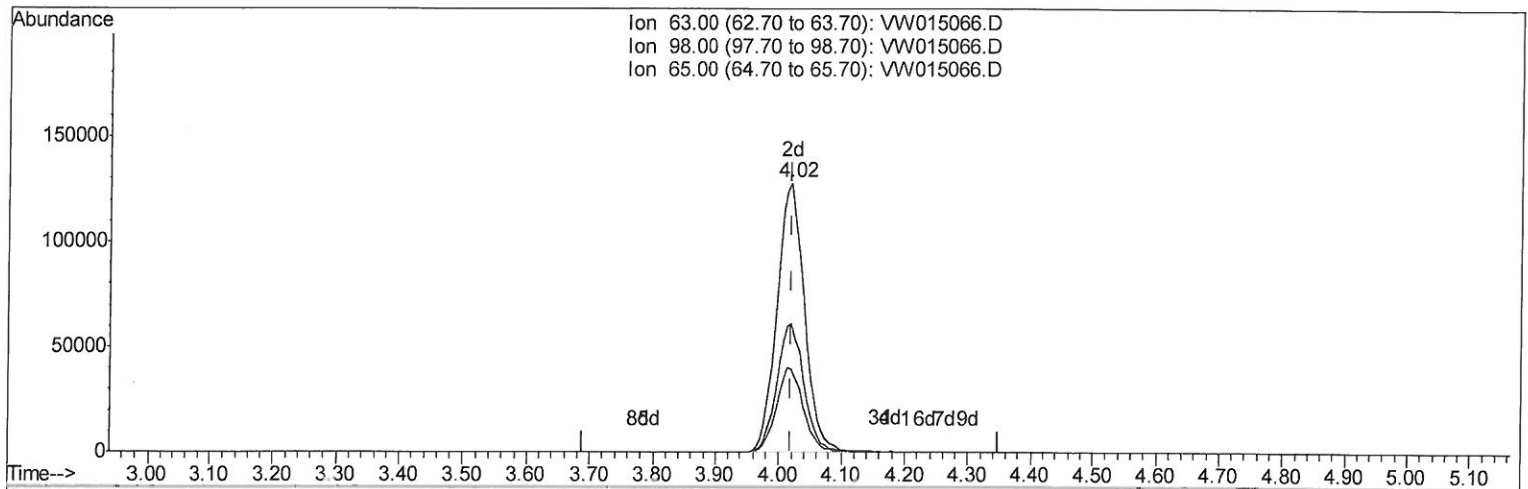

TIC: VW015066.D

(10) 1,1-Dichloroethene-d2 (S)

4.019min (+0.000) 16.31ug/L m

response 384671

Ion	Exp%	Act%
63.00	100	100
98.00	61.10	0.05#
65.00	23.30	0.02#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (Qedit)




Data File : VW015066.D
Acq On : 27 Feb 2020 15:56
Operator : SY/VA
Sample : L1677-21
Misc : 5.27G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CB8

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:29:57 PM

Quant Time: Feb 28 04:02:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

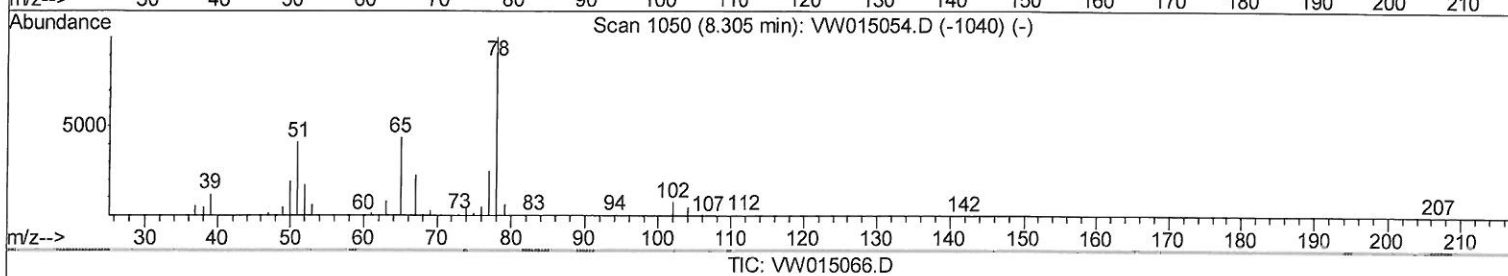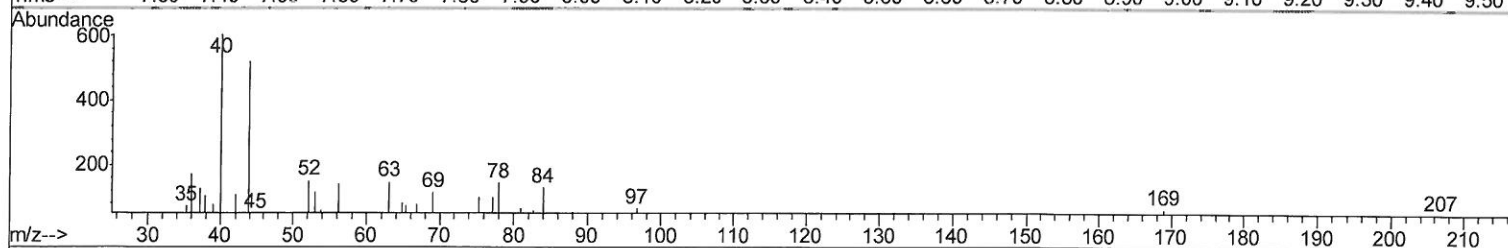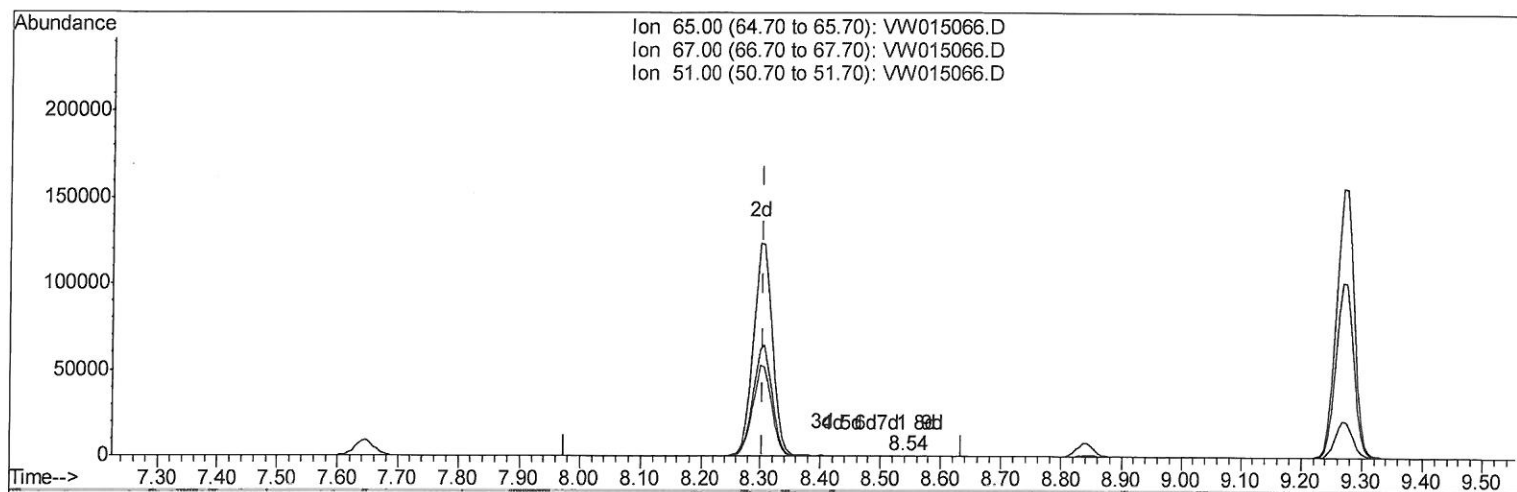

(26) 1,2-Dichloroethane-d4 (S)

8.537min (+0.232) 0.01ug/L

response 107

Ion	Exp%	Act%
65.00	100	100
67.00	53.00	49.53
51.00	129.10	93.46
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (Qedit)




Data File : VW015066.D
Acq On : 27 Feb 2020 15:56
Operator : SY/VA
Sample : L1677-21
Misc : 5.27G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CB8

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:29:57 PM

Quant Time: Feb 28 04:02:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

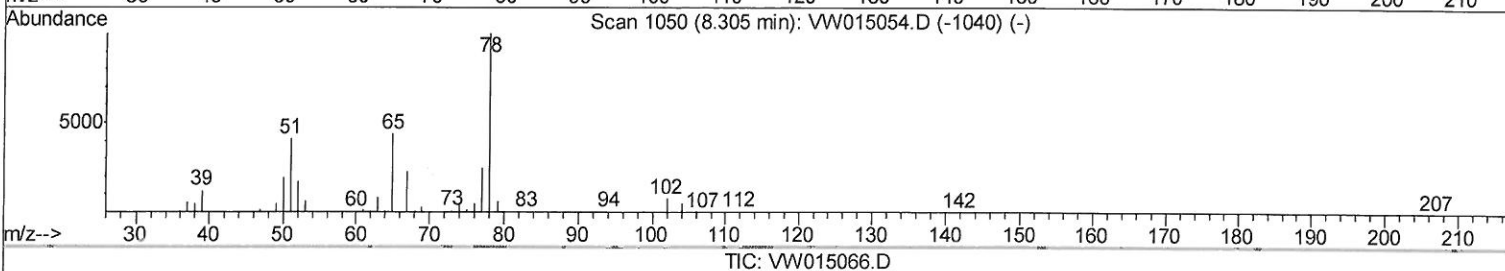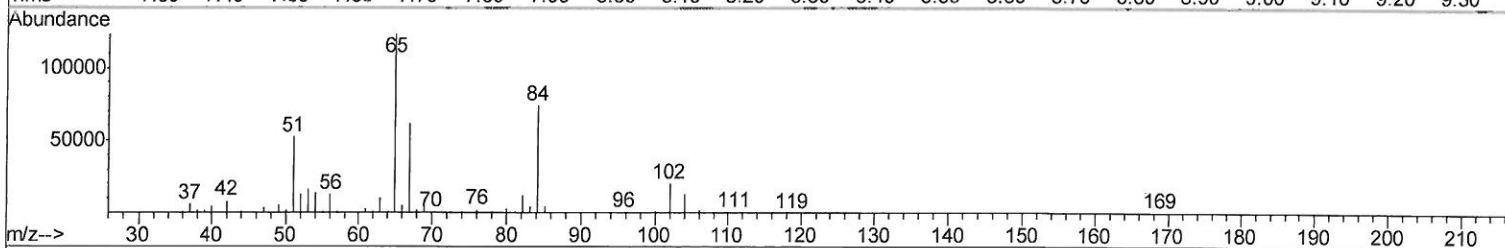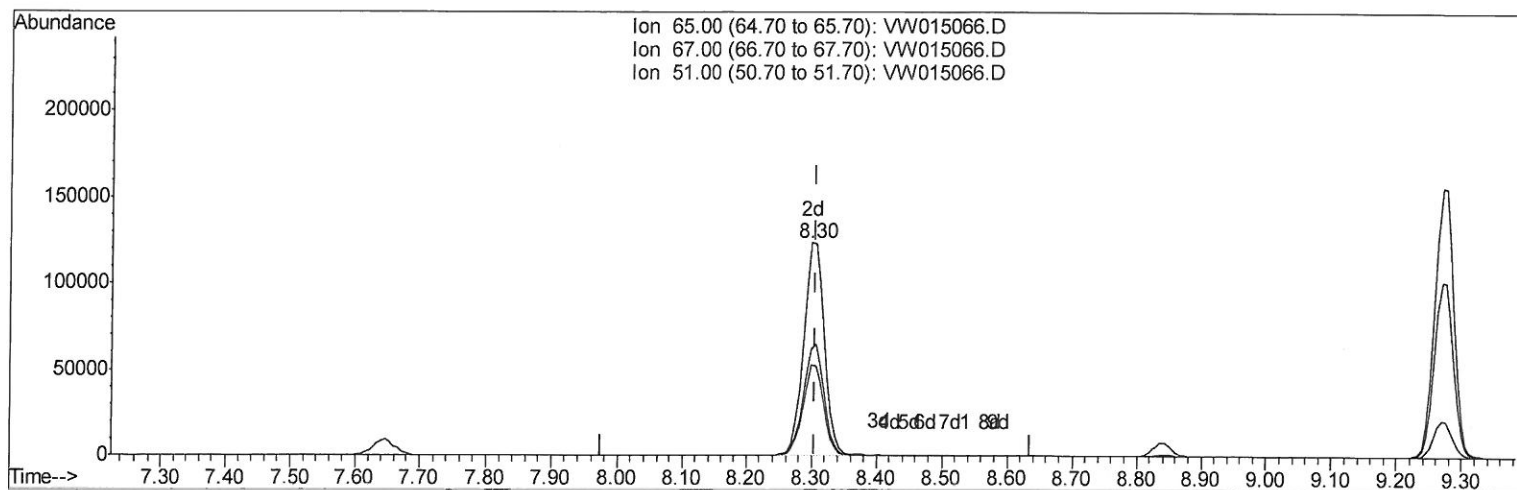

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 24.34ug/L m

response 271061

Ion	Exp%	Act%
65.00	100	100
67.00	53.00	0.02#
51.00	129.10	0.04#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (QT Reviewed)

Data File : VW015066.D
Acq On : 27 Feb 2020 15:56
Operator : SY/VA
Sample : L1677-21
Misc : 5.27G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CB8

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:29:57 PM

Quant Time: Feb 28 04:38:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	605890	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	490231	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	101824	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	317633	20.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.84%
7) Chloroethane-d5	2.89	69	237020	21.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.80%
10) 1,1-Dichloroethene-d2	4.02	63	384671m	16.31	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.24%
20) 2-Butanone-d5	7.07	46	109981	43.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.84%
24) Chloroform-d	7.65	84	471201	23.67	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.68%
26) 1,2-Dichloroethane-d4	8.30	65	271061m	24.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.36%
29) Benzene-d6	8.27	84	906676	26.91	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.64%
33) 1,2-Dichloropropane-d6	9.27	67	319767	28.35	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.40%
37) Toluene-d8	10.32	98	689613	24.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.16%
38) trans-1,3-Dichloropropene-	10.57	79	91277	21.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.60%
39) 2-Hexanone-d5	10.92	63	67259	45.04	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.08%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	184771	25.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	108998	29.22	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	116.88%

02/28/2020

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (QT Reviewed)

Data File : VW015066.D
Acq On : 27 Feb 2020 15:56
Operator : SY/VA
Sample : L1677-21
Misc : 5.27G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0CB8

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:29:57 PM

Quant Time: Feb 28 04:38:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

