

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (Qedit)




Data File : VW015069.D
Acq On : 27 Feb 2020 17:40
Operator : SY/VA
Sample : L1686-02
Misc : 5.43G/10ML/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAW01

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:30:01 PM

Quant Time: Feb 28 04:03:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

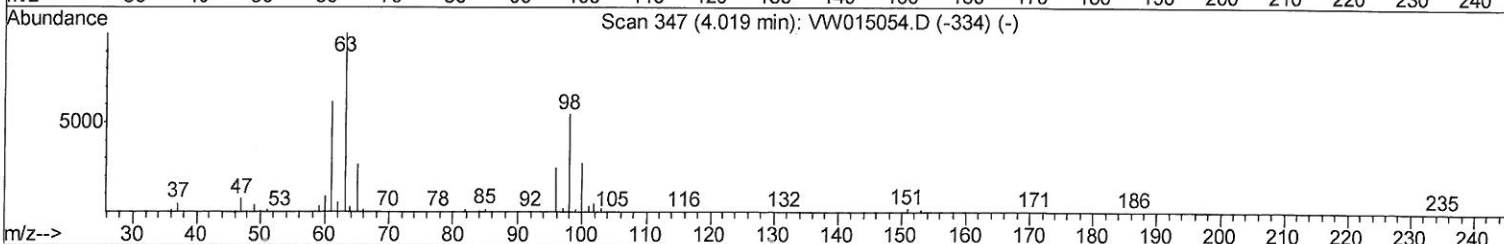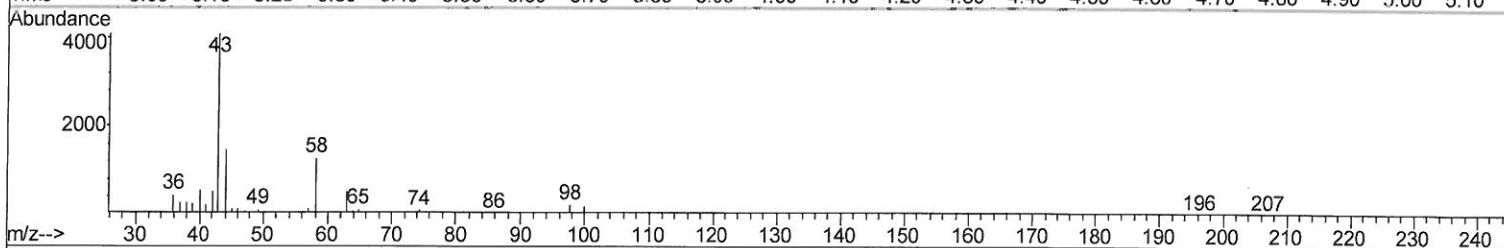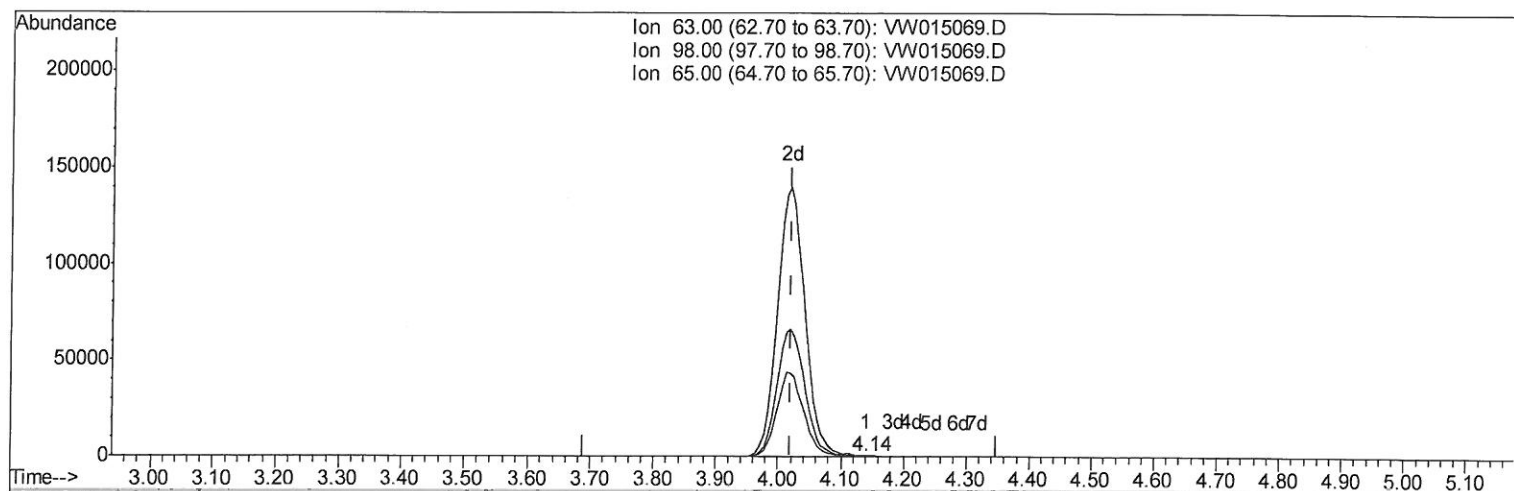

TIC: VW015069.D

(10) 1,1-Dichloroethene-d2 (S)

4.141min (+0.122) 0.04ug/L

response 858

Ion	Exp%	Act%
63.00	100	100
98.00	61.10	60.72
65.00	23.30	30.19
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (Qedit)




Data File : VW015069.D
Acq On : 27 Feb 2020 17:40
Operator : SY/VA
Sample : L1686-02
Misc : 5.43G/10ML/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAW01

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:30:01 PM

Quant Time: Feb 28 04:03:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

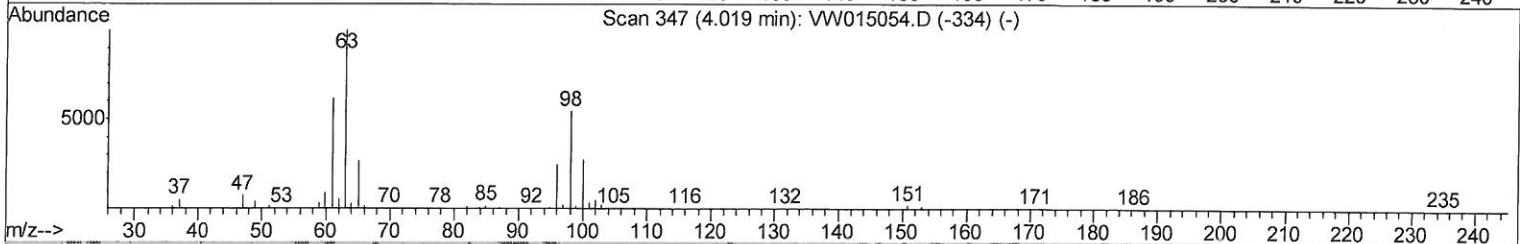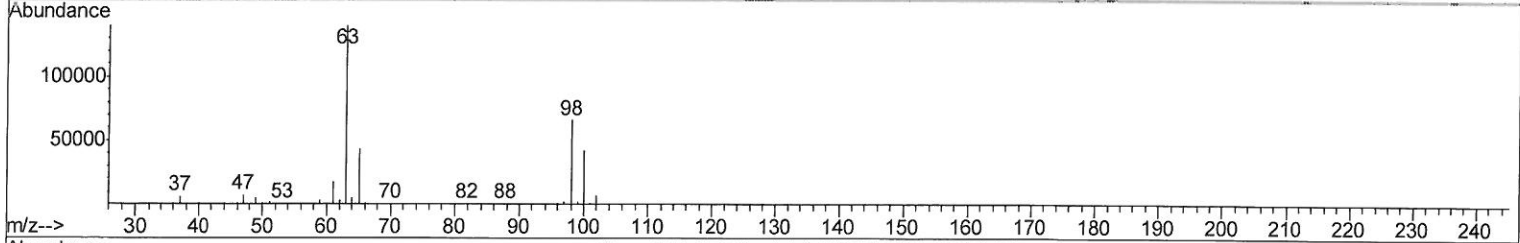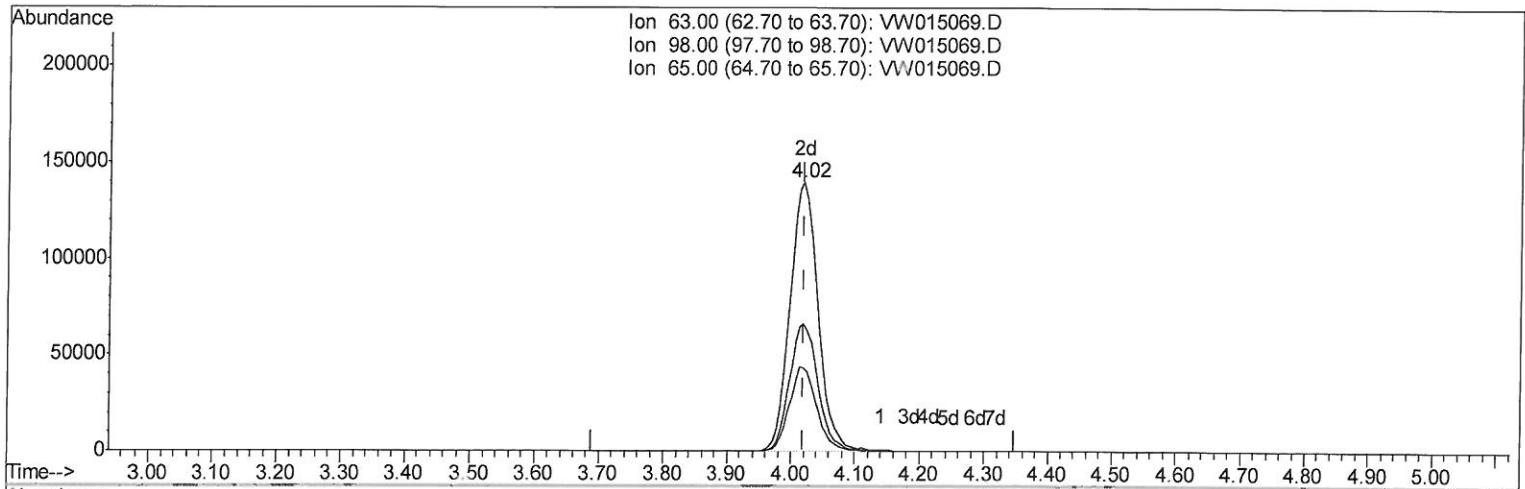

TIC: VW015069.D

(10) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 18.92ug/L m

202/28/2020 SY

response 426218

Ion	Exp%	Act%
63.00	100	100
98.00	61.10	0.12#
65.00	23.30	0.06#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
 Quantitation Report (QT Reviewed)

Data File : VW015069.D
 Acq On : 27 Feb 2020 17:40
 Operator : SY/VA
 Sample : L1686-02
 Misc : 5.43G/10ML/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAW01

Manual Integrations
 APPROVED

MMDadoda
 2/28/2020 12:30:01 PM

Quant Time: Feb 28 04:48:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 28 03:59:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	578840	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	551849	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	191275	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	337322	23.30	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.20%		
7) Chloroethane-d5	2.89	69	251243	24.07	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.28%		
10) 1,1-Dichloroethene-d2	4.02	63	426218m	18.92	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	75.68%		
20) 2-Butanone-d5	7.07	46	168953	69.81	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	139.62%#		
24) Chloroform-d	7.65	84	525730	27.64	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	110.56%		
26) 1,2-Dichloroethane-d4	8.31	65	326001	30.64	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	122.56%		
29) Benzene-d6	8.27	84	1037708	27.36	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	109.44%		
33) 1,2-Dichloropropane-d6	9.27	67	368446	29.02	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	116.08%		
37) Toluene-d8	10.32	98	856080	27.06	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	108.24%		
38) trans-1,3-Dichloropropene-	10.57	79	132944	28.33	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	113.32%		
39) 2-Hexanone-d5	10.92	63	119380	71.02	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	142.04%#		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	265504	32.37	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	129.48%#		
61) 1,2-Dichlorobenzene-d4	13.85	152	229000	32.68	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	130.72%#		

02/28/2020

Target Compounds					Qvalue
5) Vinyl chloride	2.36	62	101230	6.910	ug/L 92
13) Acetone	4.12	43	20238	7.070	ug/L 96
18) trans-1,2-Dichloroethene	5.42	96	34597	3.868	ug/L 94
22) cis-1,2-Dichloroethene	7.17	96	1934560	212.541	ug/L 93
35) Trichloroethene	9.09	95	279739	28.171	ug/L 99
44) Toluene	10.38	91	15828	0.397	ug/L 97
47) Tetrachloroethene	10.86	164	4502	0.703	ug/L 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW022720\
Quantitation Report (QT Reviewed)

Data File : VW015069.D
Acq On : 27 Feb 2020 17:40
Operator : SY/VA
Sample : L1686-02
Misc : 5.43G/10ML/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAW01

Manual Integrations
APPROVED

MMDadoda
2/28/2020 12:30:01 PM

Quant Time: Feb 28 04:48:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022420S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 28 03:59:49 2020
Response via : Initial Calibration

