
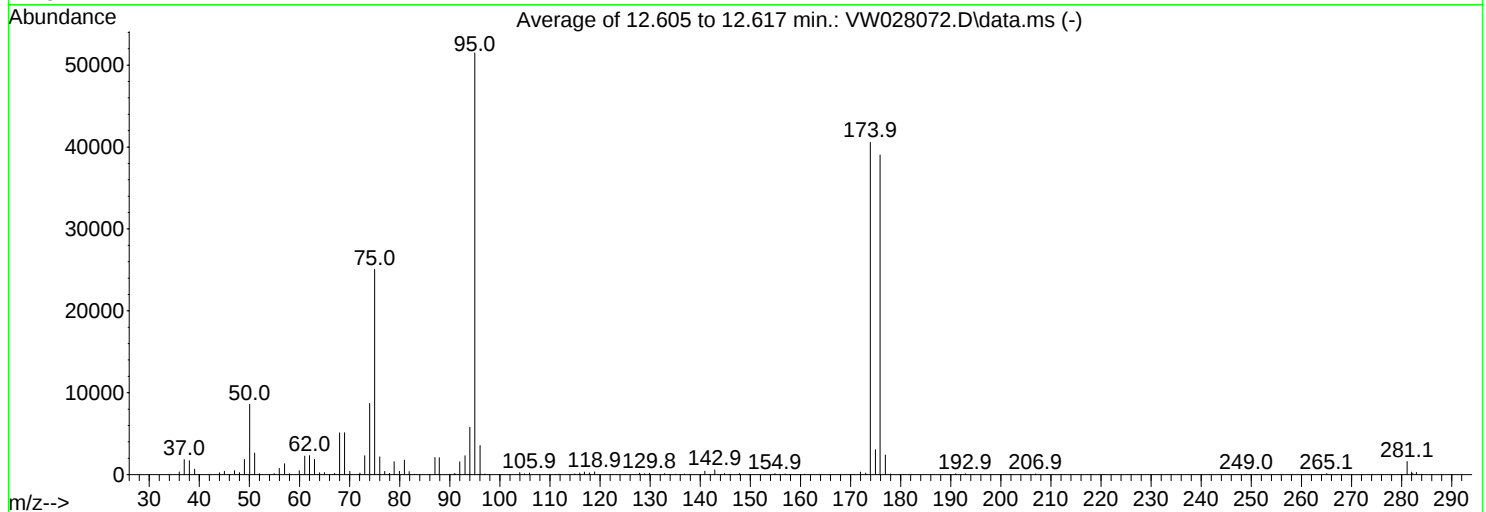


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW022824\
Data File : VW028072.D
Acq On : 28 Feb 2024 09:26
Operator : SY/MD
Sample : BFB444
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB444

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM020524SMA.M
Title : SFAM01.0
Last Update : Wed Feb 28 23:27:15 2024

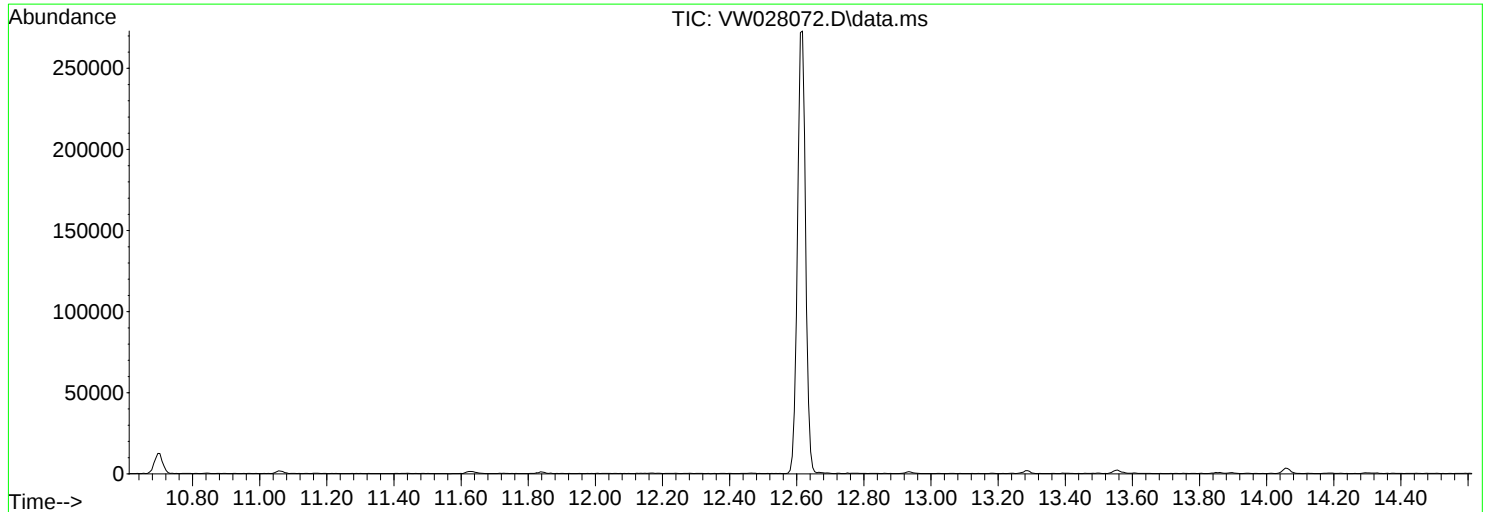

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	8573	PASS
75	95	30	80	48.7	25059	PASS
95	95	100	100	100.0	51501	PASS
96	95	5	9	6.9	3558	PASS
173	174	0.00	2	0.5	193	PASS
174	95	50	120	78.8	40584	PASS
175	174	5	9	7.5	3044	PASS
176	174	95	101	96.2	39040	PASS
177	176	5	9	6.2	2411	PASS

m/z	Abundance
40.00	129.0
44.00	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

m/z	Abundance
36.00	295.0
37.00	1517.0
38.00	1464.0
39.10	551.0
40.00	202.0
44.00	281.0
45.00	386.0
46.10	53.0
47.10	430.0
47.90	275.0
49.00	1610.0
50.00	7067.0
51.00	2109.0
51.90	105.0
54.90	142.0
55.90	595.0
57.00	1201.0
58.00	109.0
59.90	420.0
61.10	1794.0
62.00	1890.0
63.00	1482.0
64.00	198.0
65.00	283.0
67.00	116.0
68.00	4408.0
69.00	4289.0
70.00	349.0
71.90	190.0
73.00	1790.0
74.00	7026.0
75.00	20848.0
76.00	1838.0
77.00	386.0
77.70	138.0
78.90	1397.0
79.90	341.0
80.90	1503.0
81.80	315.0
85.90	58.0
87.10	1821.0
87.90	1799.0
90.90	166.0
92.00	1205.0
93.10	1724.0
94.00	4458.0
95.00	39672.0
96.00	2910.0
97.00	61.0
104.00	204.0
106.00	160.0
111.80	53.0
115.00	96.0
116.00	184.0
116.90	246.0
117.80	188.0
118.90	241.0
125.00	114.0
127.90	126.0
128.90	63.0
130.00	137.0
132.90	195.0
133.80	51.0
136.80	56.0
140.90	233.0
141.80	64.0
142.90	392.0
144.90	91.0
145.80	75.0
147.80	122.0
154.90	109.0
157.00	61.0
171.90	268.0
173.90	28288.0
175.00	1808.0
175.90	28232.0
176.90	1817.0
178.00	98.0
191.00	174.0
193.00	191.0
207.00	143.0
249.00	161.0
249.80	55.0
250.80	56.0
265.10	128.0
266.90	68.0
281.10	2094.0
282.00	663.0
283.00	455.0
284.00	113.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

m/z	Abundance
36.10	401.0
37.00	2011.0
38.00	1973.0
39.10	802.0
40.00	145.0
44.00	330.0
45.00	418.0
46.90	474.0
48.00	305.0
49.00	2043.0
50.10	9404.0
51.10	3121.0
52.00	140.0
54.90	155.0
56.00	818.0
57.00	1517.0
58.00	126.0
60.00	602.0
61.00	2629.0
62.00	2576.0
63.00	1976.0
64.00	261.0
64.90	294.0
67.00	200.0
68.00	5536.0
69.00	5533.0
70.10	504.0
72.10	242.0
73.00	2748.0
74.00	9476.0
75.00	28424.0
76.00	2412.0
77.00	428.0
77.90	281.0
78.90	1620.0
80.00	397.0
80.90	1763.0
81.90	442.0
82.90	65.0
85.90	73.0
87.00	2104.0
87.90	2186.0
90.90	224.0
92.00	1694.0
93.00	2613.0
94.00	6383.0
95.00	58448.0
96.10	3702.0
97.00	70.0
103.90	308.0
104.90	104.0
105.80	214.0
111.10	59.0
111.80	53.0
114.90	65.0
115.90	247.0
116.80	400.0
117.90	257.0
118.90	397.0
127.90	202.0
128.90	126.0
129.80	239.0
132.90	126.0
135.10	69.0
136.90	86.0
140.90	426.0
142.90	715.0
144.80	146.0
145.90	66.0
147.90	125.0
154.80	136.0
156.90	112.0
157.80	61.0
159.00	57.0
160.80	67.0
172.00	300.0
174.00	48528.0
175.00	3228.0
175.90	39400.0
177.00	2796.0
178.00	70.0
191.00	99.0
192.80	179.0
206.90	104.0
248.70	116.0
265.10	154.0
281.10	1523.0
282.20	415.0
282.90	157.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444

m/z	Abundance
35.90	303.0
37.00	1978.0
38.00	1662.0
39.00	624.0
40.00	157.0
44.00	310.0
45.00	435.0
46.10	74.0
47.00	543.0
48.10	204.0
49.00	1920.0
50.10	9249.0
51.10	2667.0
52.00	116.0
55.00	139.0
56.00	896.0
57.00	1277.0
58.10	74.0
60.00	460.0
61.10	2355.0
62.00	2511.0
63.00	2111.0
64.00	250.0
65.00	178.0
67.00	138.0
68.00	5355.0
69.00	5542.0
70.10	381.0
72.00	336.0
73.00	2393.0
74.00	9603.0
75.00	25904.0
76.00	2286.0
77.00	366.0
78.00	212.0
78.90	1742.0
80.00	486.0
81.00	2094.0
82.00	379.0
82.90	83.0
87.00	2327.0
87.90	2244.0
91.10	215.0
92.00	1821.0
93.00	2569.0
94.00	6505.0
95.00	56384.0
96.00	4063.0
97.00	111.0
104.00	242.0
104.90	167.0
105.90	226.0
111.80	79.0
114.90	135.0
115.90	152.0
116.90	310.0
117.90	225.0
118.90	344.0
127.90	188.0
128.90	153.0
129.80	158.0
133.00	97.0
135.10	93.0
136.90	83.0
140.90	647.0
142.90	658.0
144.90	175.0
147.90	138.0
149.80	73.0
152.80	55.0
155.00	190.0
156.90	119.0
160.80	82.0
170.70	61.0
171.90	368.0
173.00	580.0
174.00	44936.0
174.90	4096.0
175.90	49488.0
176.90	2621.0
177.90	56.0
191.10	72.0
206.90	56.0
251.10	70.0
264.90	115.0
281.00	1204.0
282.00	266.0
283.00	214.0

Instrument :
MSVOA_W
ClientSampleId :
BFB444