

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030119\
Quantitation Report (LSC Reviewed)


Data File : VW008918.D
Acq On : 01 Mar 2019 13:02
Operator : SY/VA
Sample : K1657-01
Misc : 7.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB647

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:19 PM

Quant Time: Mar 04 17:25:59 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

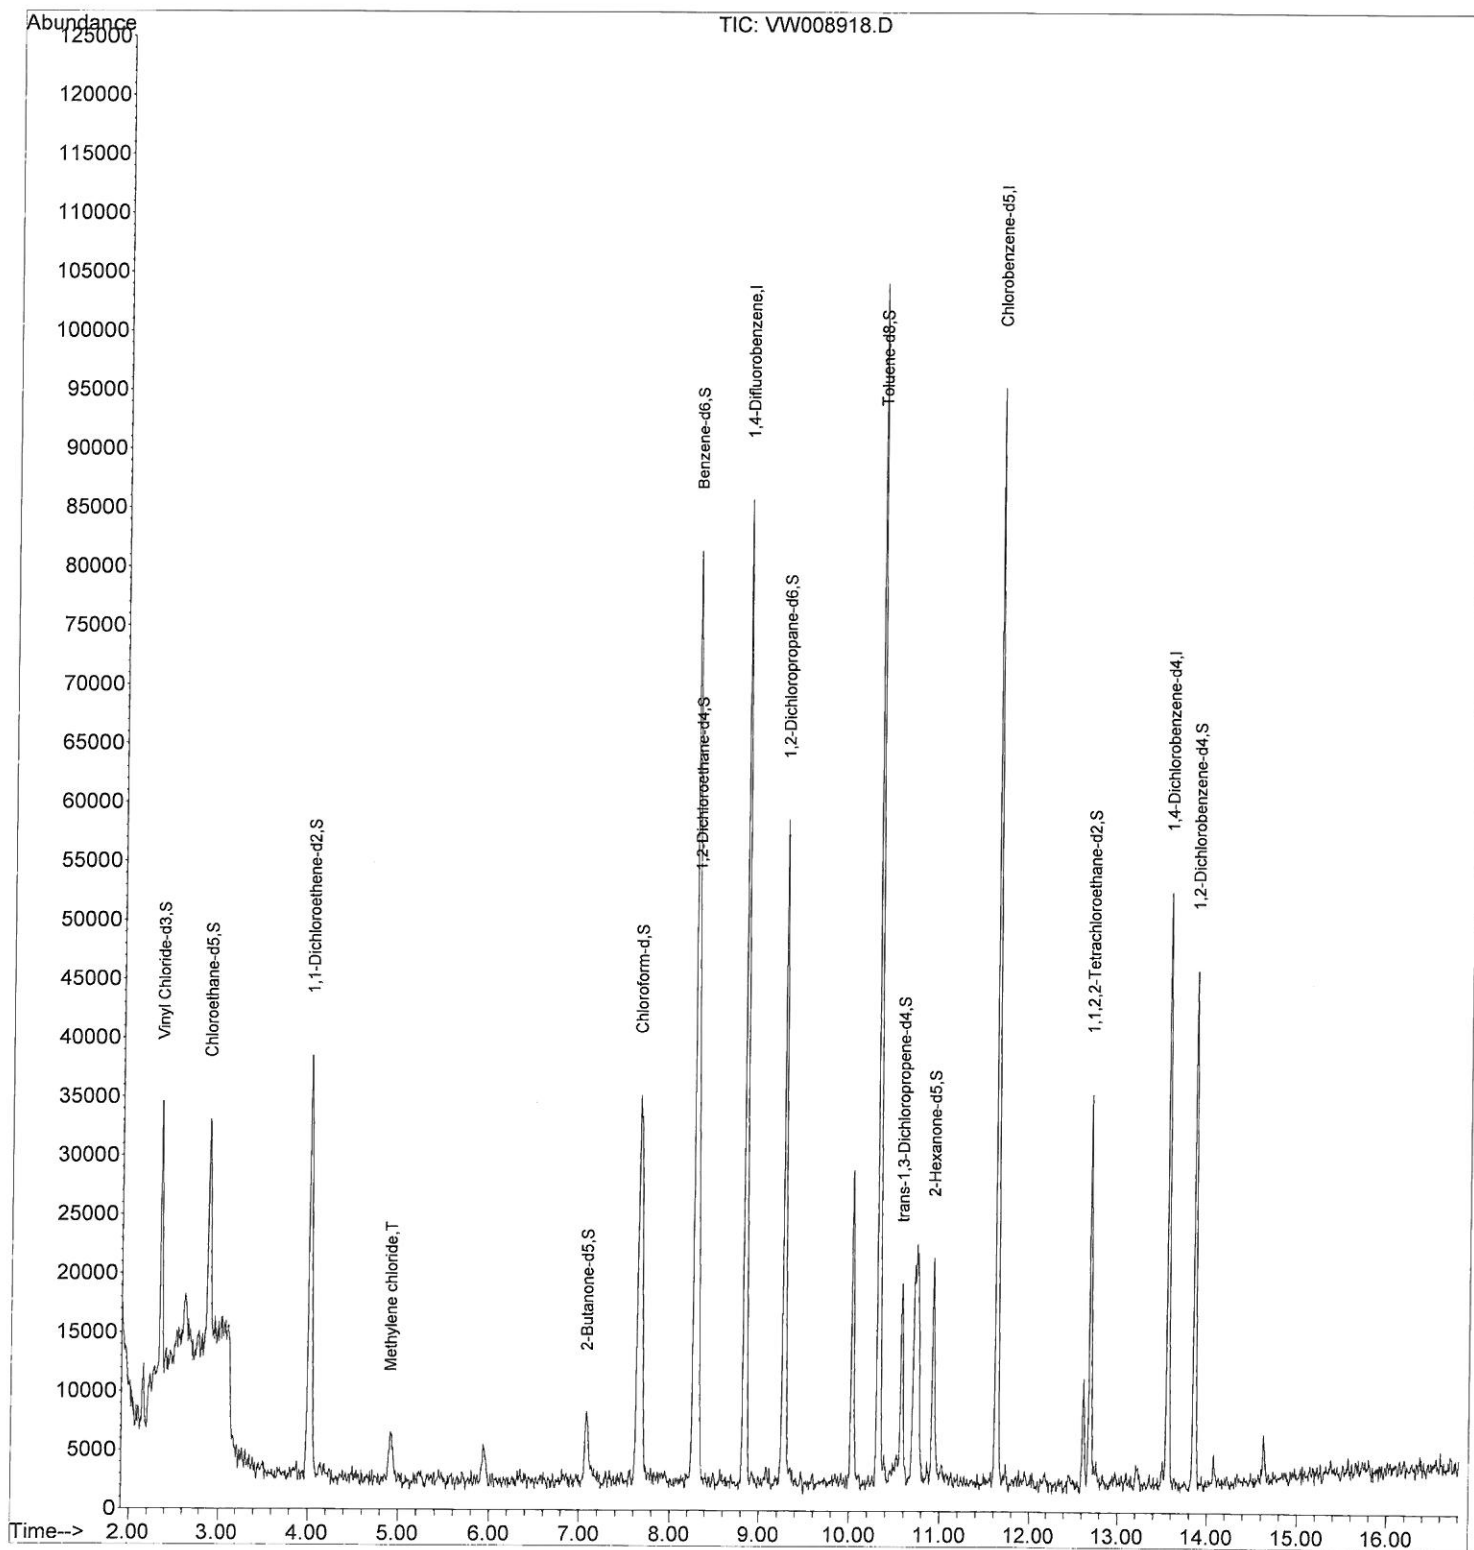

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008918.D
Acq On : 01 Mar 2019 13:02
Operator : SY/VA
Sample : K1657-01
Misc : 7.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB647

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:19 PM

Quant Time: Mar 02 02:58:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

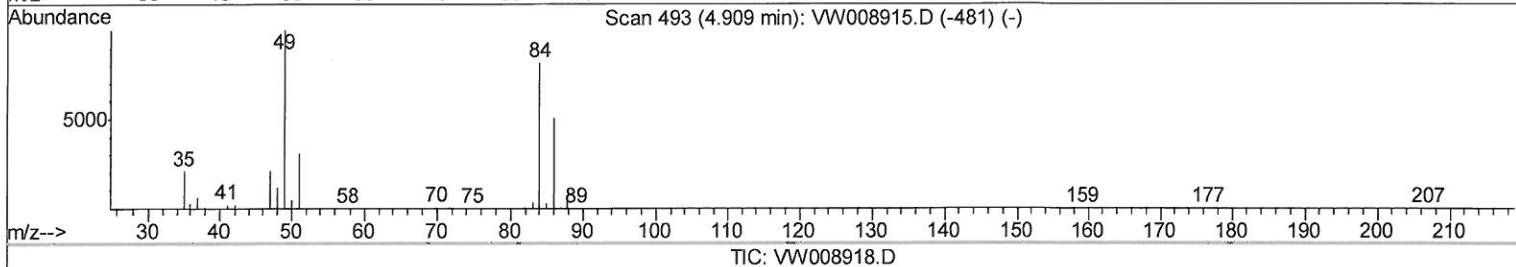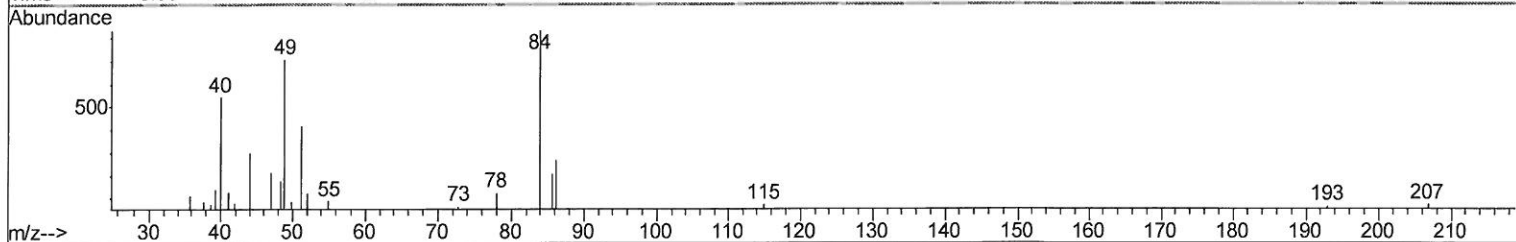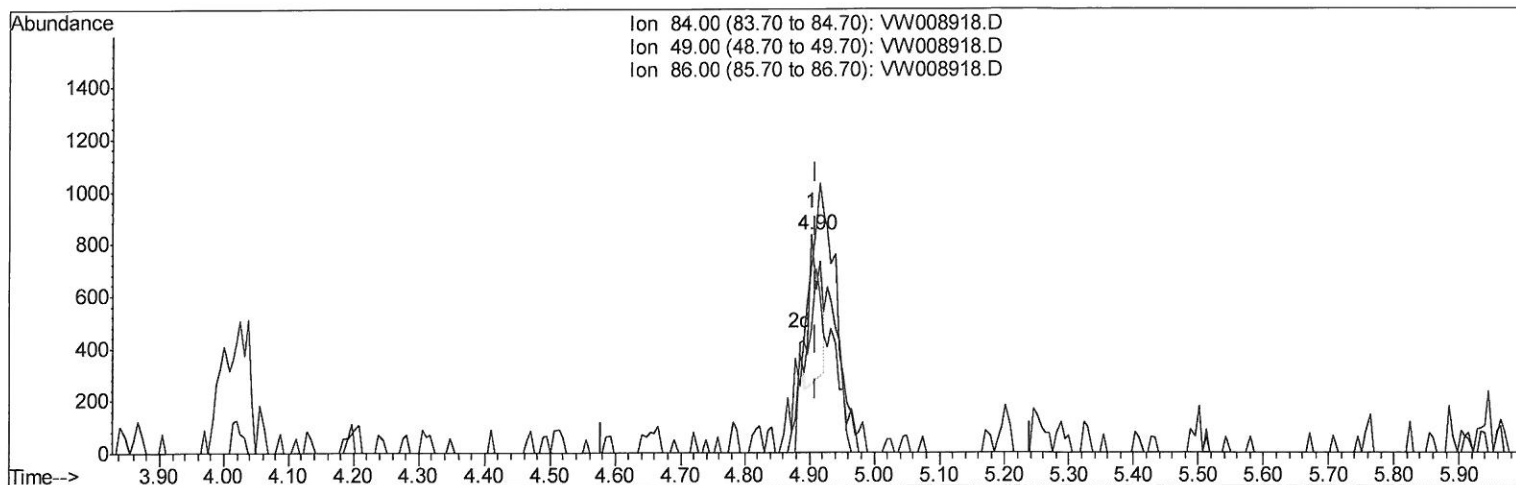

(16) Methylene chloride (T)

4.903min (-0.006) 0.60ug/L

response 651

Ion	Exp%	Act%
84.00	100	100
49.00	113.10	84.65
86.00	61.70	56.71
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008918.D
Acq On : 01 Mar 2019 13:02
Operator : SY/VA
Sample : K1657-01
Misc : 7.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB647

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:19 PM

Quant Time: Mar 02 02:58:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

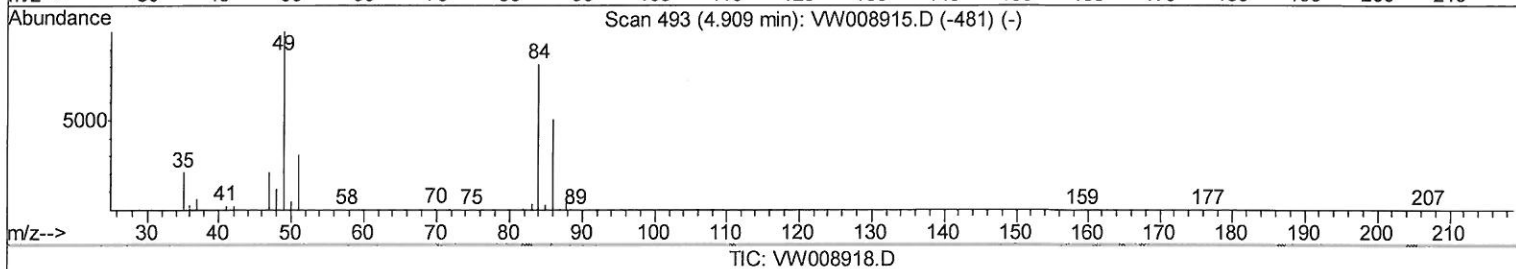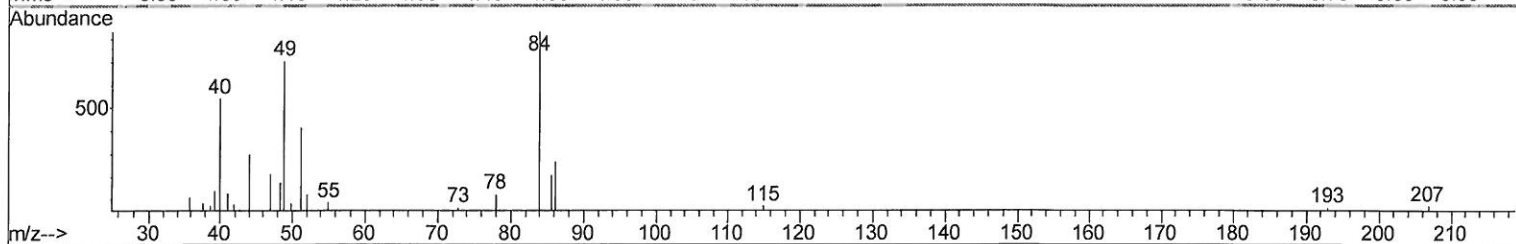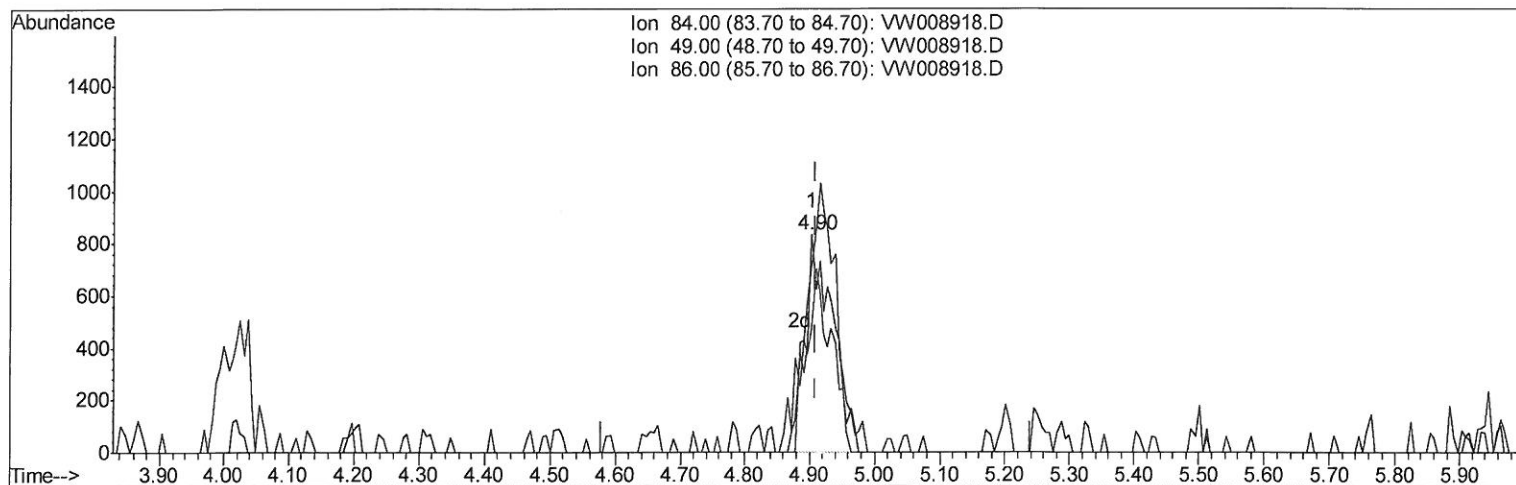

(16) Methylene chloride (T)

4.903min (-0.006) 2.26ug/L m

> 03/04/19 Sy

response 2472

Ion	Exp%	Act%
84.00	100	100
49.00	113.10	84.65
86.00	61.70	32.01#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008918.D
Acq On : 01 Mar 2019 13:02
Operator : SY/VA
Sample : K1657-01
Misc : 7.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB647

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:19 PM

Quant Time: Mar 02 02:58:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

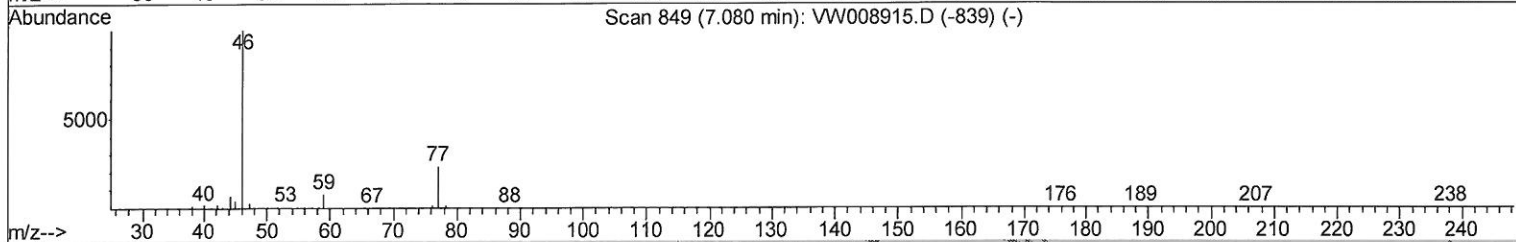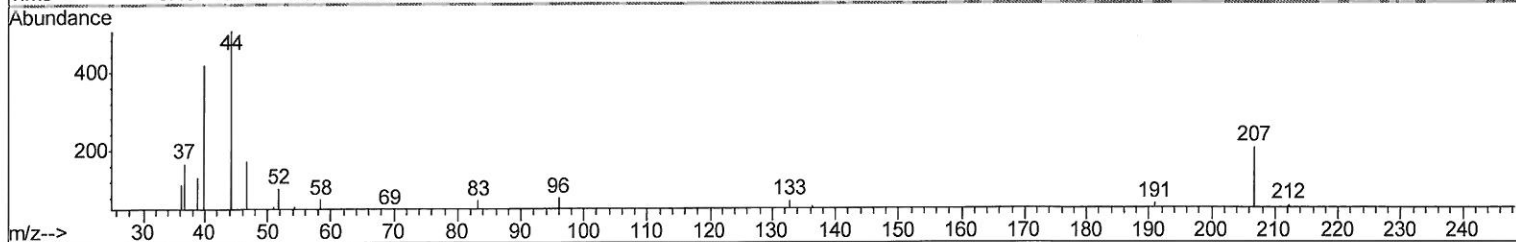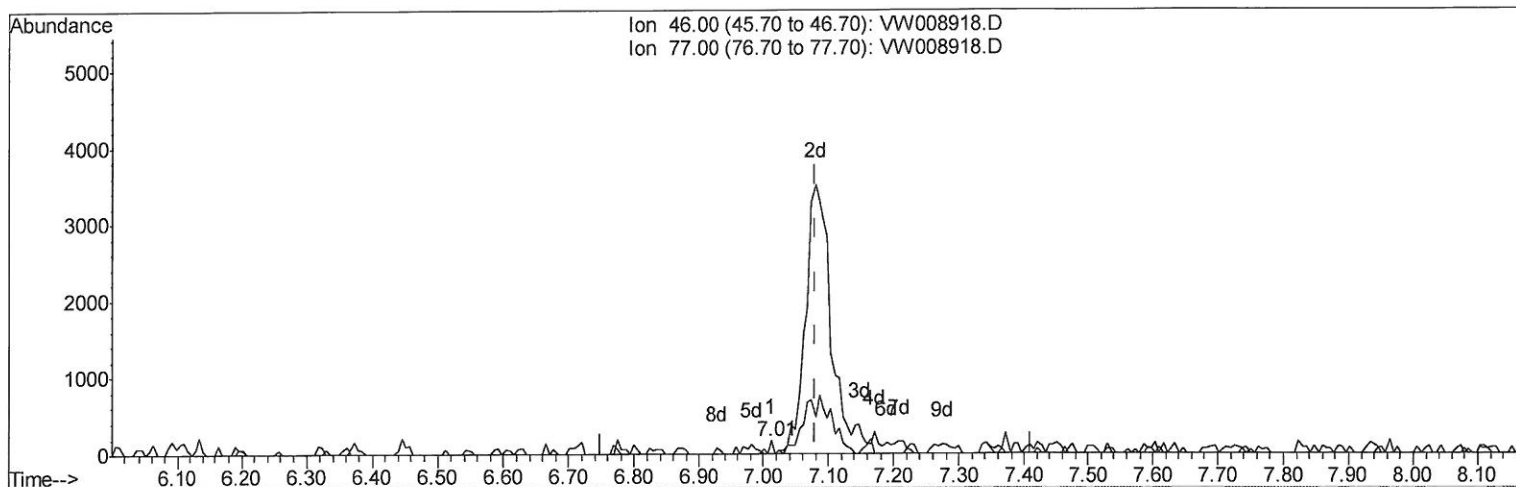

TIC: VW008918.D

(20) 2-Butanone-d5 (S)
7.013min (-0.067) 0.20ug/L
response 63

Ion	Exp%	Act%
46.00	100	100
77.00	26.90	30.16
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008918.D
Acq On : 01 Mar 2019 13:02
Operator : SY/VA
Sample : K1657-01
Misc : 7.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB647

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:19 PM

Quant Time: Mar 02 02:58:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

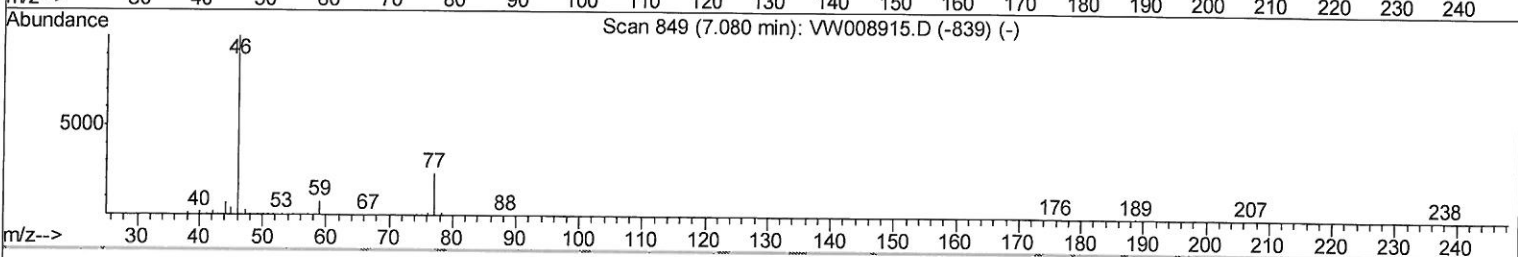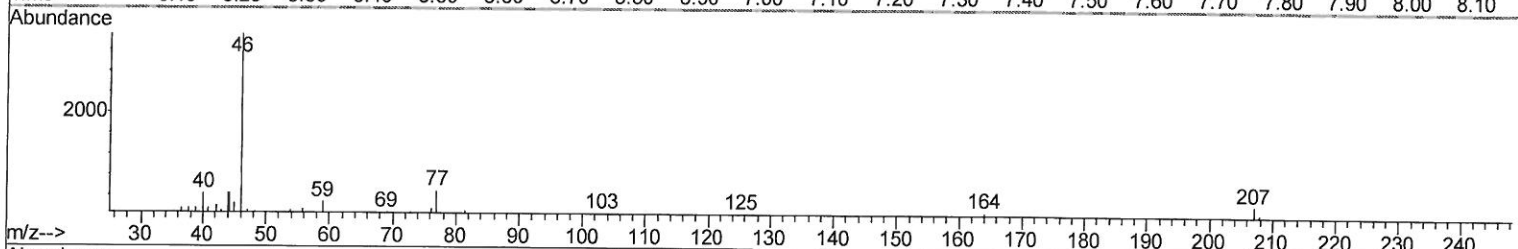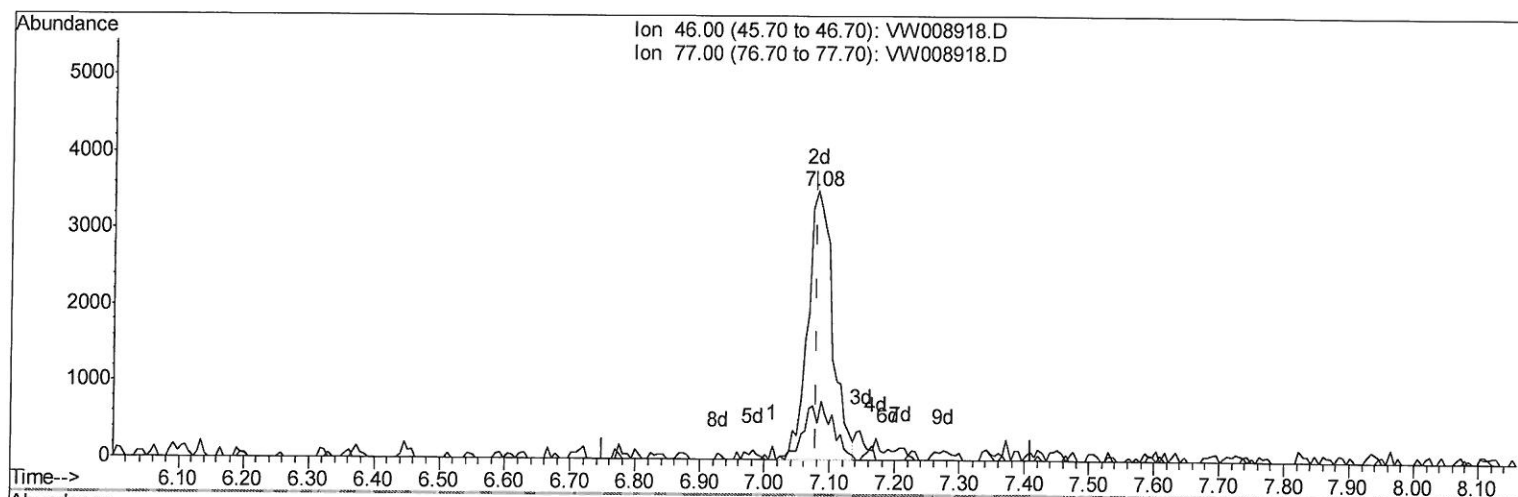

TIC: VW008918.D

(20) 2-Butanone-d5 (S)

7.080min (0.000) 29.82ug/L m

response 9358

Ion	Exp%	Act%
46.00	100	100
77.00	26.90	0.20#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030119\
Quantitation Report (LSC Reviewed)

Data File : VW008918.D
Acq On : 01 Mar 2019 13:02
Operator : SY/VA
Sample : K1657-01
Misc : 7.18G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB647

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:19 PM

Quant Time: Mar 04 17:25:59 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	67655	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	49204	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	12483	25.00	ug/L	0.00

System Monitoring Compounds						
4) Vinyl Chloride-d3	2.35	65	20773	19.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.96%
7) Chloroethane-d5	2.89	69	19646	20.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.16%
10) 1,1-Dichloroethene-d2	4.02	63	32421	18.52	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.08%
20) 2-Butanone-d5	7.08	46	9358m	29.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.64%
24) Chloroform-d	7.65	84	19030	11.63	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	46.52%
26) 1,2-Dichloroethane-d4	8.31	65	24223	25.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.36%
29) Benzene-d6	8.27	84	78609	33.28	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	133.12%
33) 1,2-Dichloropropane-d6	9.27	67	23253	33.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	134.40%#
37) Toluene-d8	10.32	98	62930	26.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.40%
38) trans-1,3-Dichloropropene-	10.58	79	7713	22.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.96%
39) 2-Hexanone-d5	10.93	63	5871	31.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.28%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	14347	20.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.60%
61) 1,2-Dichlorobenzene-d4	13.86	152	11368	25.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.20%

Target Compounds					Qvalue
16) Methylene chloride	4.90	84	2472m	2.260	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

03/04/19 Sy

03/04/19 Sy