

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (QT Reviewed)


Data File : VW008931.D
Acq On : 01 Mar 2019 18:34
Operator : SY/VA
Sample : K1662-03
Misc : 3.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BFC59

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:38 PM

Quant Time: Mar 02 03:54:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

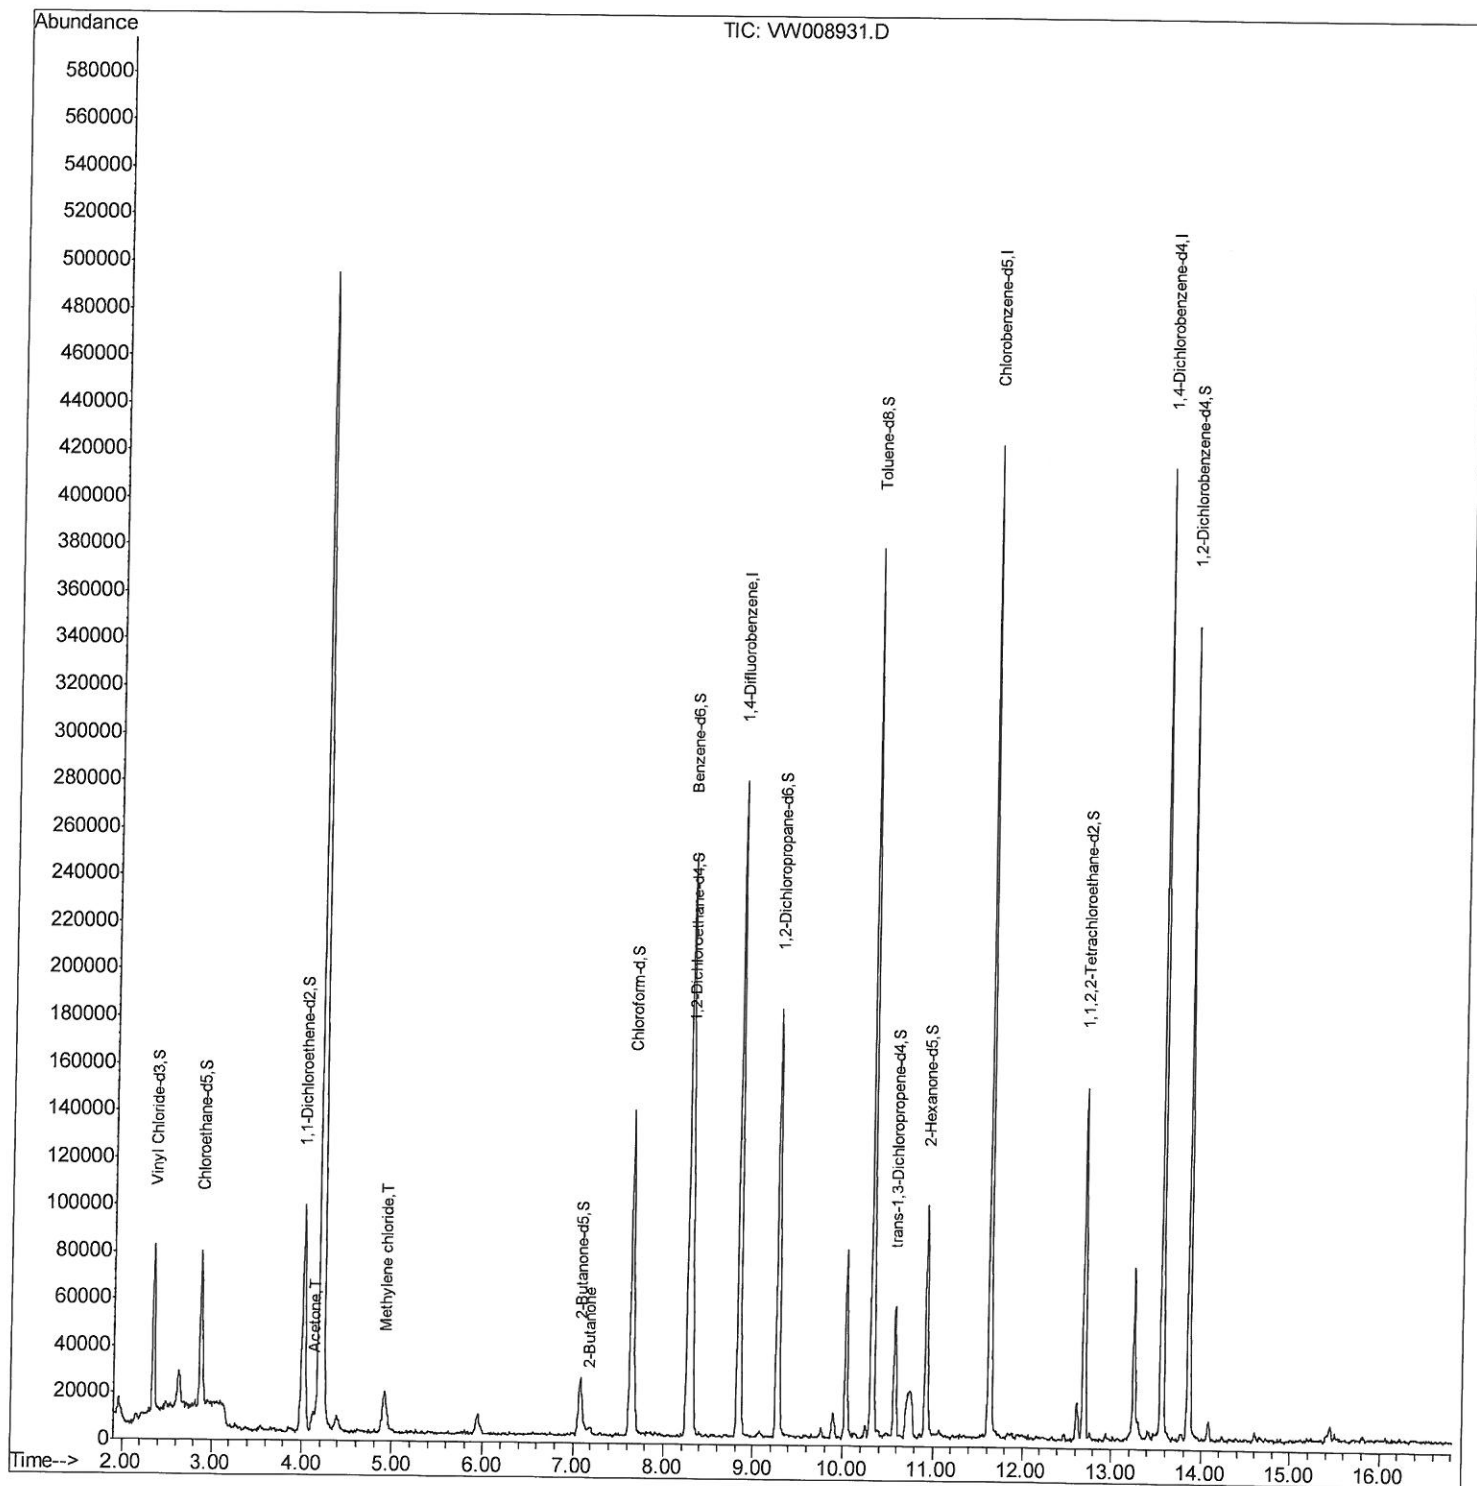

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008931.D
Acq On : 01 Mar 2019 18:34
Operator : SY/VA
Sample : K1662-03
Misc : 3.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFC59

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:38 PM

Quant Time: Mar 02 02:59:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

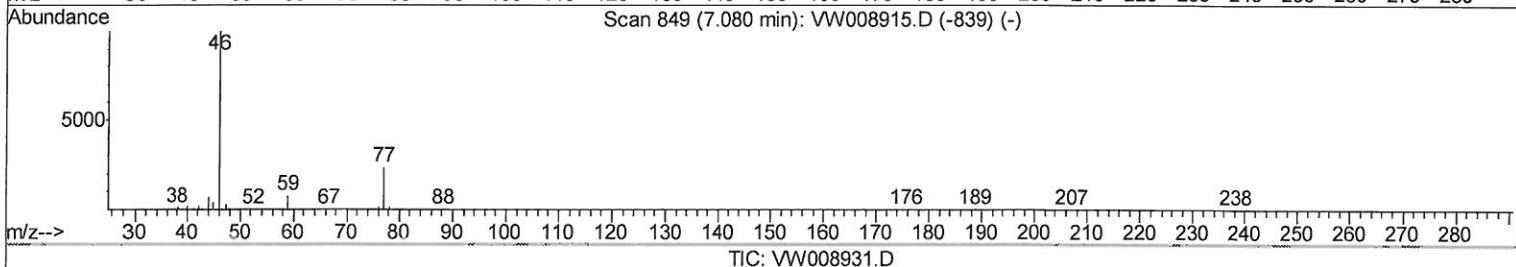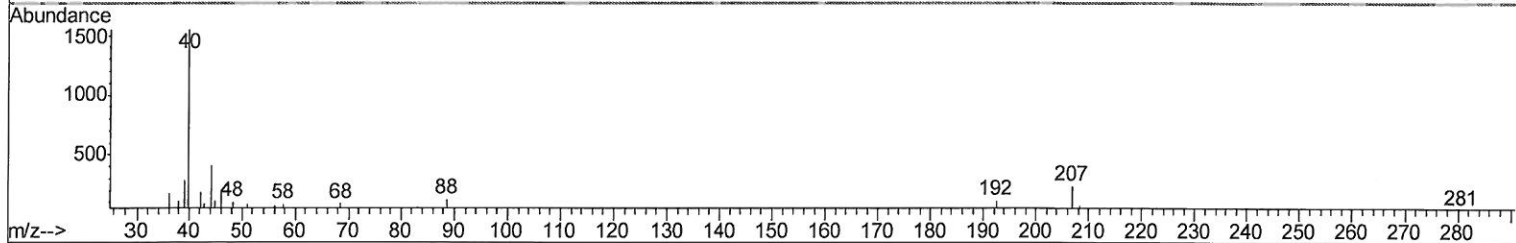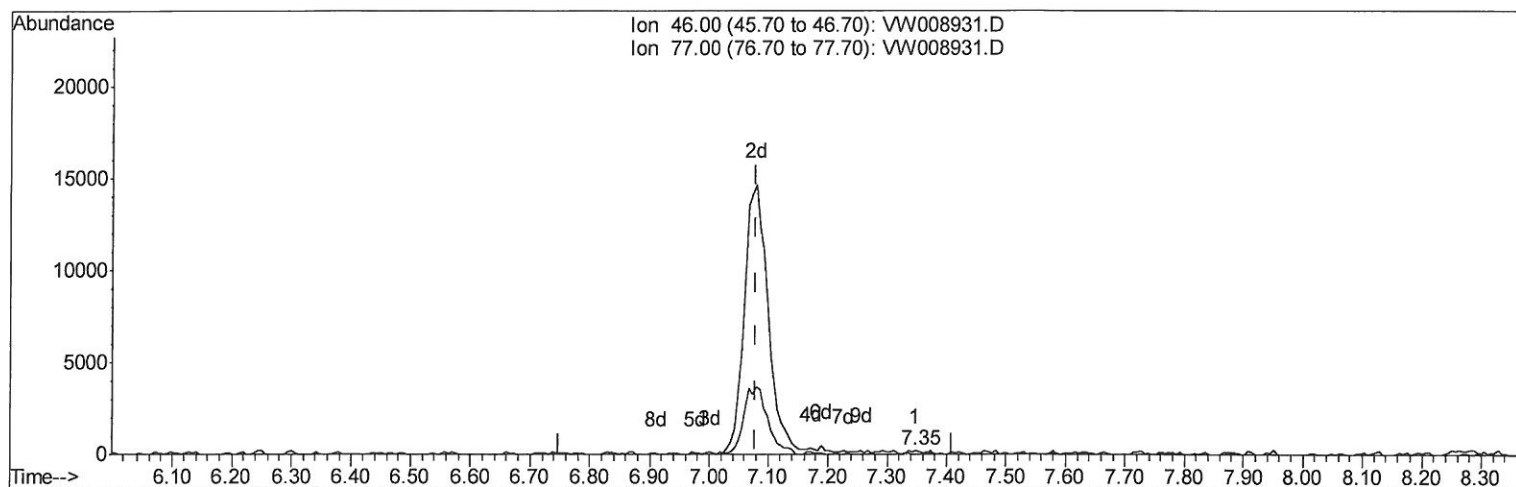

TIC: VW008931.D

(20) 2-Butanone-d5 (S)
7.348min (+0.268) 0.26ug/L

response 266

Ion	Exp%	Act%
46.00	100	100
77.00	26.90	20.30
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008931.D
Acq On : 01 Mar 2019 18:34
Operator : SY/VA
Sample : K1662-03
Misc : 3.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFC59

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:38 PM

Quant Time: Mar 02 02:59:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

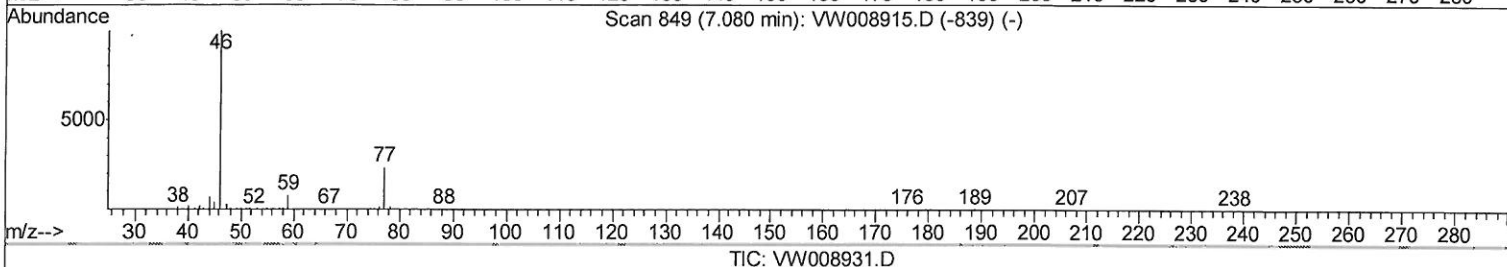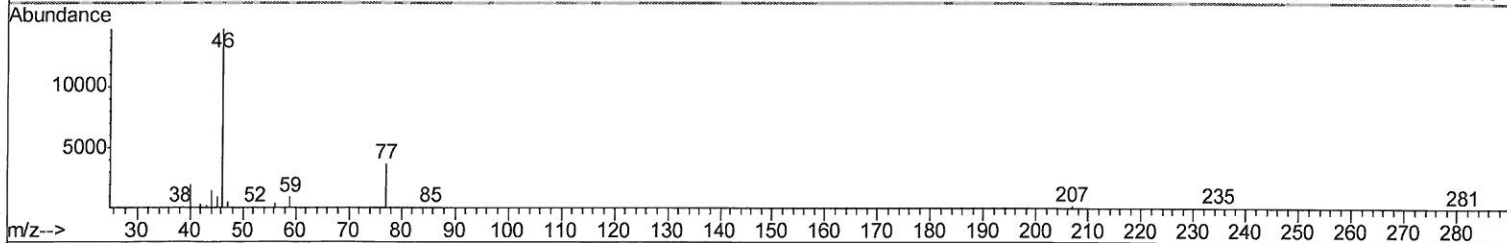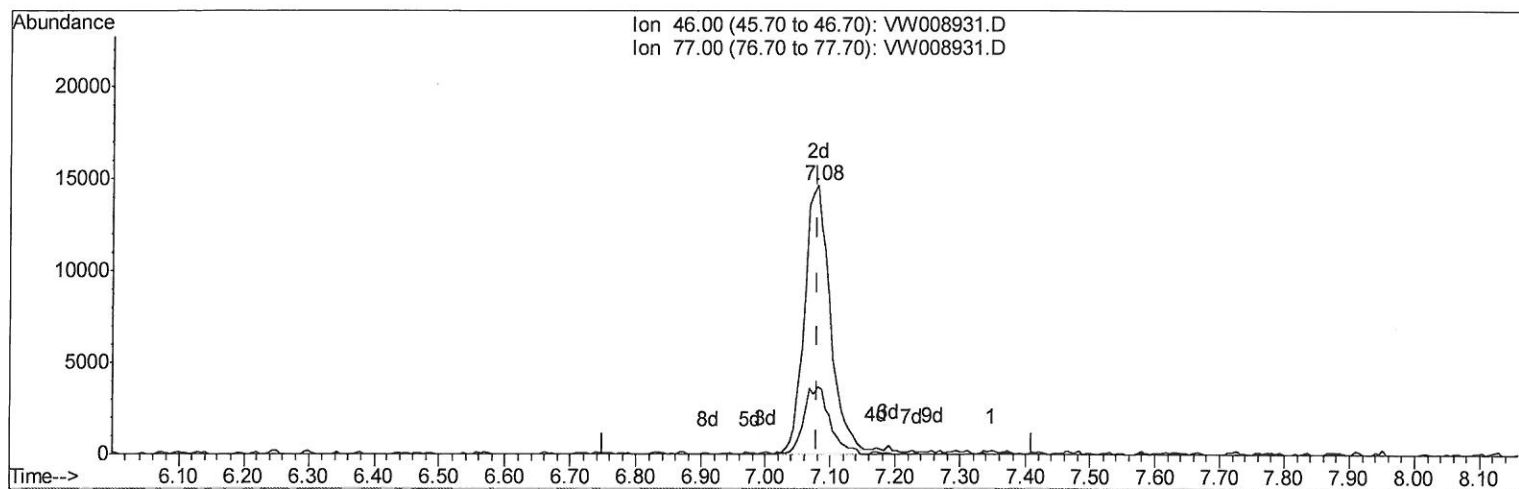

(20) 2-Butanone-d5 (S)

7.080min (+0.000) 39.43ug/L m

response 40818

Ion	Exp%	Act%
46.00	100	100
77.00	26.90	0.13#
0.00	0.00	0.00
0.00	0.00	0.00

203/04/19 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008931.D
Acq On : 01 Mar 2019 18:34
Operator : SY/VA
Sample : K1662-03
Misc : 3.92G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFC59

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:38 PM

Quant Time: Mar 02 02:59:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

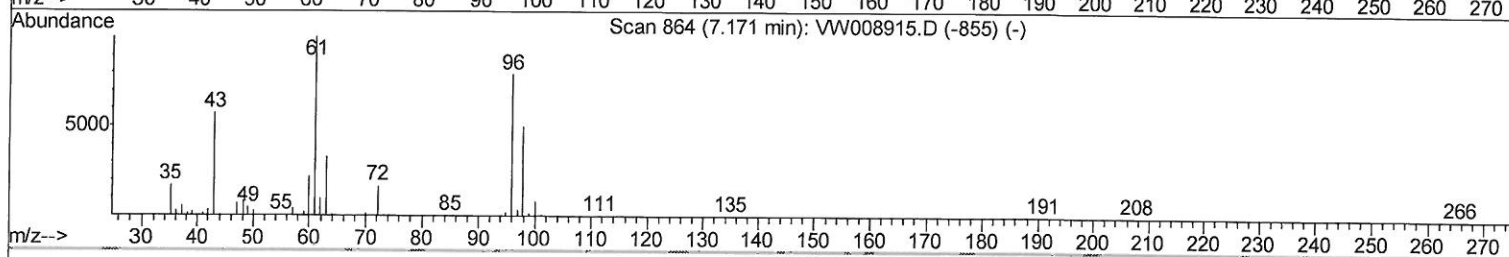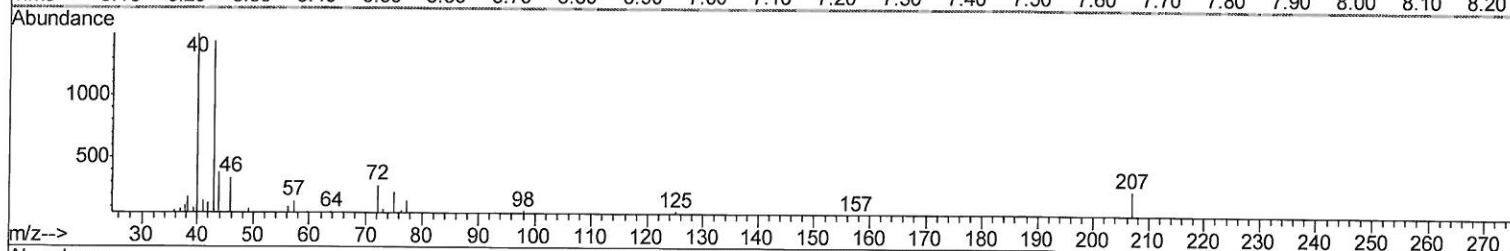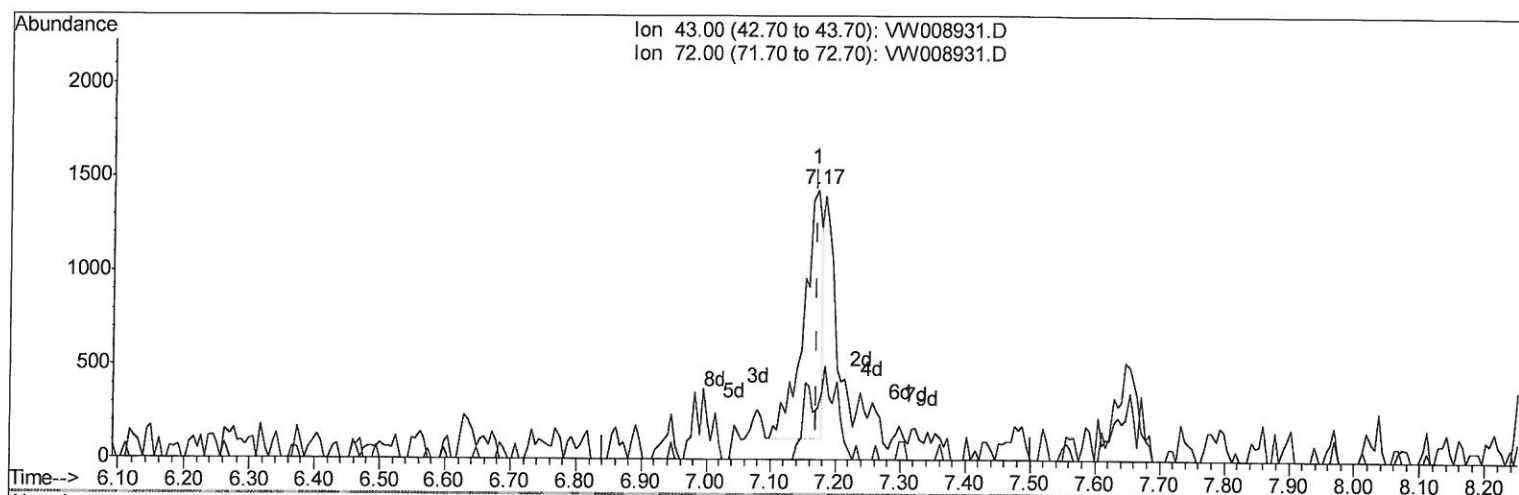

TIC: VW008931.D

(21) 2-Butanone

7.171min (+0.000) 1.93ug/L

response 2652

Ion	Exp%	Act%
43.00	100	100
72.00	28.90	24.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (Qedit)




Data File : VW008931.D
Acq On : 01 Mar 2019 18:34
Operator : SY/VA
Sample : K1662-03
Misc : 3.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BFC59

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:38 PM

Quant Time: Mar 02 02:59:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

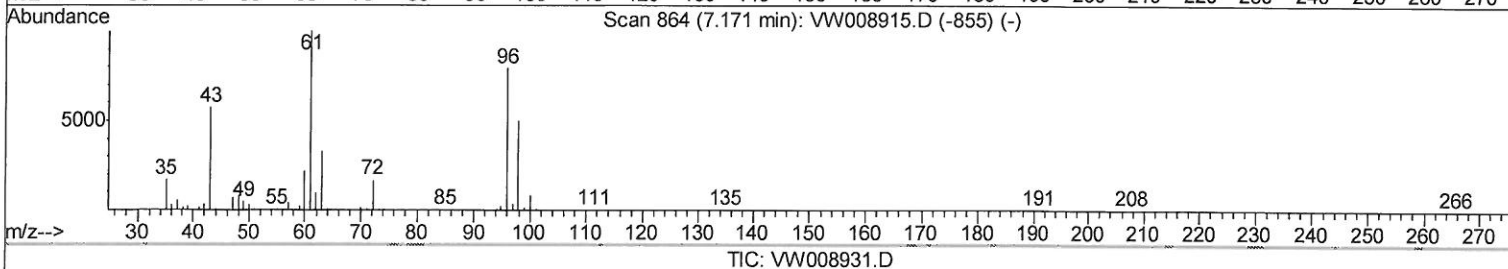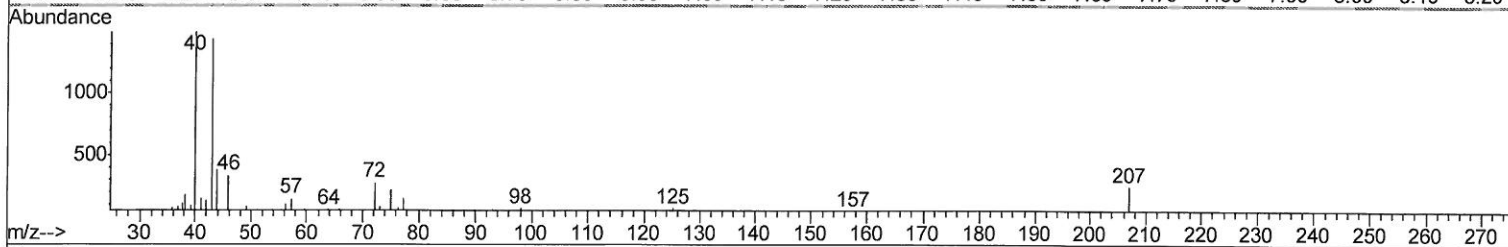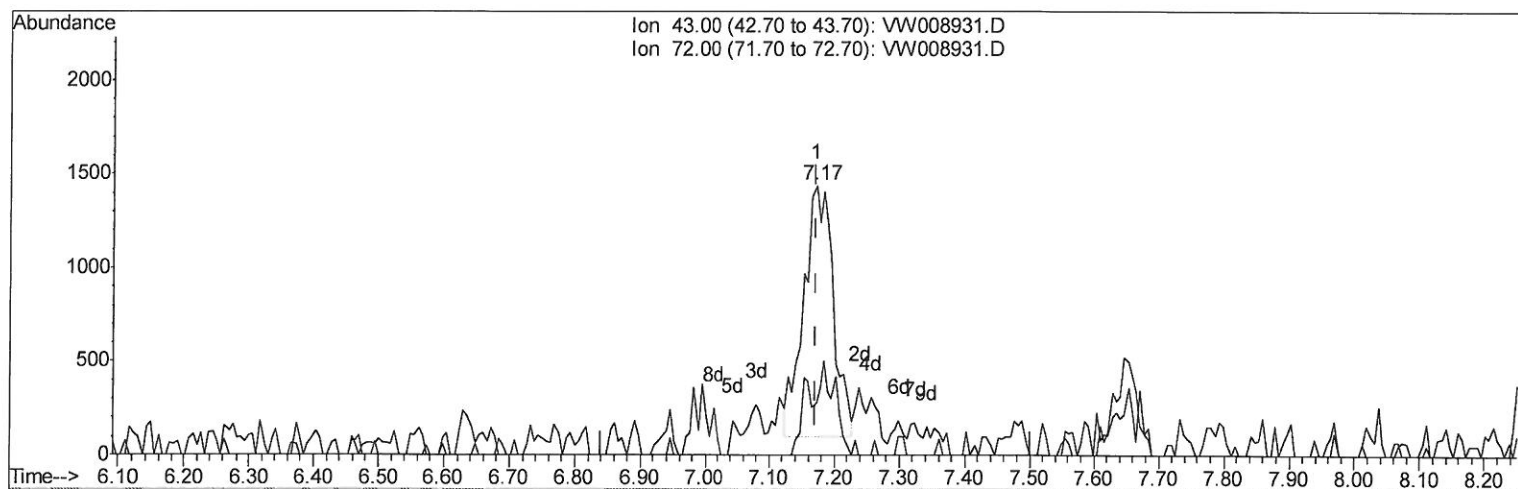

(21) 2-Butanone

7.171min (+0.000) 3.09ug/L m

response 4246

Ion	Exp%	Act%
43.00	100	100
72.00	28.90	15.24
0.00	0.00	0.00
0.00	0.00	0.00

03/04/19 Sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW030119\
Quantitation Report (QT Reviewed)

Data File : VW008931.D
Acq On : 01 Mar 2019 18:34
Operator : SY/VA
Sample : K1662-03
Misc : 3.92G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFC59

Manual Integrations
APPROVED

MMDadoda
3/5/2019 11:47:38 PM

Quant Time: Mar 02 03:54:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM022019S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 02 02:55:16 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	223149	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	224103	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	106249	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	61511	17.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.88%
7) Chloroethane-d5	2.89	69	64053	20.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.20%
10) 1,1-Dichloroethene-d2	4.01	63	87425	15.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.56%
20) 2-Butanone-d5	7.08	46	40818m	39.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.86%
24) Chloroform-d	7.65	84	122349	22.67	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.68%
26) 1,2-Dichloroethane-d4	8.31	65	79012	24.81	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.24%
29) Benzene-d6	8.27	84	244681	22.74	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.96%
33) 1,2-Dichloropropane-d6	9.27	67	75541	23.97	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.88%
37) Toluene-d8	10.32	98	241477	22.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.64%
38) trans-1,3-Dichloropropene-	10.57	79	29043	18.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.56%
39) 2-Hexanone-d5	10.93	63	29483	34.34	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.68%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	67741	21.41	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.64%
61) 1,2-Dichlorobenzene-d4	13.86	152	88852	23.47	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.88%

Target Compounds

					Qvalue
13) Acetone	4.12	43	14942	15.215	ug/L 97
16) Methylene chloride	4.92	84	11917	3.303	ug/L # 73
21) 2-Butanone	7.17	43	4246m	3.090	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

03/04/19 SC

03/04/19 SC