

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
 Data File : VW022156.D
 Acq On : 03 Mar 2022 09:42
 Operator : SY/VA
 Sample : VW0303SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 04 00:32:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 04 00:31:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	161758	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	152517	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	76002	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	41471	19.656	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.640%
7) Chloroethane-d5	2.879	69	31536	18.997	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.000%
11) 1,1-Dichloroethene-d2	4.013	63	46777	14.478	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.920%
21) 2-Butanone-d5	7.092	46	15319	43.184	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.360%
24) Chloroform-d	7.647	84	77660	21.518	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.080%
26) 1,2-Dichloroethane-d4	8.305	65	41145	21.932	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.720%
32) Benzene-d6	8.275	84	145181	20.453	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.800%
36) 1,2-Dichloropropane-d6	9.274	67	42622	21.622	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.480%
41) Toluene-d8	10.323	98	134960	19.125	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.480%
43) trans-1,3-Dichloroprop...	10.579	79	16772	19.190	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.760%
47) 2-Hexanone-d5	10.927	63	13677	42.186	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.380%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	37436	21.640	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	51970	21.289	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.160%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	4488	2.126	ug/L #	4
37) 1,2-Dichloropropane	9.274	63	5156	2.997	ug/L #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030322\
Data File : VW022156.D
Acq On : 03 Mar 2022 09:42
Operator : SY/VA
Sample : VW0303SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Mar 04 00:32:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 04 00:31:34 2022
Response via : Initial Calibration

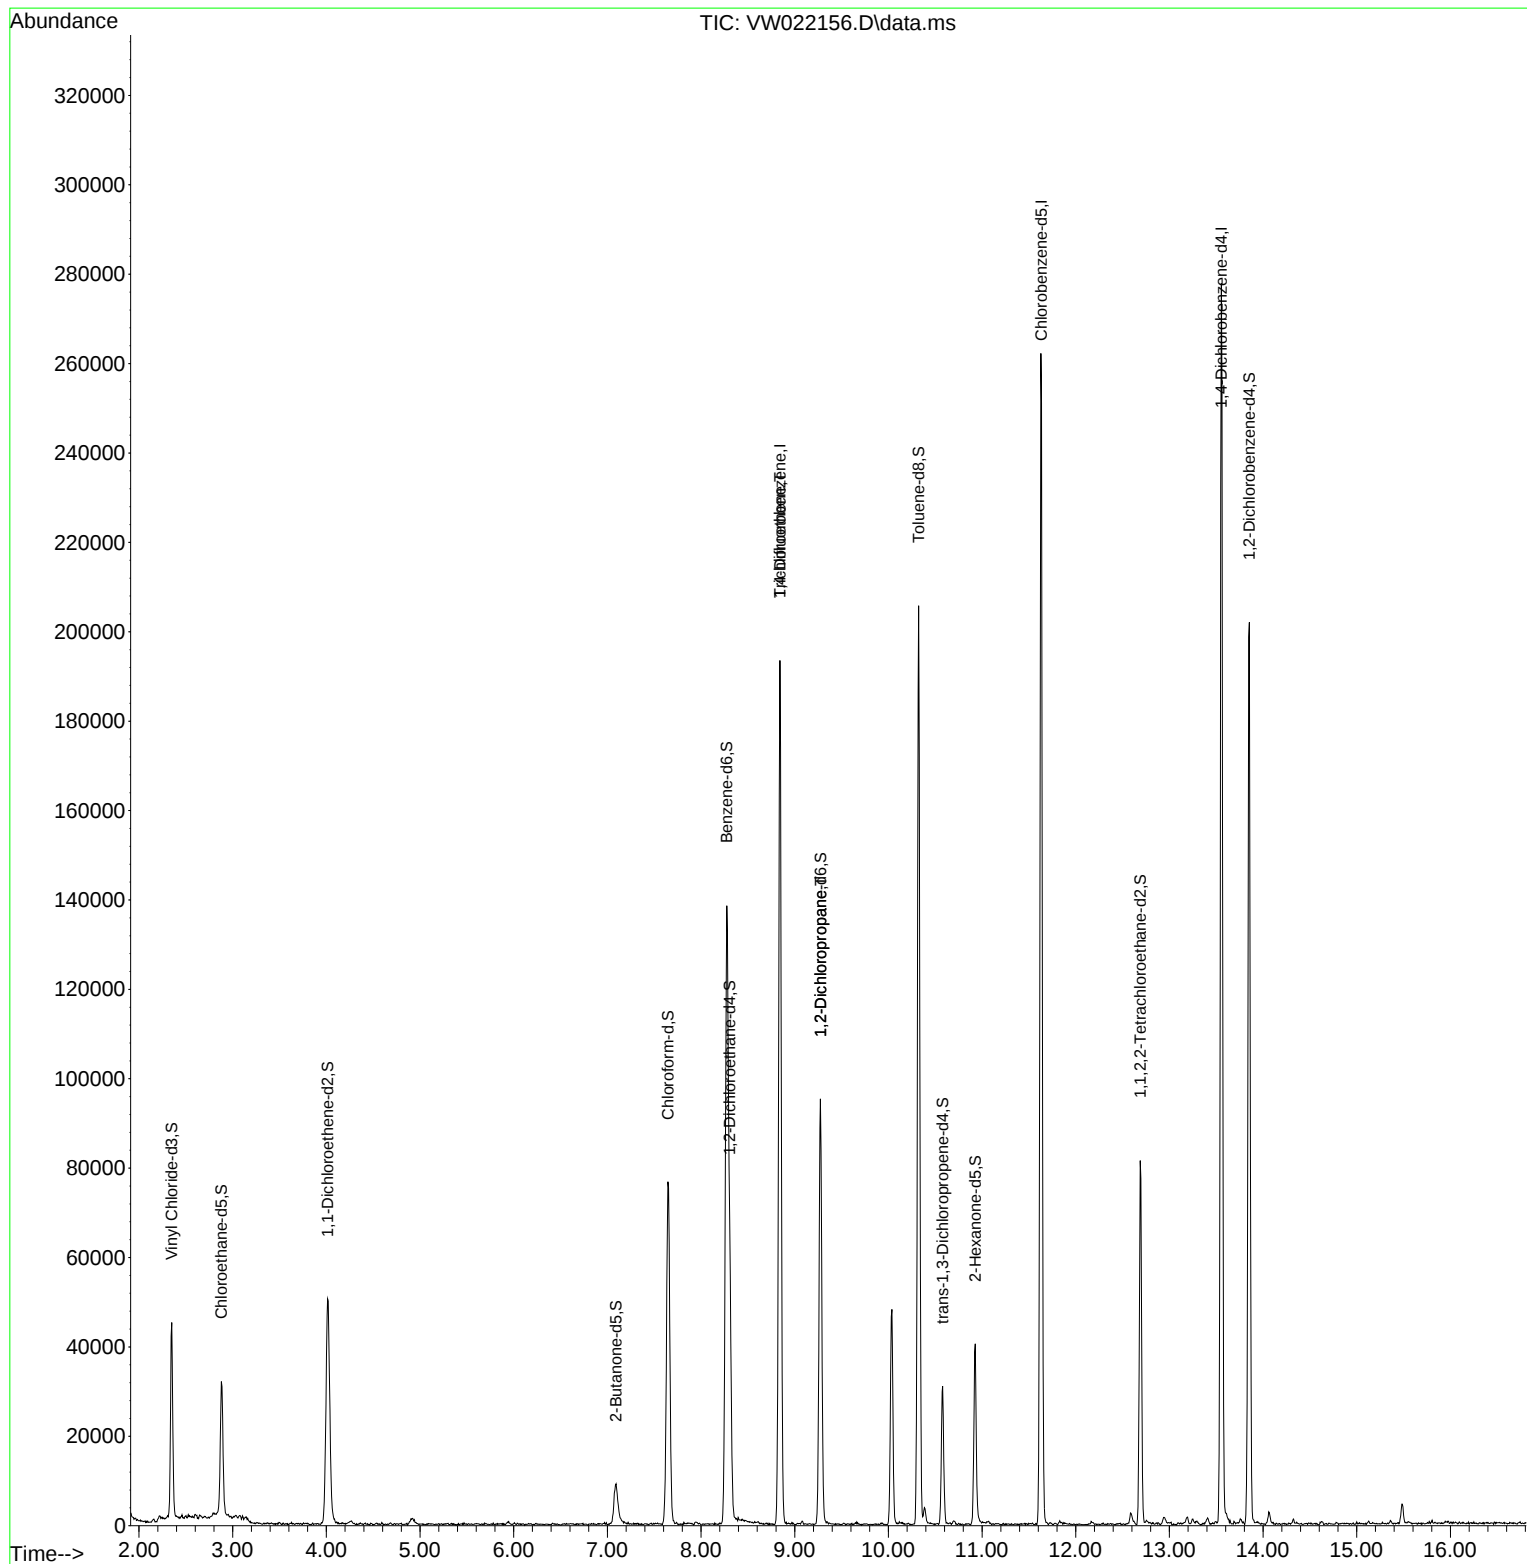

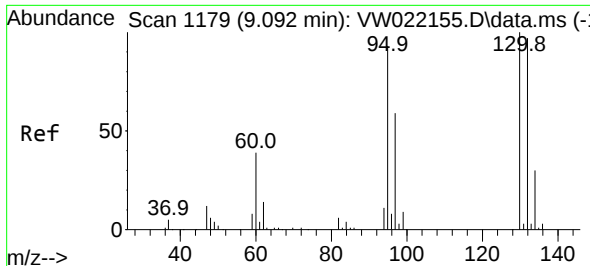




#34
 Trichloroethene
 Concen: 2.126 ug/L
 RT: 8.842 min Scan# 1179
 Delta R.T. -0.250 min
 Lab File: VW022156.D
 Acq: 03 Mar 2022 09:42

Instrument :
 MSVOA_W
 ClientSampleId :

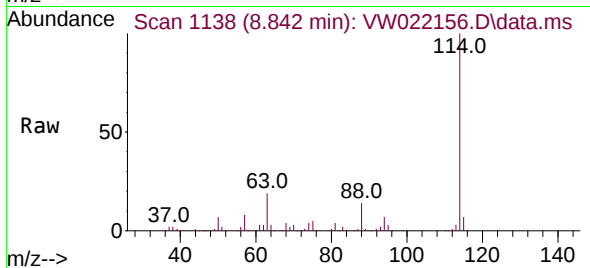

Tgt Ion: 95 Resp: 4488

Ion	Ratio	Lower	Upper
95	100		
97	0.0	44.4	82.4#
132	0.0	71.7	133.1#
130	0.0	71.7	133.1#

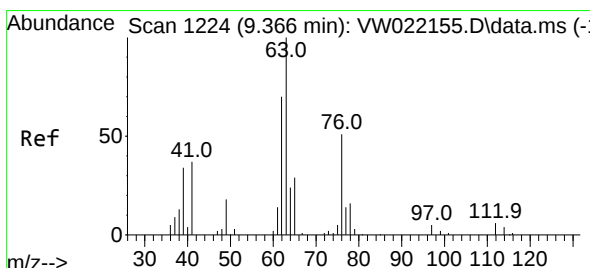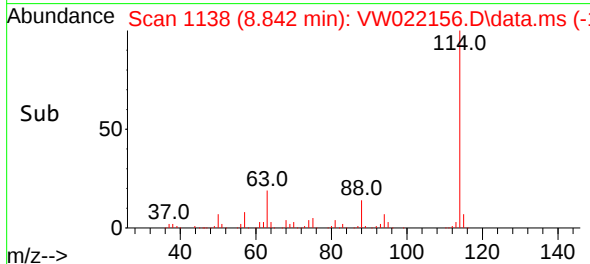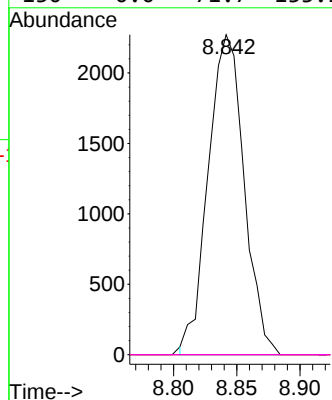

#37
 1,2-Dichloropropane
 Concen: 2.997 ug/L
 RT: 9.274 min Scan# 1209
 Delta R.T. -0.091 min
 Lab File: VW022156.D
 Acq: 03 Mar 2022 09:42

Tgt Ion: 63 Resp: 5156

Ion	Ratio	Lower	Upper
63	100		
112	1.3	4.1	6.1#

